

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 17:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 17:47:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 17:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	135.9E6	292.7E6	97.464	100.359
28)	SA Decachlor...	9.110	7.933	189.2E6	263.2E6	96.955	97.931
Target Compounds							
23)	Chlordane-1	4.733	3.794	71810394	98306464	981.496	990.611
24)	Chlordane-2	5.263	4.370	74043782	110.8E6	972.541	970.668
25)	Chlordane-3	5.974	5.000	313.0E6	330.8E6	1018.063	998.752
26)	Chlordane-4	6.057	5.063	371.6E6	318.3E6	1014.544	1011.096
27)	Chlordane-5	6.908	5.957	67710328	119.1E6	997.874	995.071



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 17:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 17:47:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 17:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

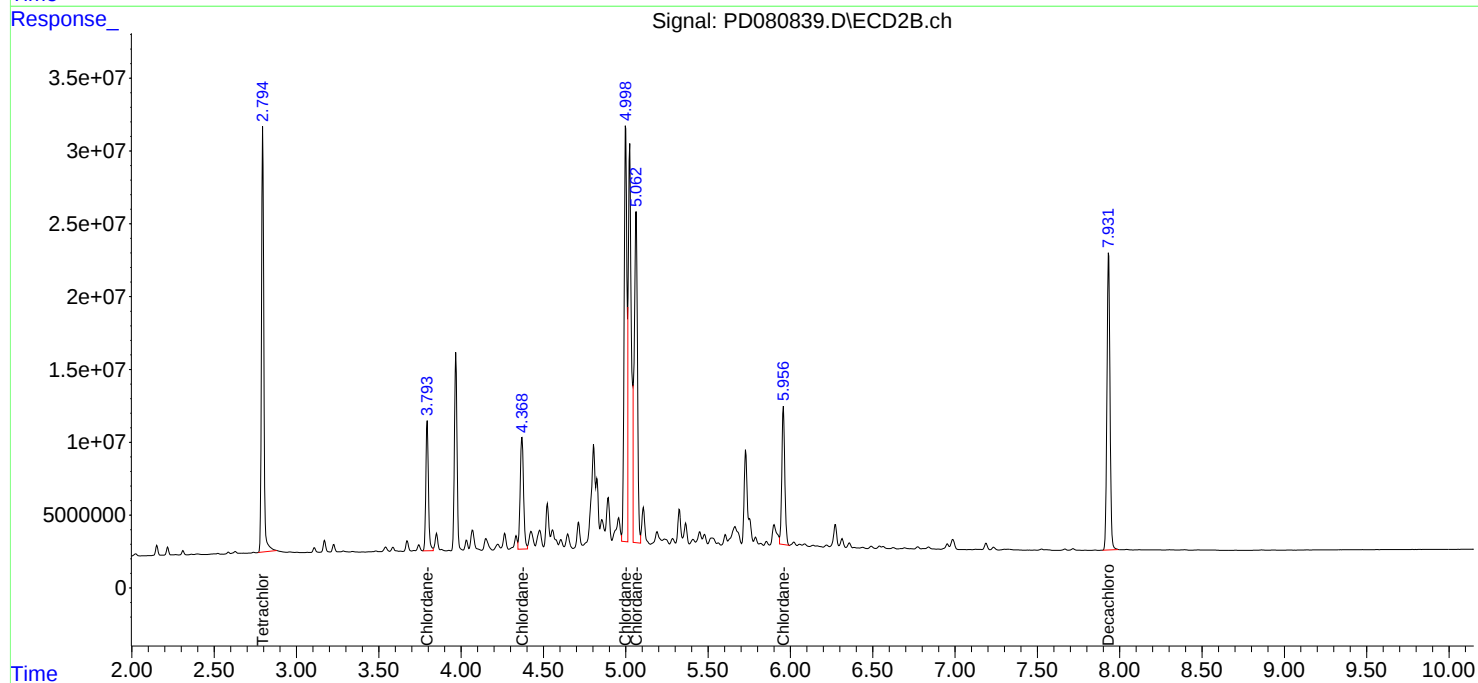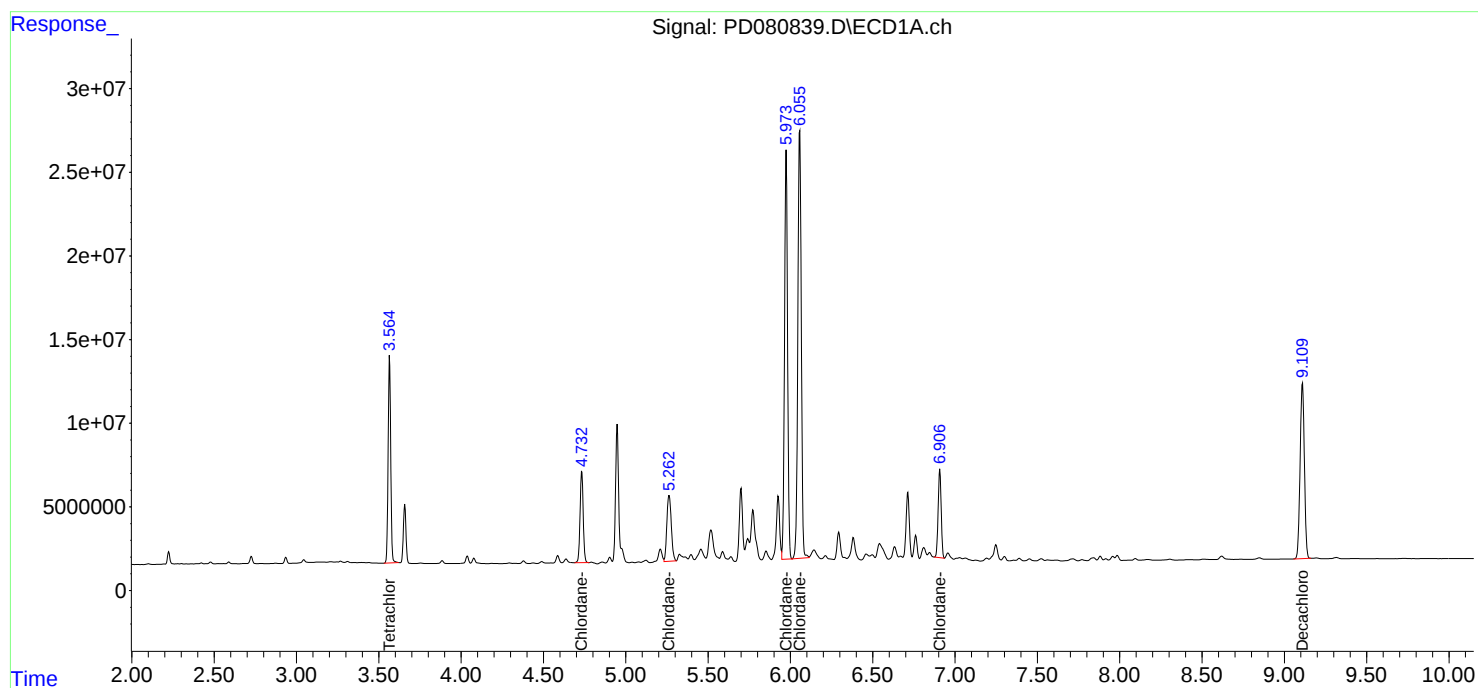


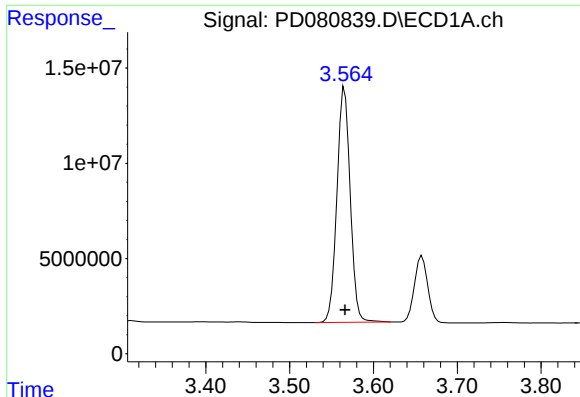

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 135888228
Conc: 97.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

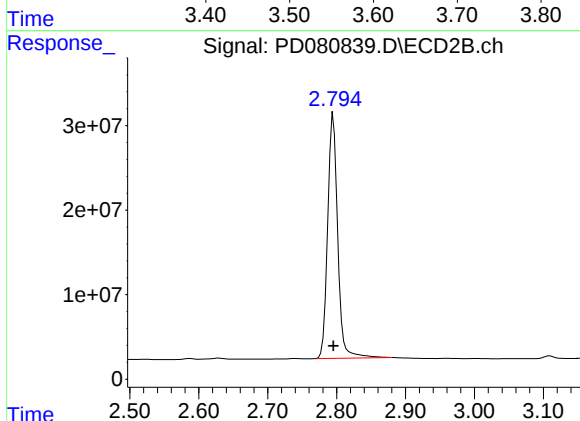


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 292744873
Conc: 100.36 ng/ml

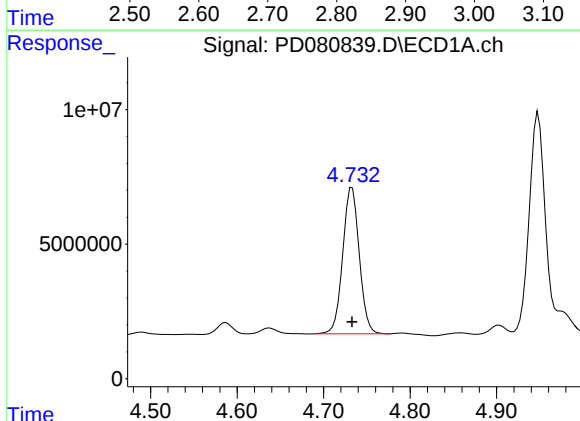


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 71810394
Conc: 981.50 ng/ml

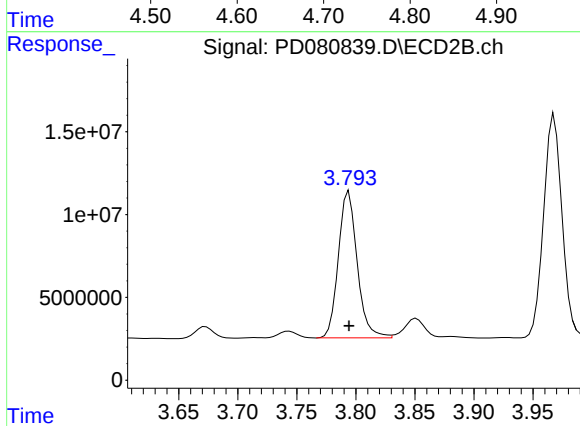

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 98306464
Conc: 990.61 ng/ml

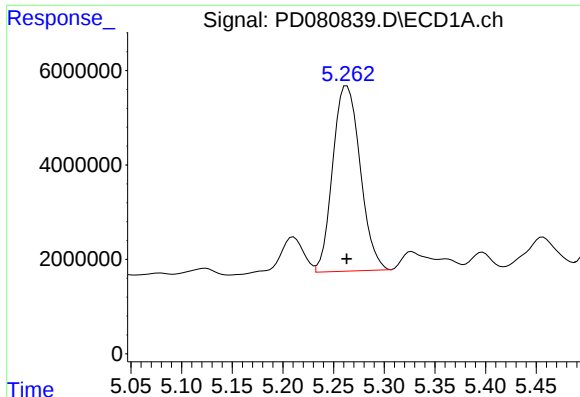

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 74043782
Conc: 972.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

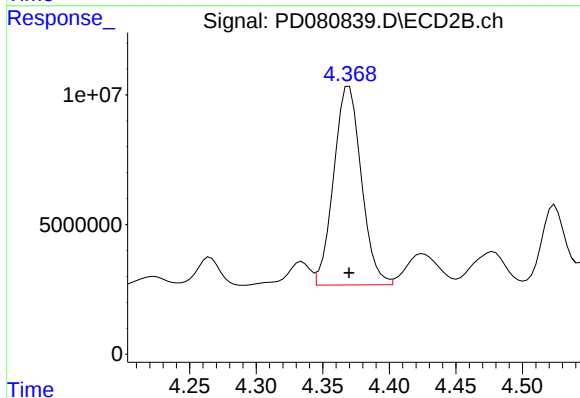


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 110842810
Conc: 970.67 ng/ml

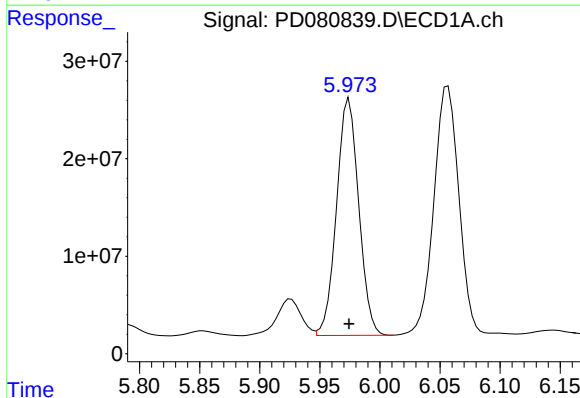


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 312994298
Conc: 1018.06 ng/ml

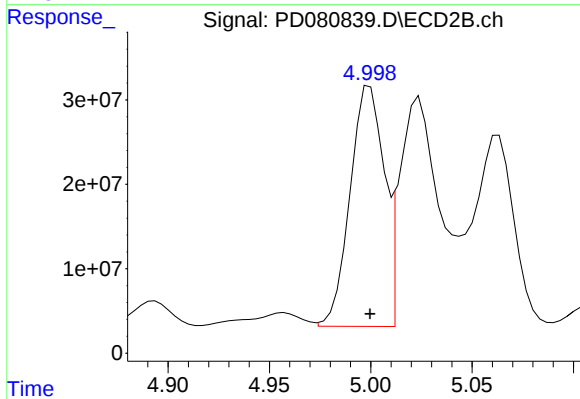

#25 Chlordane-3


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 330812128
Conc: 998.75 ng/ml

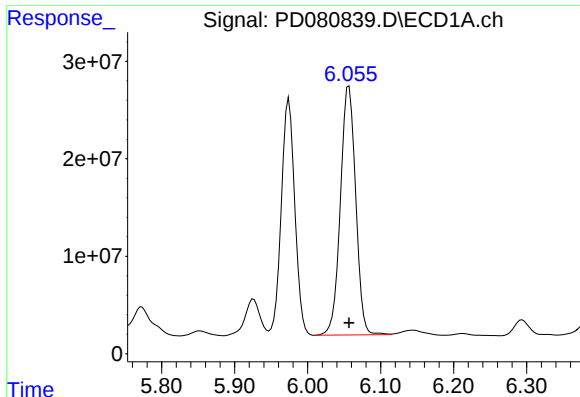

#26 Chlordane-4


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 371638300
Conc: 1014.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

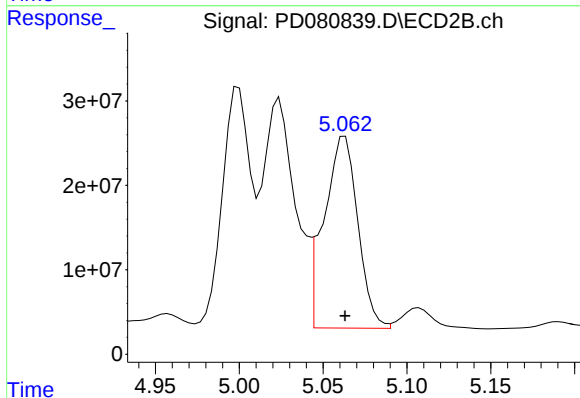


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 318303683
Conc: 1011.10 ng/ml

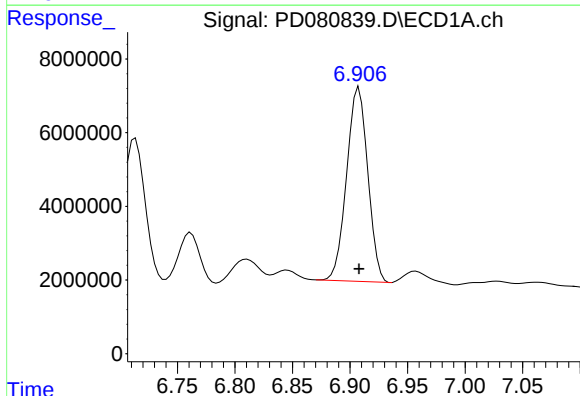


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 67710328
Conc: 997.87 ng/ml

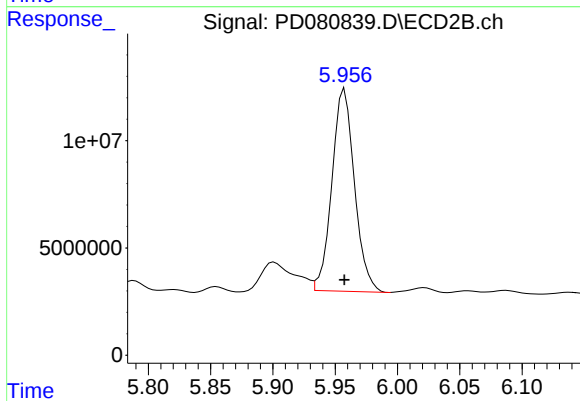

#27 Chlordane-5


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 119124890
Conc: 995.07 ng/ml

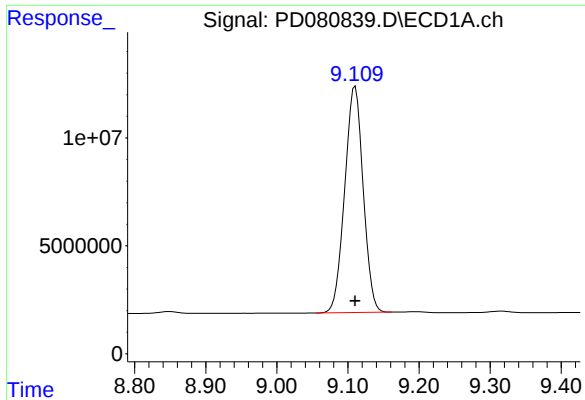

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 189180278
Conc: 96.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

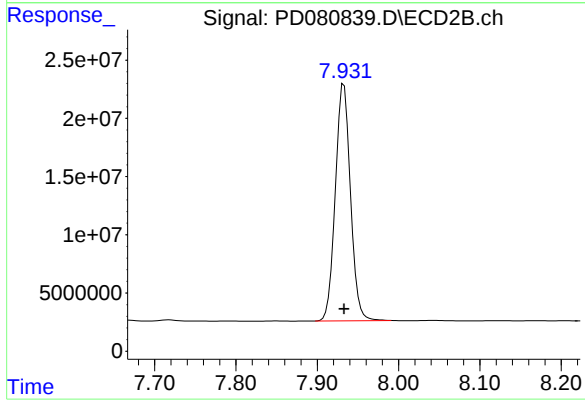

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 263227162
Conc: 97.93 ng/ml