

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 17:19
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 17:49:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 17:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	105.0E6	215.8E6	75.201	74.324
28)	SA Decachlor...	9.110	7.934	143.7E6	198.7E6	74.088	74.278
Target Compounds							
23)	Chlordane-1	4.733	3.794	55453723	73486523	755.272	743.644
24)	Chlordane-2	5.263	4.370	56315647	84121306	743.094	741.056
25)	Chlordane-3	5.975	5.000	228.6E6	249.3E6	745.595	751.715
26)	Chlordane-4	6.057	5.063	272.2E6	232.7E6	745.295	742.741
27)	Chlordane-5	6.909	5.958	49867568	88896915	739.877	745.031



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 17:19
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 17:49:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 17:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

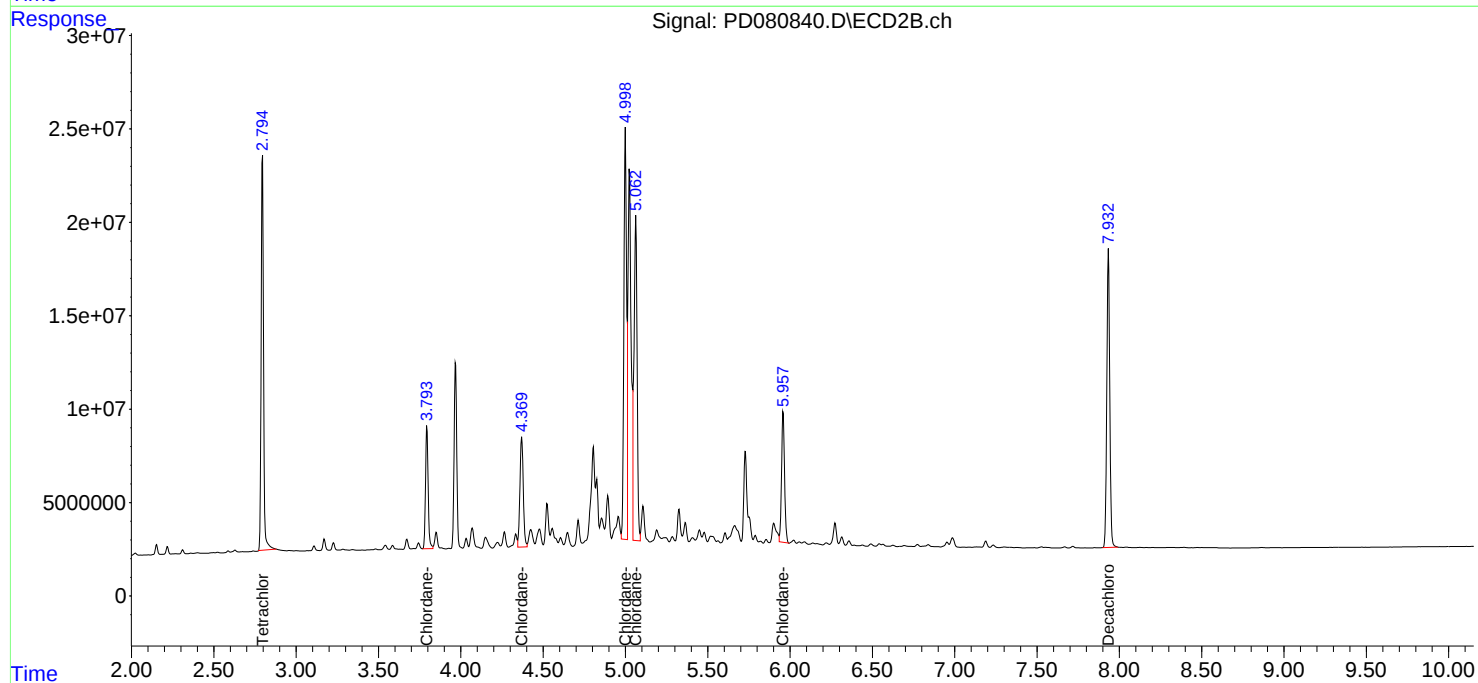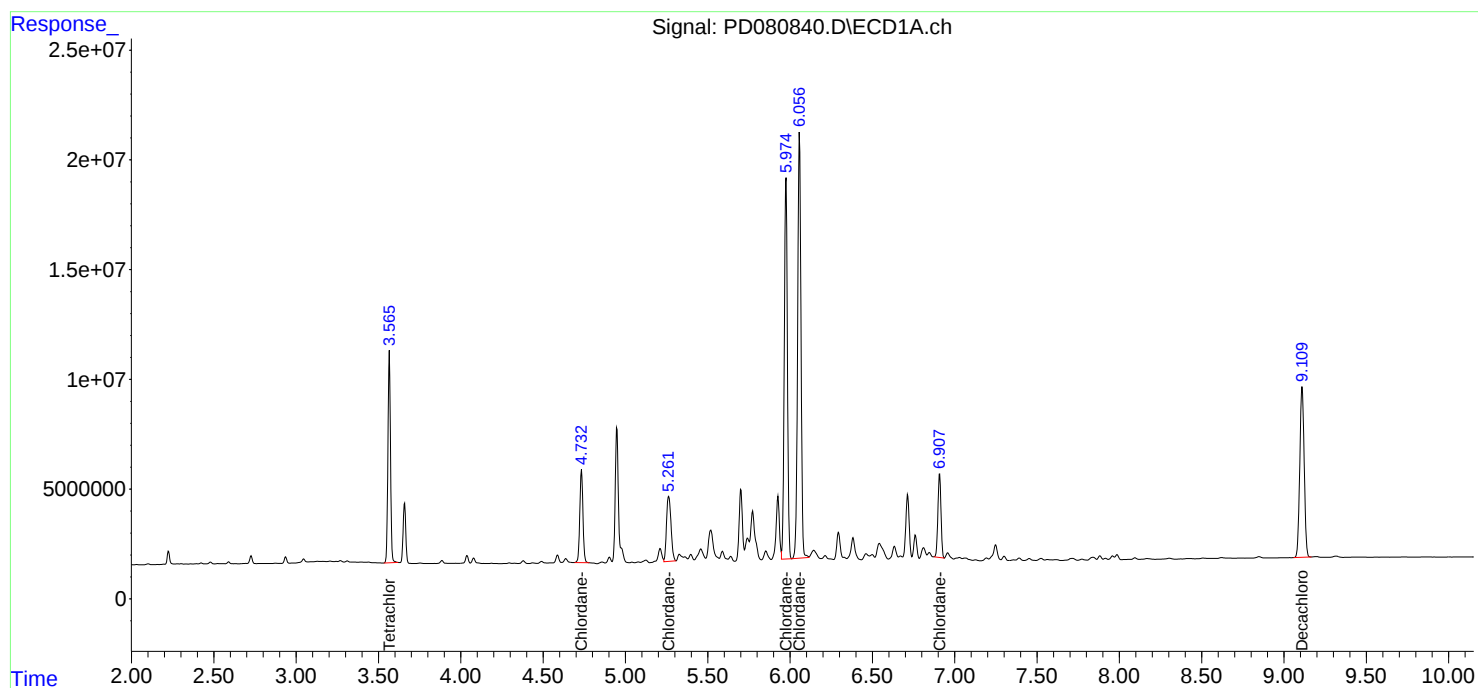


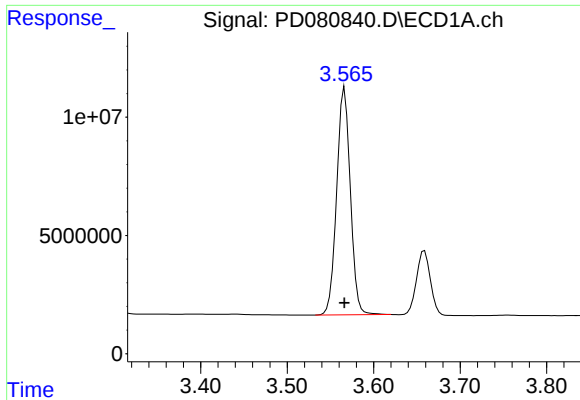

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 104990229
Conc: 75.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

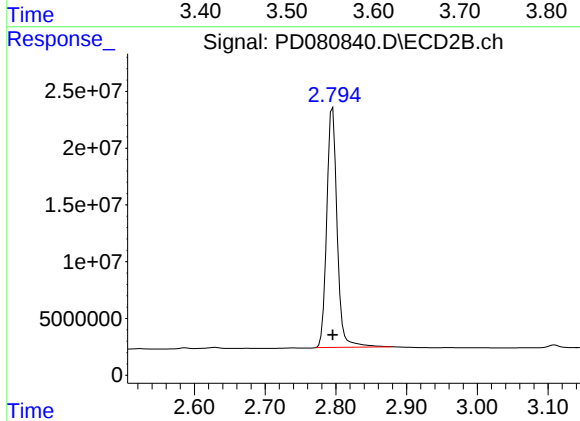


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 215827317
Conc: 74.32 ng/ml

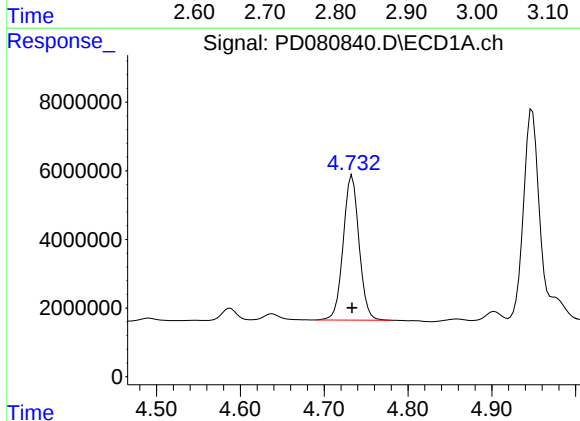


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 55453723
Conc: 755.27 ng/ml

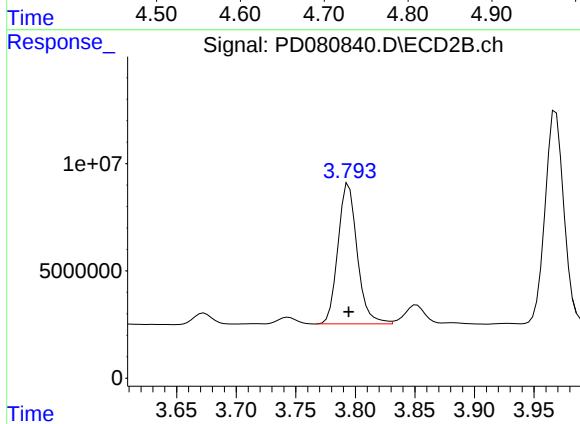

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 73486523
Conc: 743.64 ng/ml

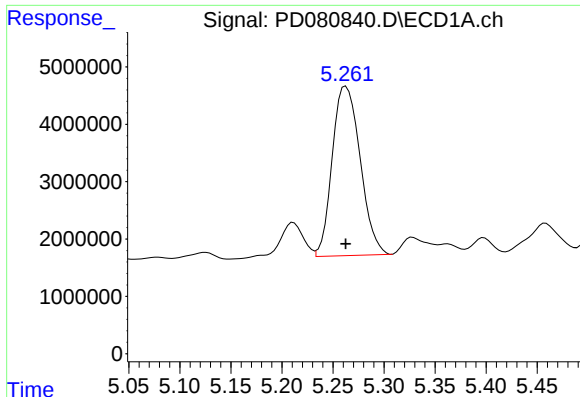

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 56315647
Conc: 743.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

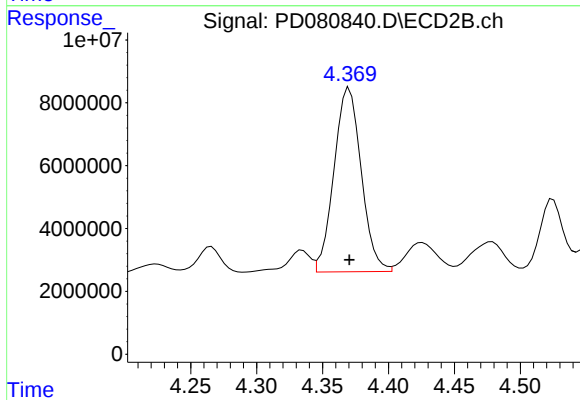


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 84121306
Conc: 741.06 ng/ml

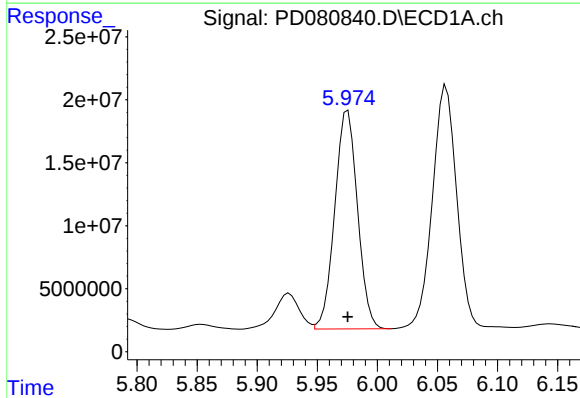


#25 Chlordane-3

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 228555159
Conc: 745.59 ng/ml

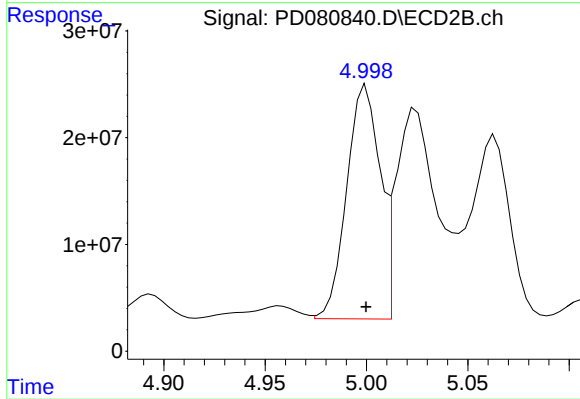

#25 Chlordane-3


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 249272090
Conc: 751.71 ng/ml

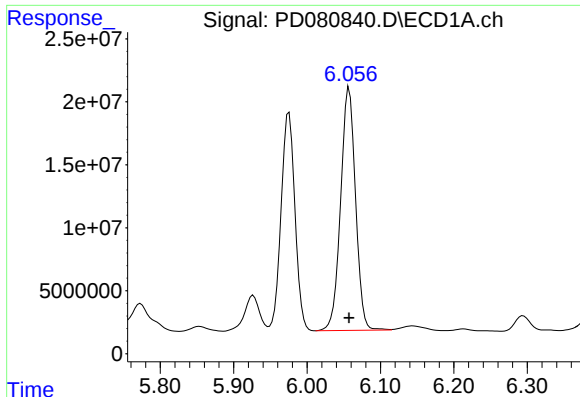

#26 Chlordane-4


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 272155986
Conc: 745.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

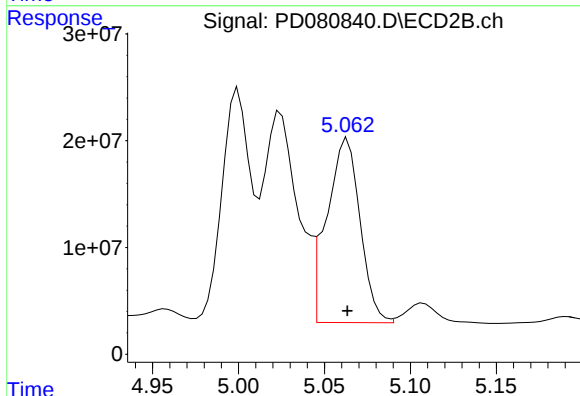


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 232696542
Conc: 742.74 ng/ml

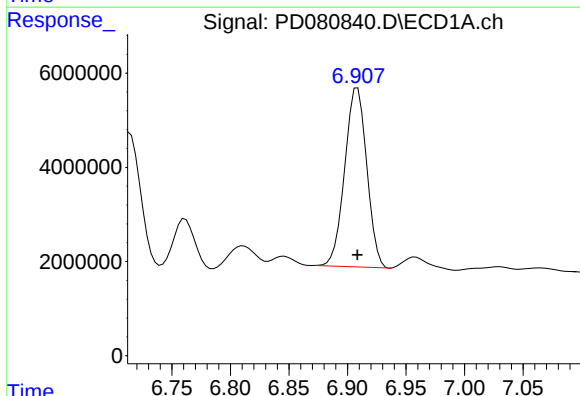


#27 Chlordane-5

R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 49867568
Conc: 739.88 ng/ml

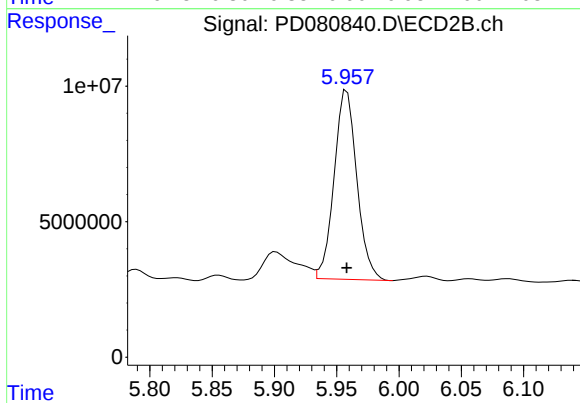

#27 Chlordane-5


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 88896915
Conc: 745.03 ng/ml

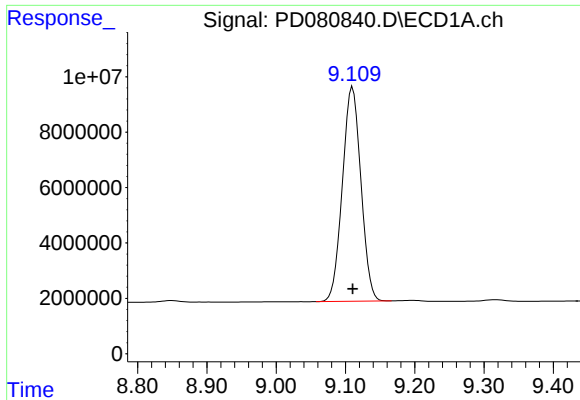

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 143688001
Conc: 74.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

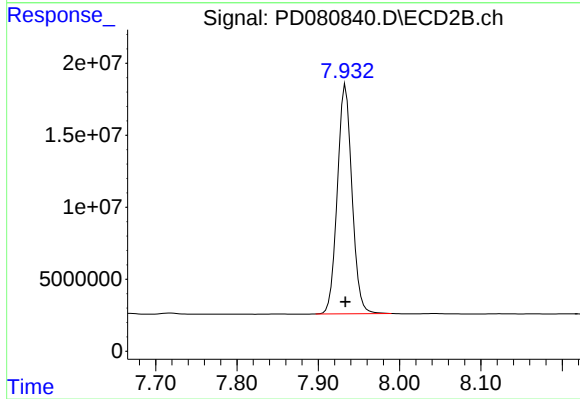

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 198694145
Conc: 74.28 ng/ml