

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 17:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 17:45:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 17:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	71480477	145.3E6	50.000	50.000
28)	SA Decachlor...	9.110	7.933	100.5E6	137.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.733	3.794	37258991	50084958	500.000	500.000
24)	Chlordane-2	5.263	4.370	39112455	58770860	500.000	500.000
25)	Chlordane-3	5.974	4.999	150.9E6	165.8E6	500.000	500.000
26)	Chlordane-4	6.057	5.063	180.5E6	155.7E6	500.000	500.000
27)	Chlordane-5	6.908	5.957	33999442	60152499	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 17:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 17:45:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 17:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

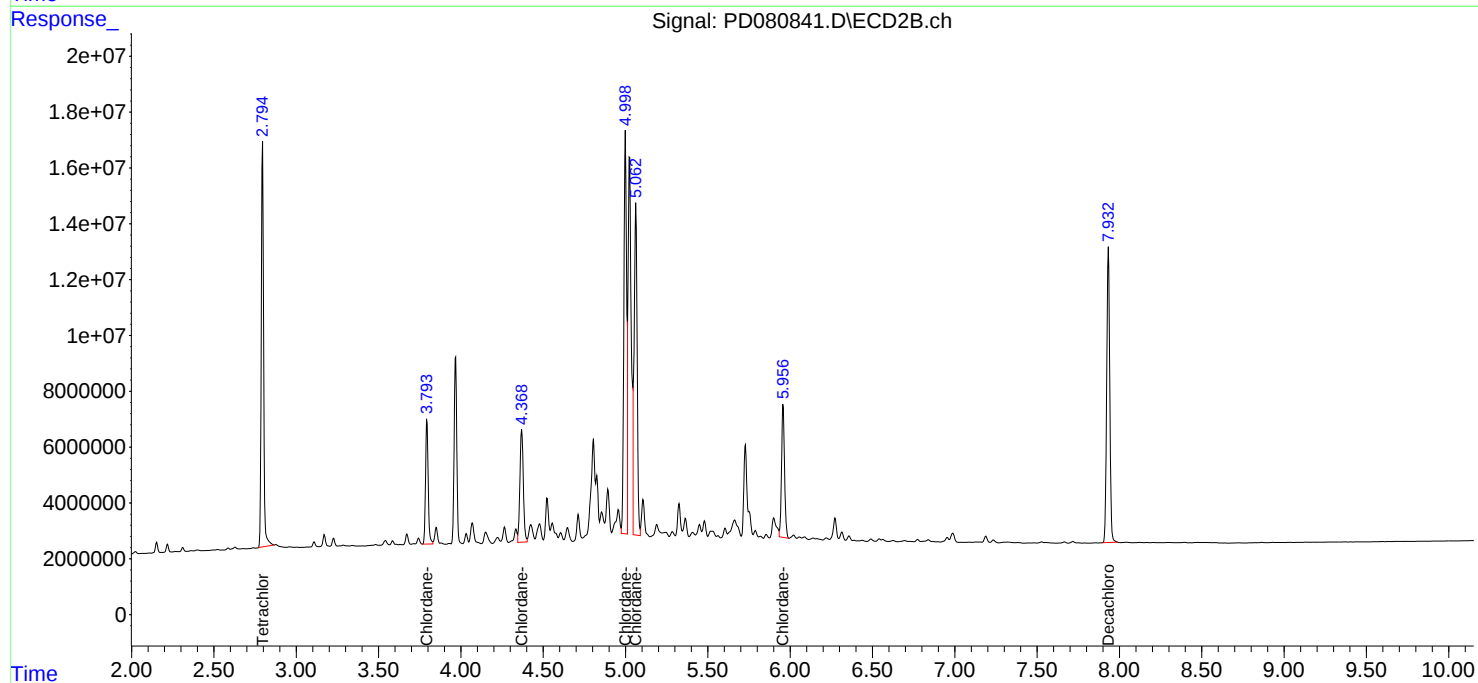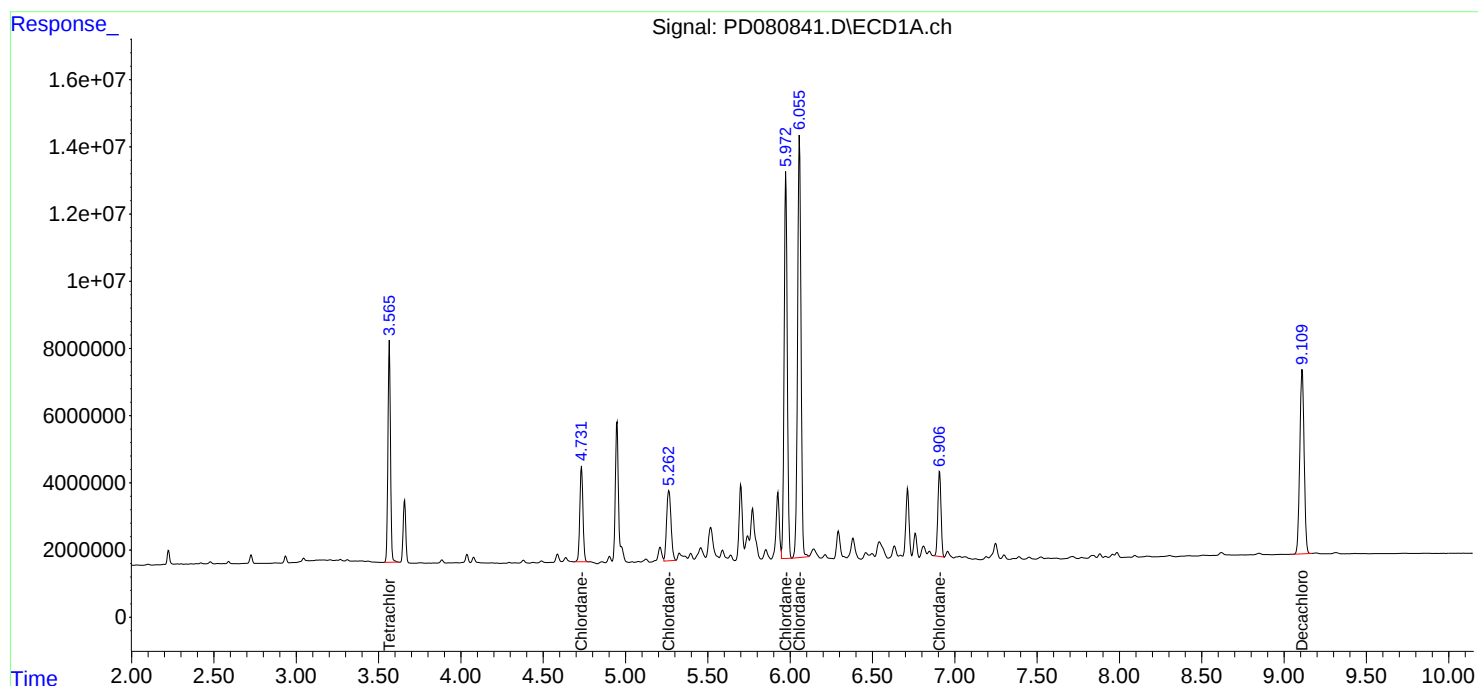


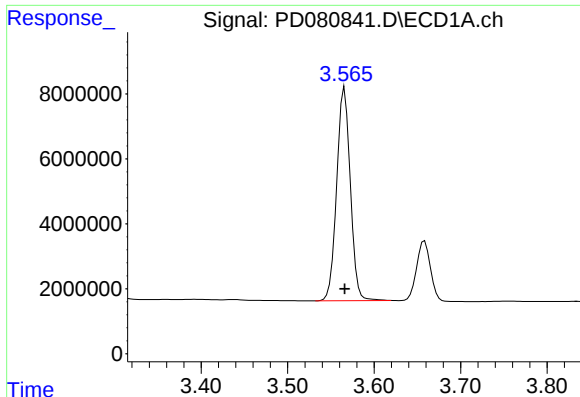

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 71480477
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

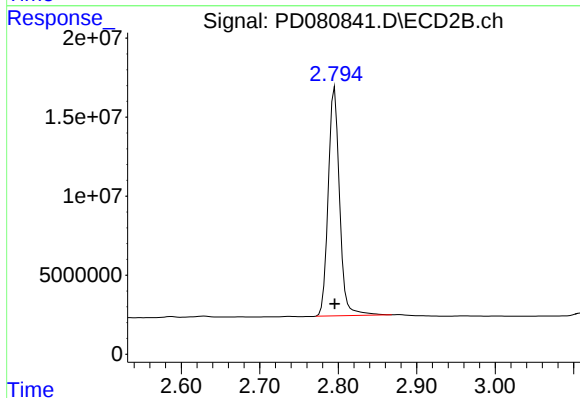


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 145325062
Conc: 50.00 ng/ml

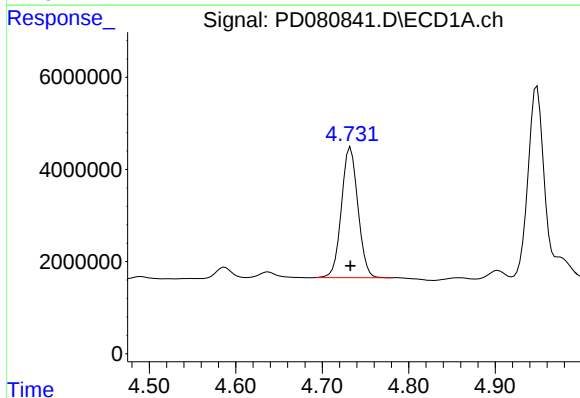


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 37258991
Conc: 500.00 ng/ml

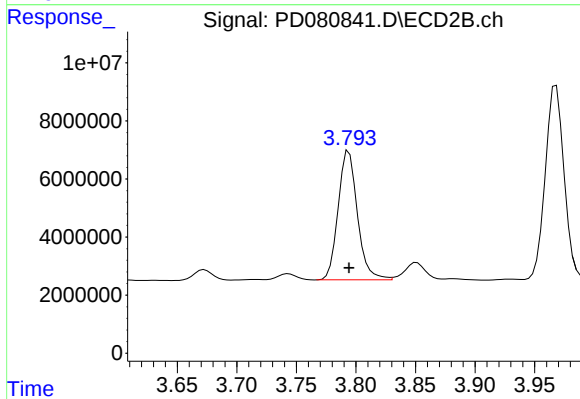

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 50084958
Conc: 500.00 ng/ml

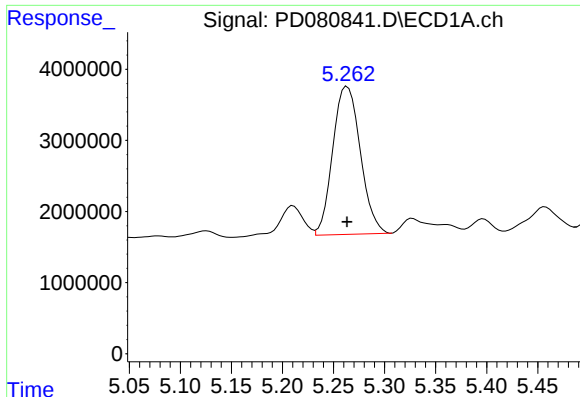

#24 Chlordane-2


R.T.: 5.263 min
Delta R.T.: 0.000 min
Response: 39112455
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

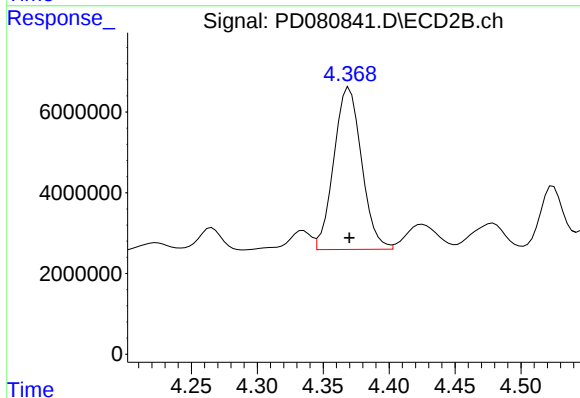


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 58770860
Conc: 500.00 ng/ml

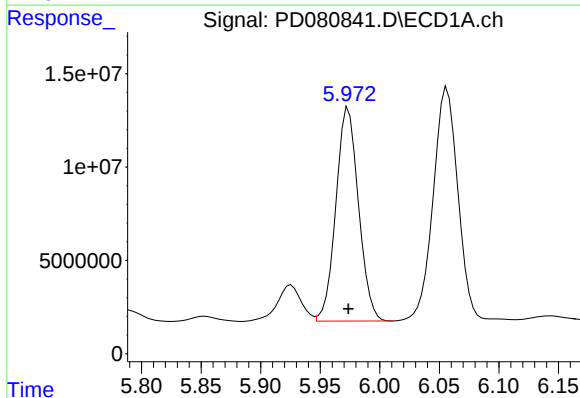


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 150943883
Conc: 500.00 ng/ml

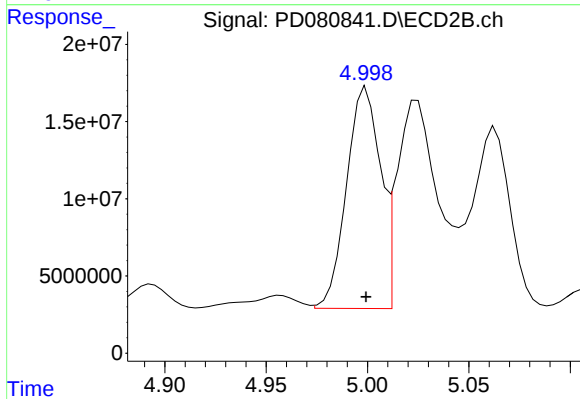

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 165819558
Conc: 500.00 ng/ml

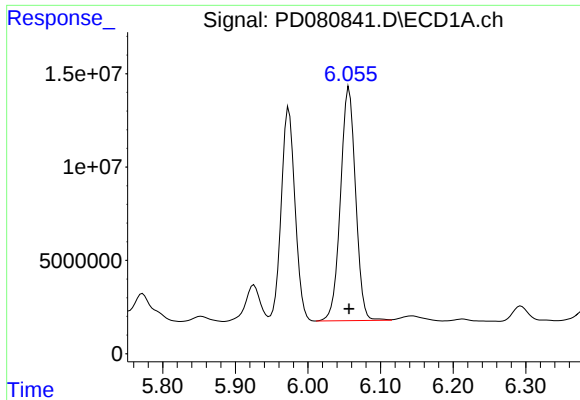

#26 Chlordane-4


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 180491477
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

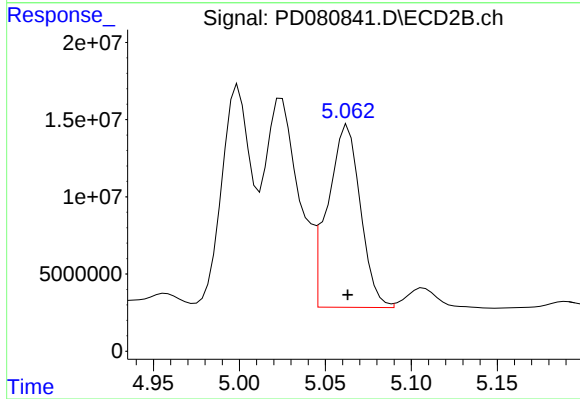


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 155658636
Conc: 500.00 ng/ml

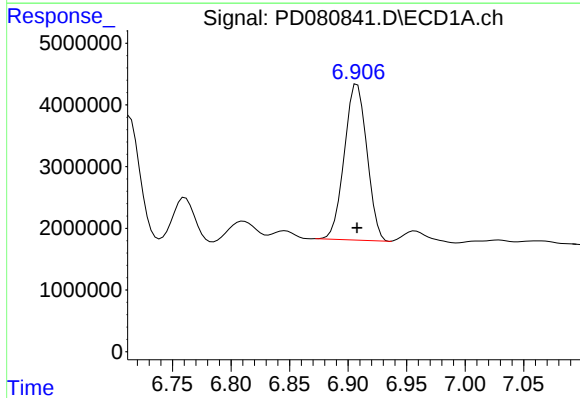


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 33999442
Conc: 500.00 ng/ml

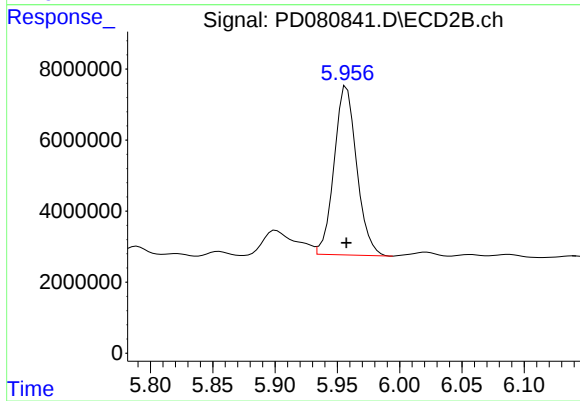

#27 Chlordane-5


R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 60152499
Conc: 500.00 ng/ml

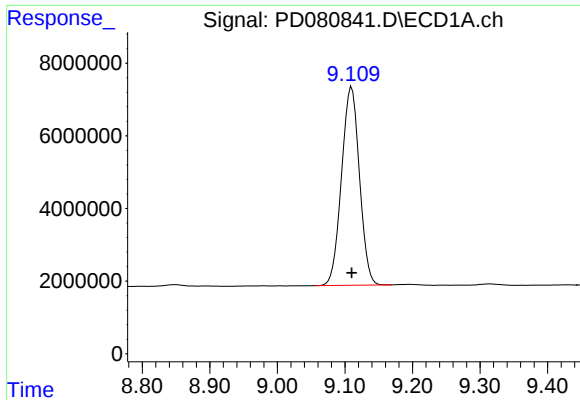

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 100531427
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

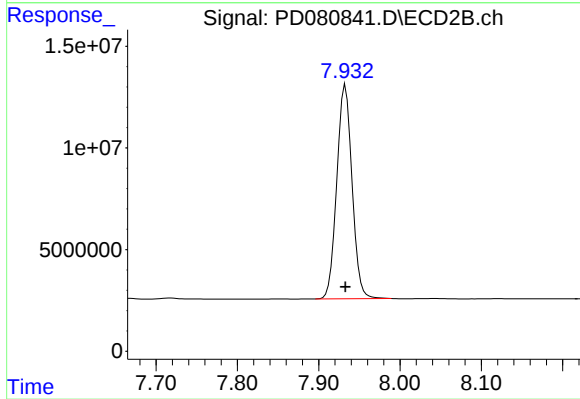

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 137174222
Conc: 50.00 ng/ml