

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2024 03:04
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 11:09:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:08:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	75945151	153.8E6	52.223	51.965
28)	SA Decachlor...	9.112	7.935	104.5E6	147.5E6	50.163	51.921
Target Compounds							
23)	Chlordane-1	4.734	3.795	39229145	53577958	508.072	526.853
24)	Chlordane-2	5.265	4.371	41134470	62418984	496.902	509.248
25)	Chlordane-3	5.975	5.001	162.5E6	178.1E6	514.446	530.674
26)	Chlordane-4	6.057	5.065	194.7E6	170.8E6	511.360	537.630
27)	Chlordane-5	6.908	5.959	35519754	64003864	508.805	527.904



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2024 03:04
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 11:09:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:08:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

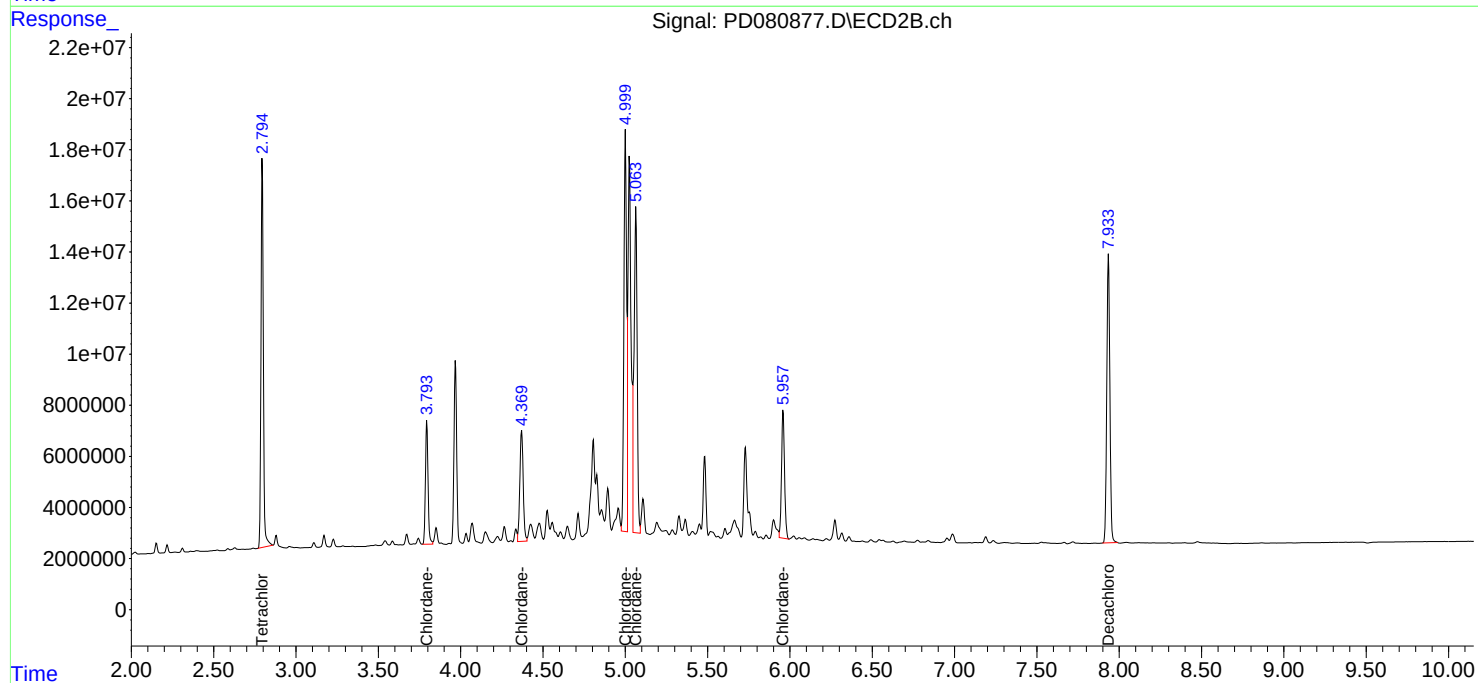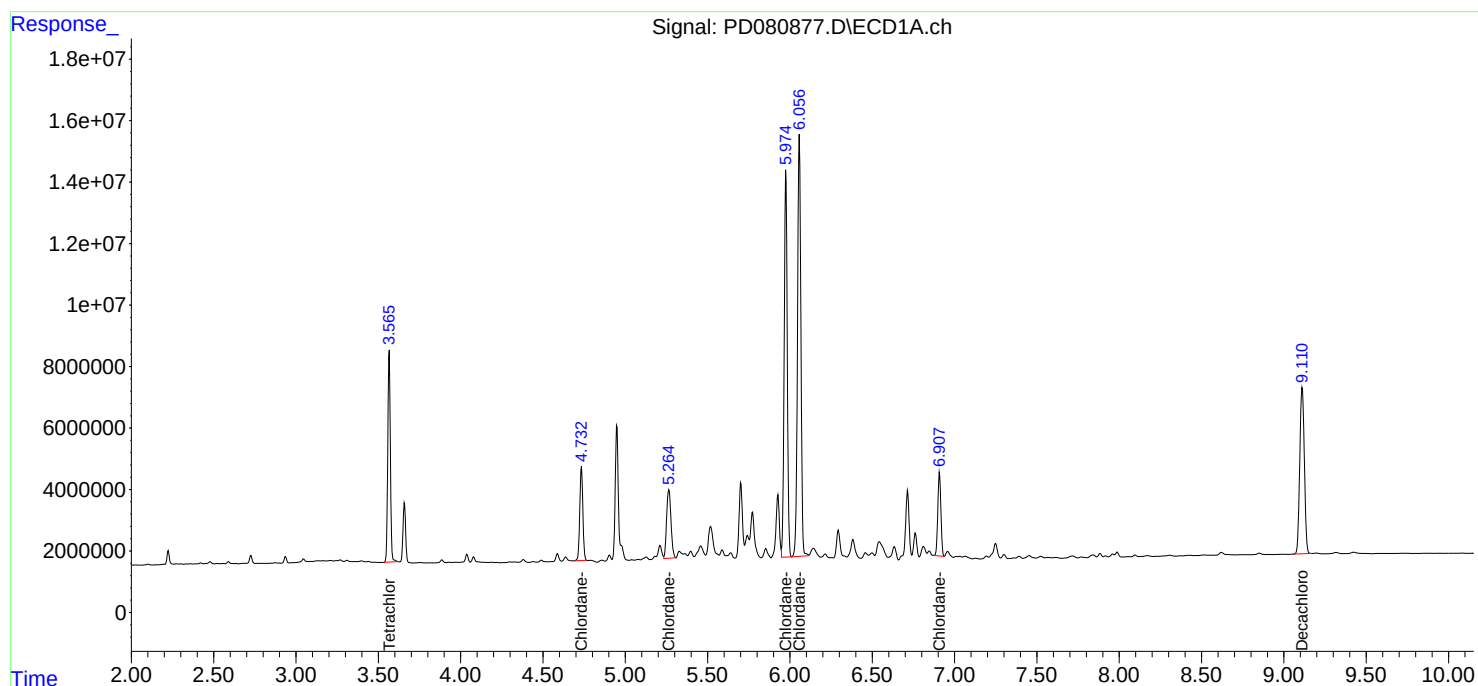


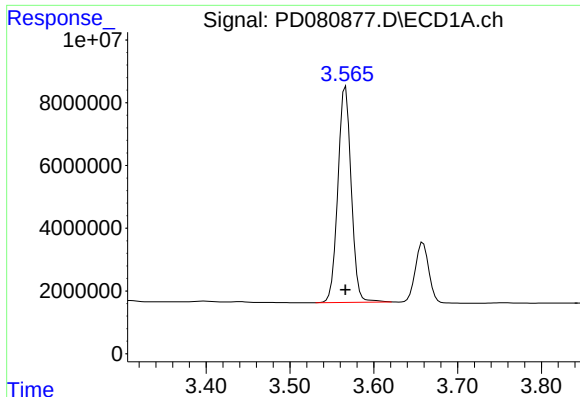

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 75945151
Conc: 52.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

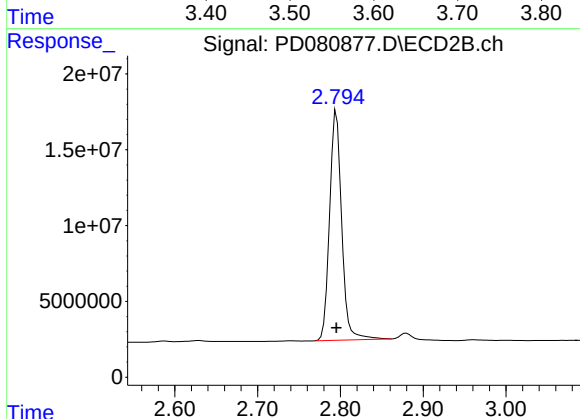


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 153752678
Conc: 51.97 ng/ml

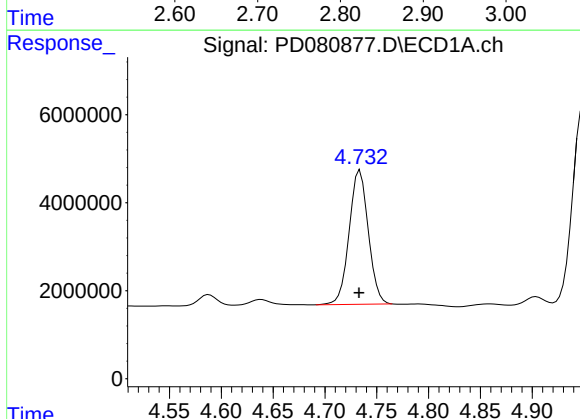


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 39229145
Conc: 508.07 ng/ml

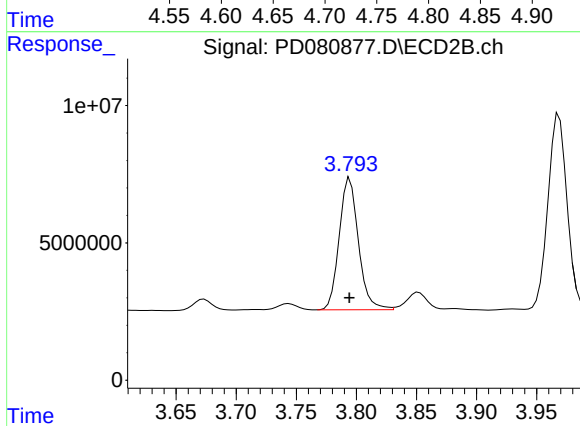

#23 Chlordane-1


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 53577958
Conc: 526.85 ng/ml

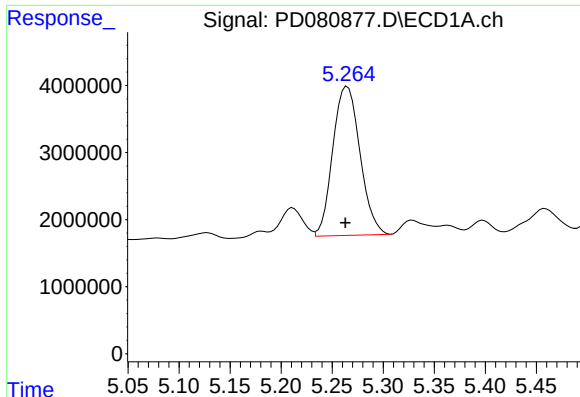

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.002 min
Response: 41134470
Conc: 496.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

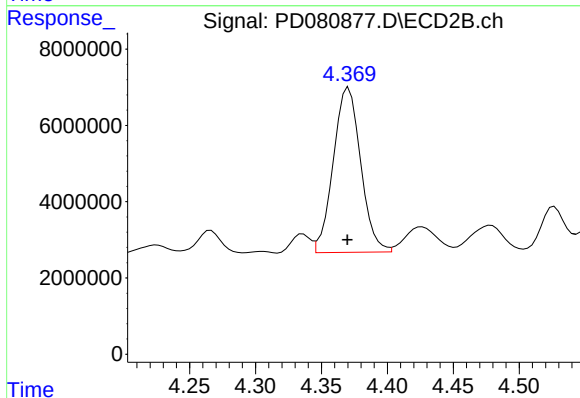


#24 Chlordane-2

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 62418984
Conc: 509.25 ng/ml

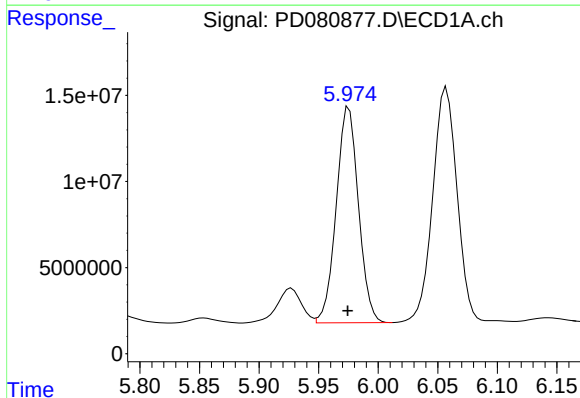


#25 Chlordane-3

R.T.: 5.975 min
Delta R.T.: 0.001 min
Response: 162458898
Conc: 514.45 ng/ml

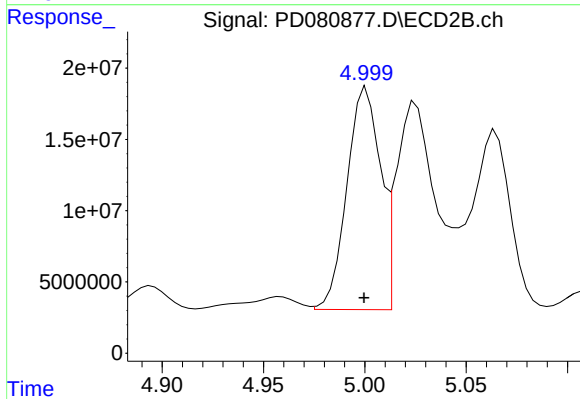

#25 Chlordane-3


R.T.: 5.001 min
Delta R.T.: 0.001 min
Response: 178102663
Conc: 530.67 ng/ml

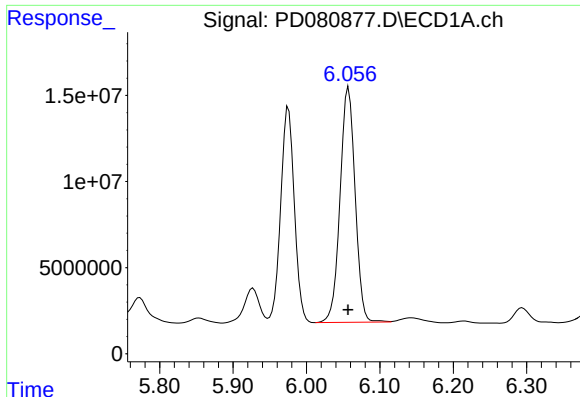

#26 Chlordane-4


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 194697803
Conc: 511.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

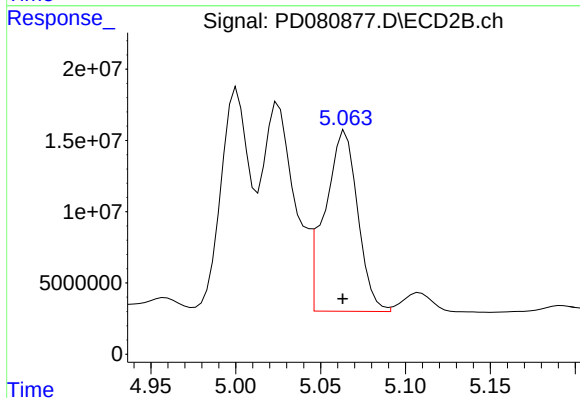


#26 Chlordane-4

R.T.: 5.065 min
Delta R.T.: 0.002 min
Response: 170802416
Conc: 537.63 ng/ml

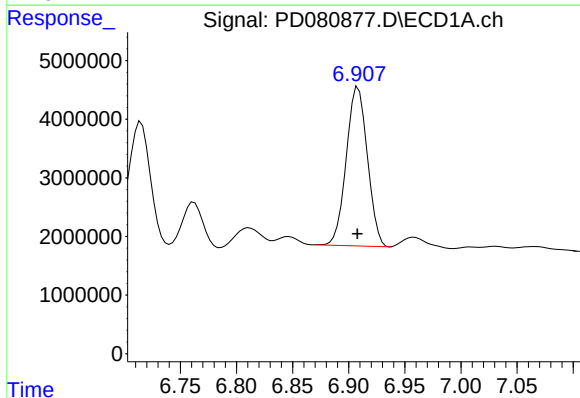


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 35519754
Conc: 508.81 ng/ml

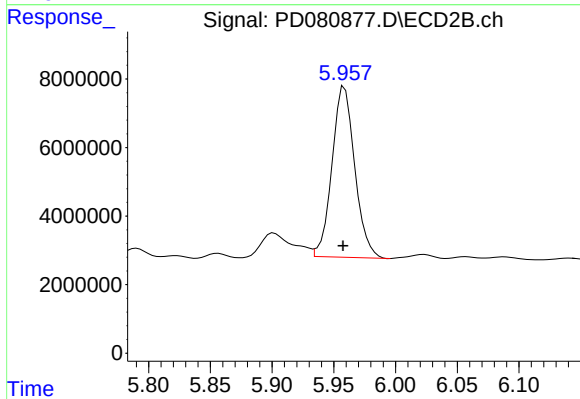

#27 Chlordane-5


R.T.: 5.959 min
Delta R.T.: 0.001 min
Response: 64003864
Conc: 527.90 ng/ml

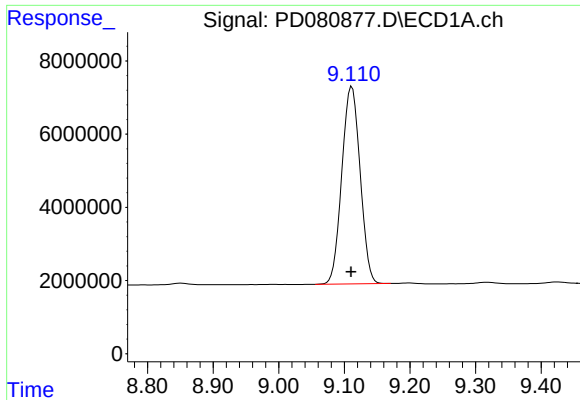

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.001 min
Response: 104548482
Conc: 50.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

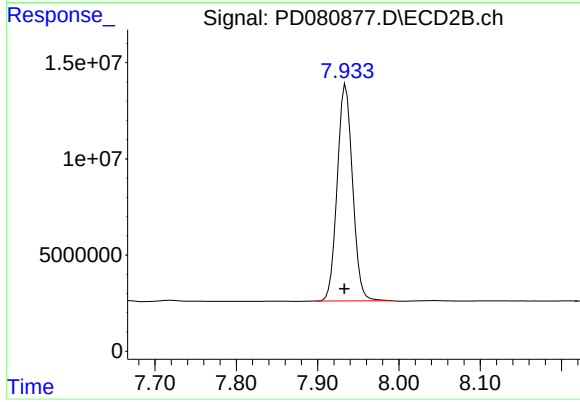

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.002 min
Response: 147486488
Conc: 51.92 ng/ml