

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 12:35
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 17:55:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 17:33:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	0.000	4.662f	0	227219	N.D. <MDL
5) MB	Aldrin	0.000	5.511	0	1618468	N.D. 0.165
6) B	beta-BHC	4.437f	4.821f	264708	1427862	0.425 0.334
7) B	delta-BHC	0.000	5.059	0	5028646	N.D. 0.493
8) B	Heptachlo...	5.165f	5.892	406800	2897849	0.299 0.334
9) A	Endosulfan I	0.000	6.265	0	1090628	N.D. 0.122
10) B	trans-Chl...	0.000	6.161	0	3711674	N.D. 0.395
11) B	cis-Chlor...	0.000	6.227	0	2844120	N.D. 0.320
15) B	Endosulfa...	6.284f	6.904f	4487199	17794991	4.130 2.473 #
16) A	4,4'-DDD	0.000	6.904f	0	17794991	N.D. 2.477
20) A	Methoxychlor	7.038f	7.621	1483987	392939	2.377 0.119 #
24)	Toxaphene-3	6.284	0.000	4487199	0	324.025 N.D. #
26)	Toxaphene-5	7.081	0.000	3915020	0	112.683 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 12:35
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 17:55:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 17:33:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

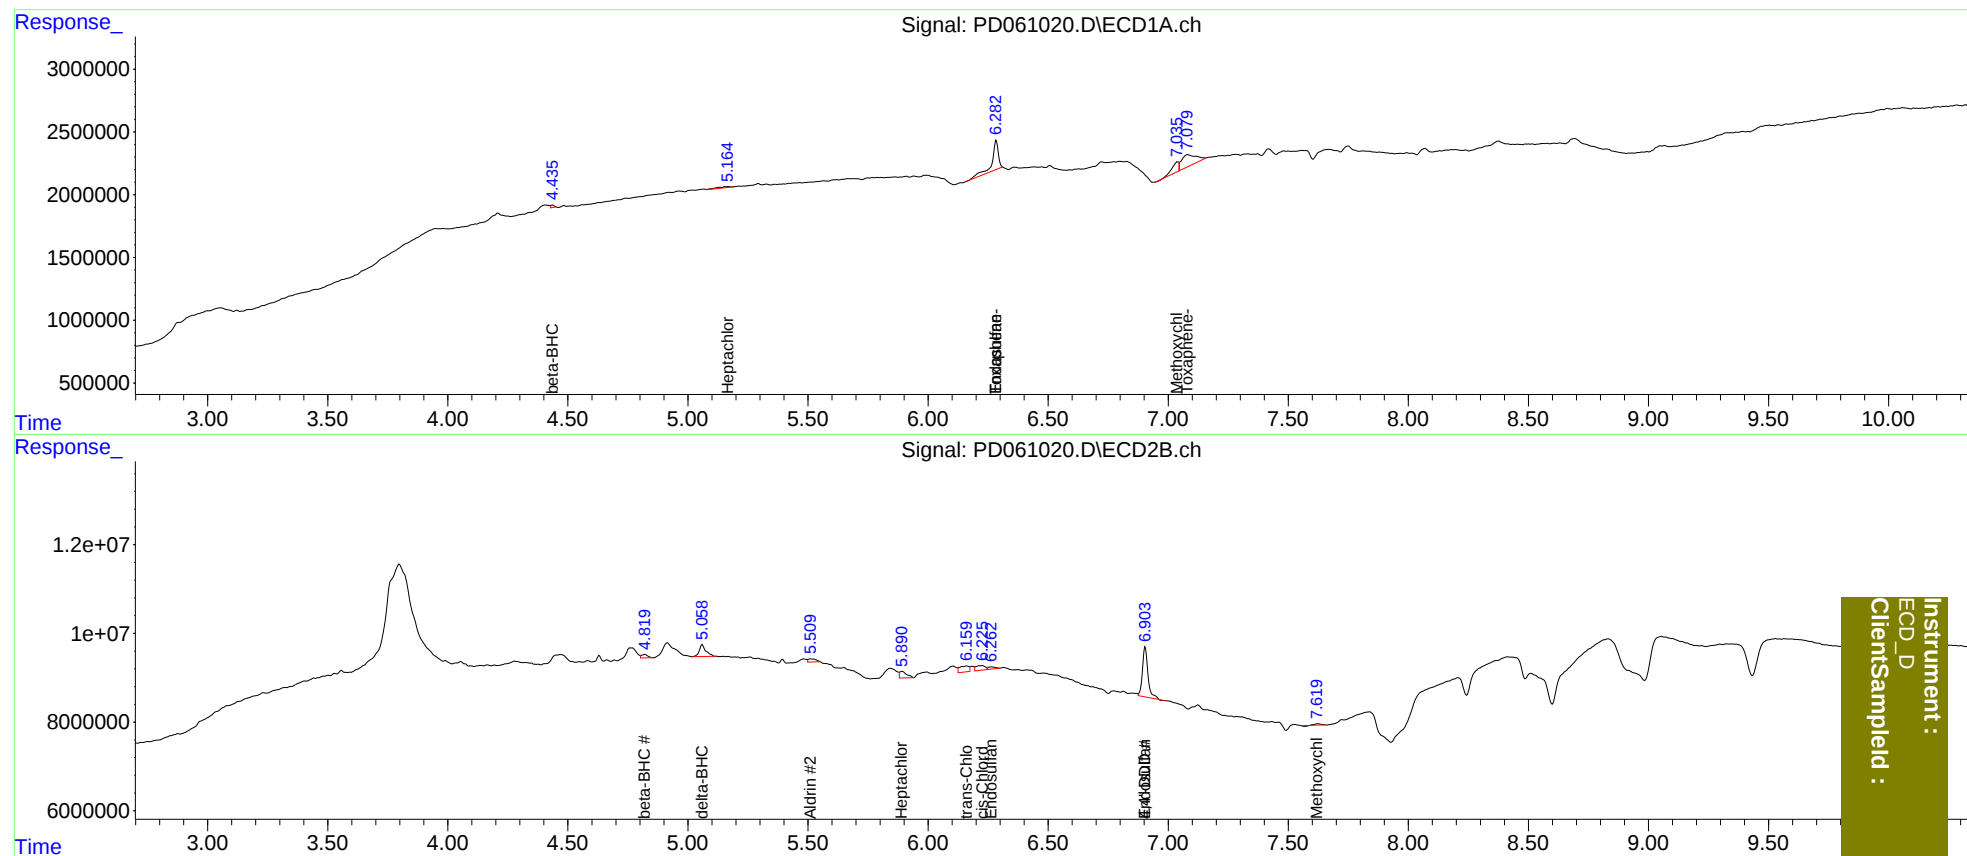


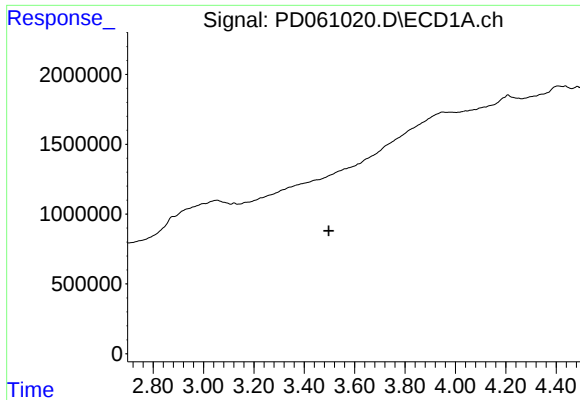

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

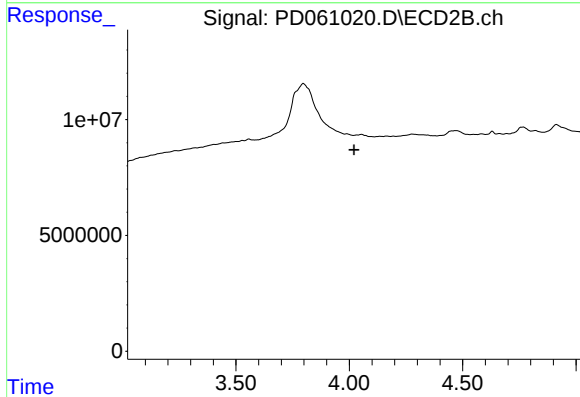


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.021 min
Response: 0
Conc: N.D.

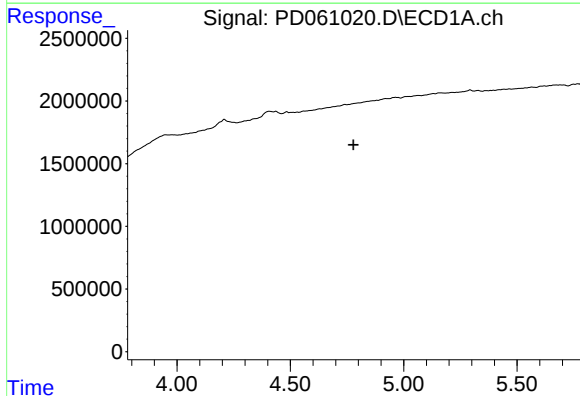


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.779 min
Response: 0
Conc: N.D.

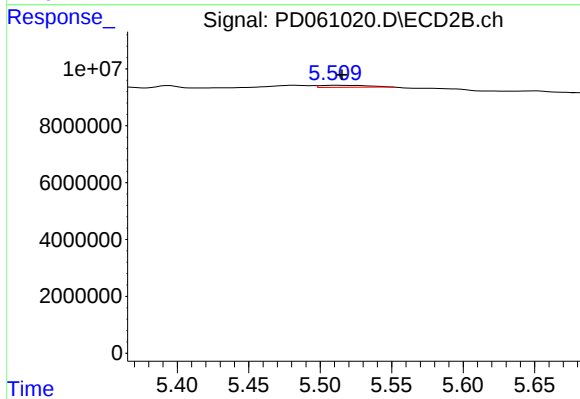

#5 Aldrin


R.T.: 5.511 min
Delta R.T.: -0.004 min
Response: 1618468
Conc: 0.16 ng/ml

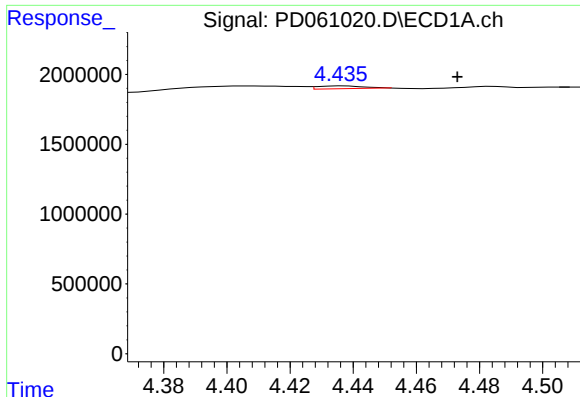

#6 beta-BHC


R.T.: 4.437 min
Delta R.T.: -0.036 min
Response: 264708
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

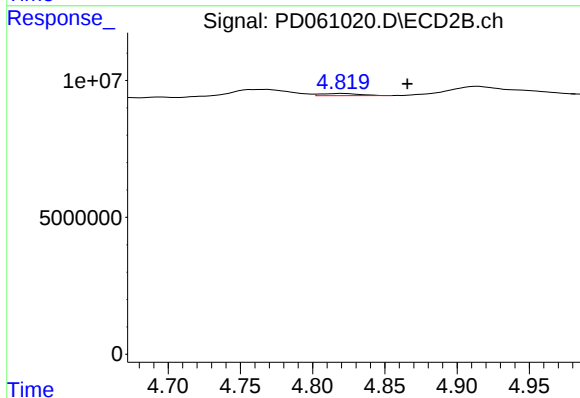


#6 beta-BHC

R.T.: 4.821 min
Delta R.T.: -0.045 min
Response: 1427862
Conc: 0.33 ng/ml

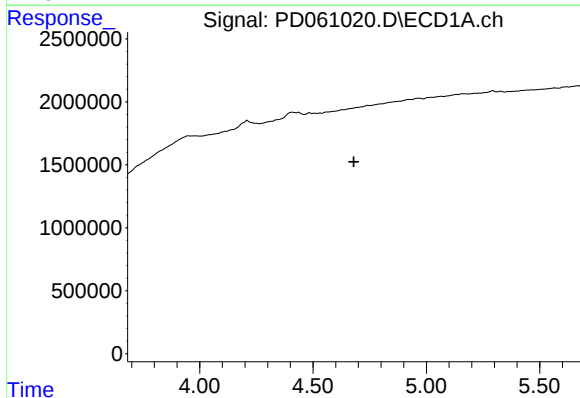


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.680 min
Response: 0
Conc: N.D.

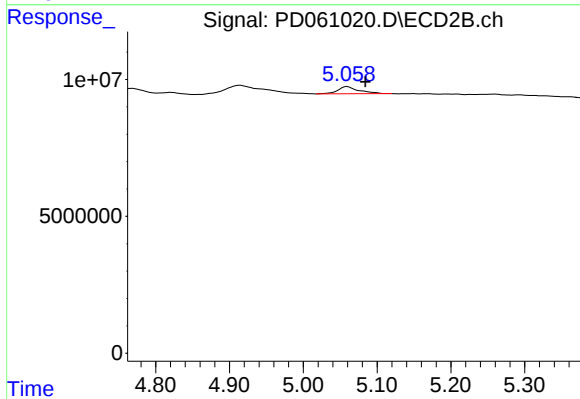

#7 delta-BHC


R.T.: 5.059 min
Delta R.T.: -0.025 min
Response: 5028646
Conc: 0.49 ng/ml

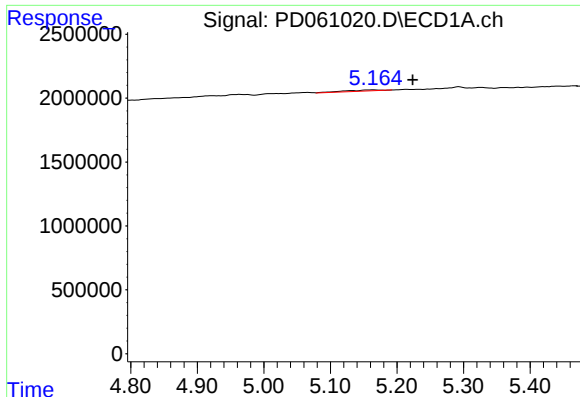

#8 Heptachlor epoxide


R.T.: 5.165 min
Delta R.T.: -0.059 min
Response: 406800
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

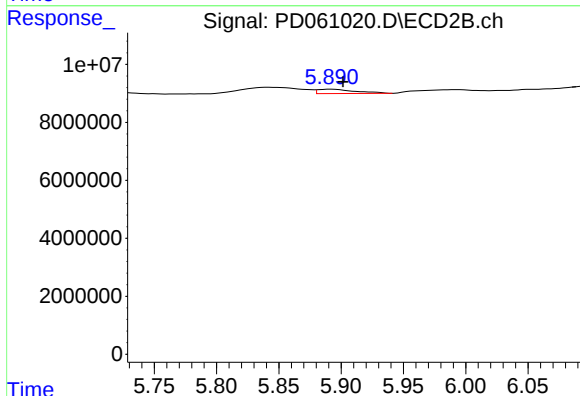


#8 Heptachlor epoxide

R.T.: 5.892 min
Delta R.T.: -0.010 min
Response: 2897849
Conc: 0.33 ng/ml

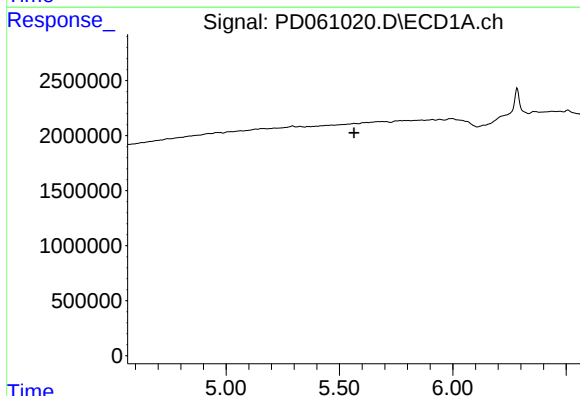


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

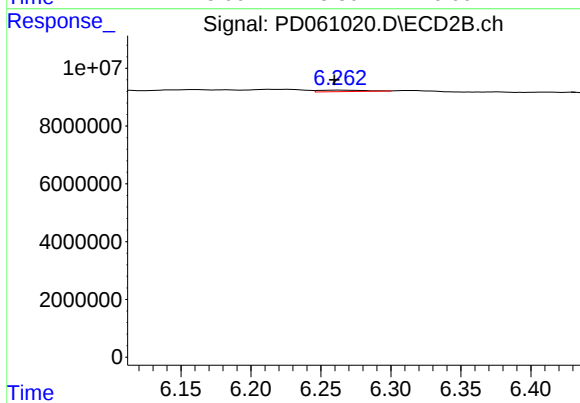

#9 Endosulfan I


R.T.: 6.265 min
Delta R.T.: 0.005 min
Response: 1090628
Conc: 0.12 ng/ml

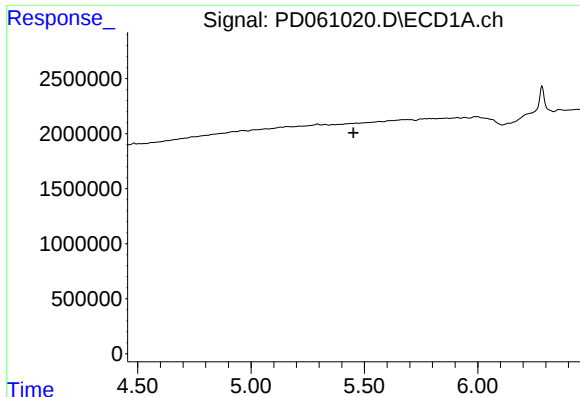

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.452 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

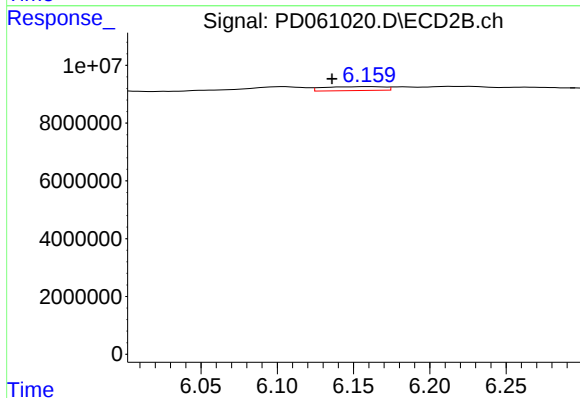


#10 trans-Chlordane

R.T.: 6.161 min
Delta R.T.: 0.025 min
Response: 3711674
Conc: 0.39 ng/ml

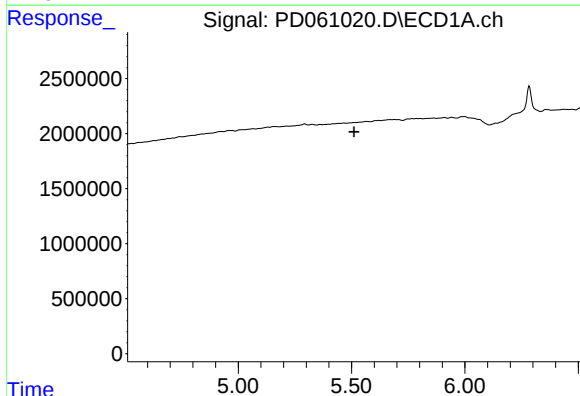


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

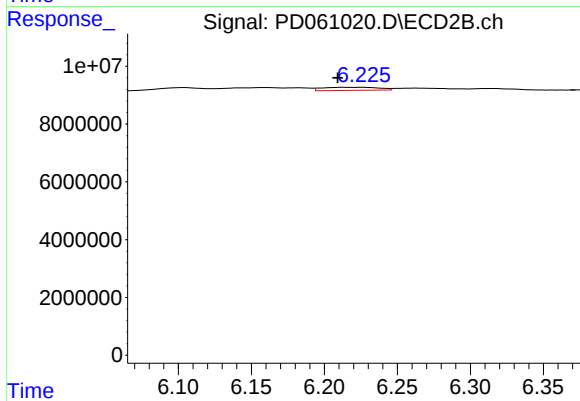

#11 cis-Chlordane


R.T.: 6.227 min
Delta R.T.: 0.018 min
Response: 2844120
Conc: 0.32 ng/ml

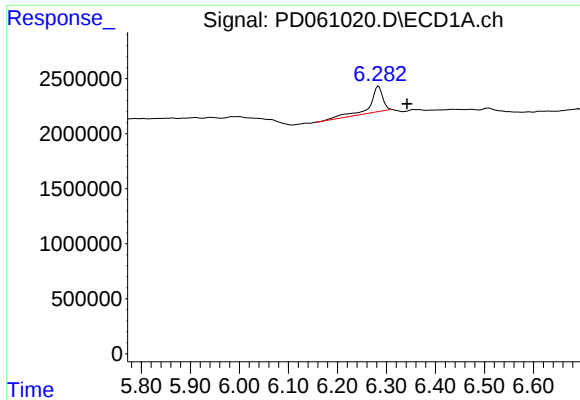

#15 Endosulfan II


R.T.: 6.284 min
Delta R.T.: -0.058 min
Response: 4487199
Conc: 4.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

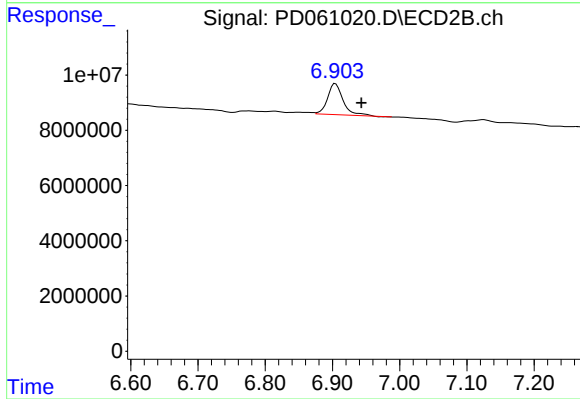


#15 Endosulfan II

R.T.: 6.904 min
Delta R.T.: -0.039 min
Response: 17794991
Conc: 2.47 ng/ml

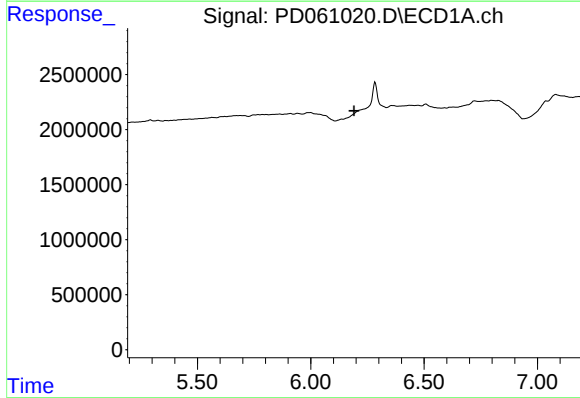


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.191 min
Response: 0
Conc: N.D.

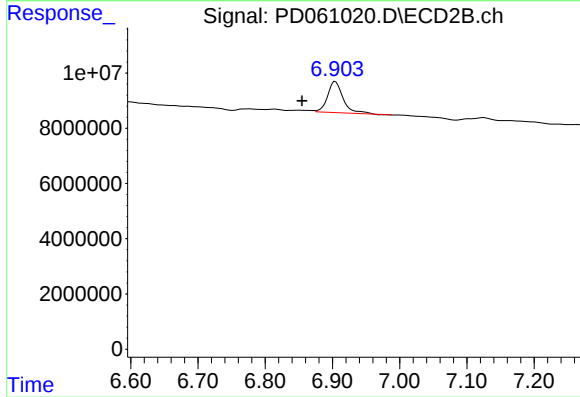

#16 4,4'-DDD


R.T.: 6.904 min
Delta R.T.: 0.049 min
Response: 17794991
Conc: 2.48 ng/ml

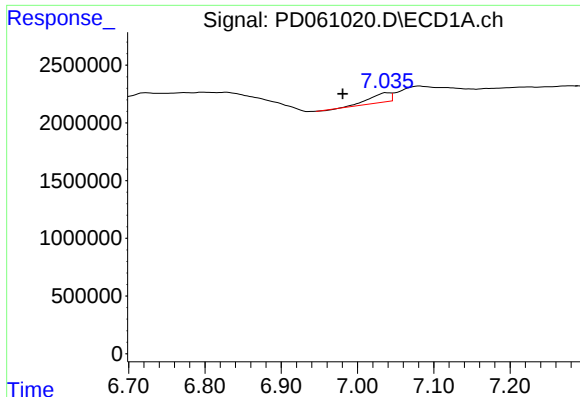

#20 Methoxychlor


R.T.: 7.038 min
Delta R.T.: 0.057 min
Response: 1483987
Conc: 2.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

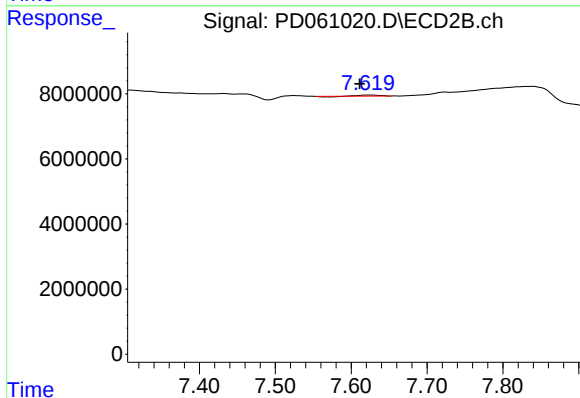


#20 Methoxychlor

R.T.: 7.621 min
Delta R.T.: 0.009 min
Response: 392939
Conc: 0.12 ng/ml

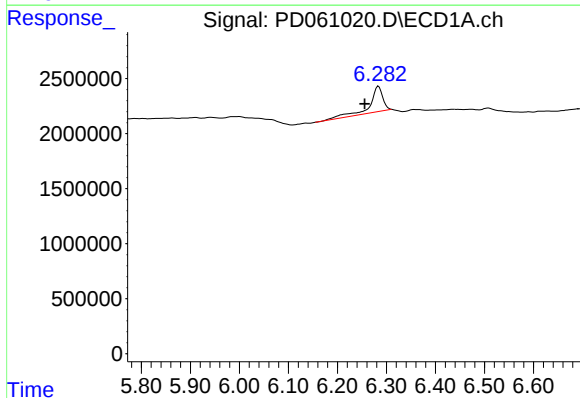


#24 Toxaphene-3

R.T.: 6.284 min
Delta R.T.: 0.028 min
Response: 4487199
Conc: 324.03 ng/ml

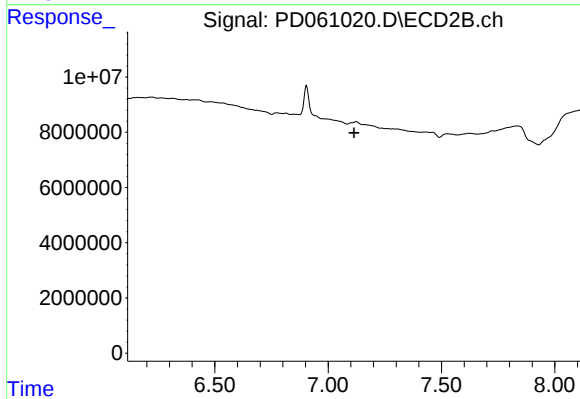

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.114 min
Response: 0
Conc: N.D.

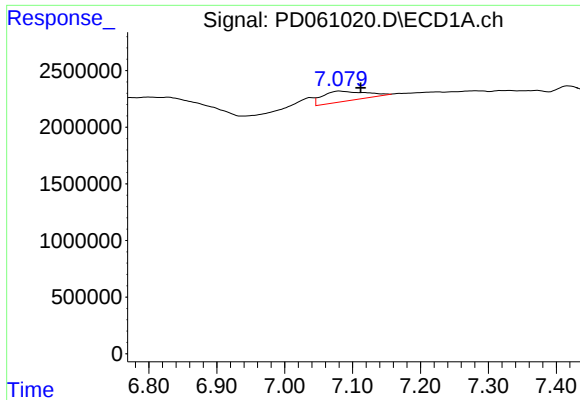

#26 Toxaphene-5


R.T.: 7.081 min
Delta R.T.: -0.031 min
Response: 3915020
Conc: 112.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

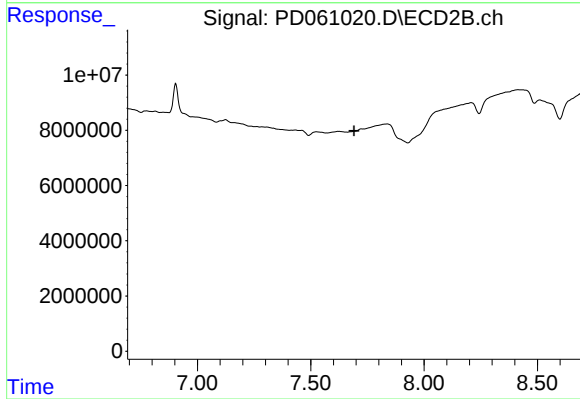


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.692 min
Response: 0
Conc: N.D.

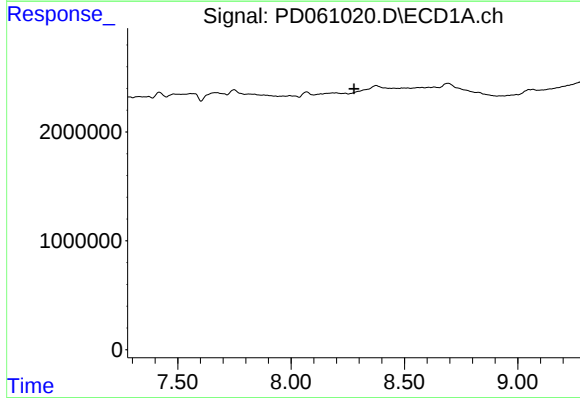

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.278 min
Response: 0
Conc: N.D.

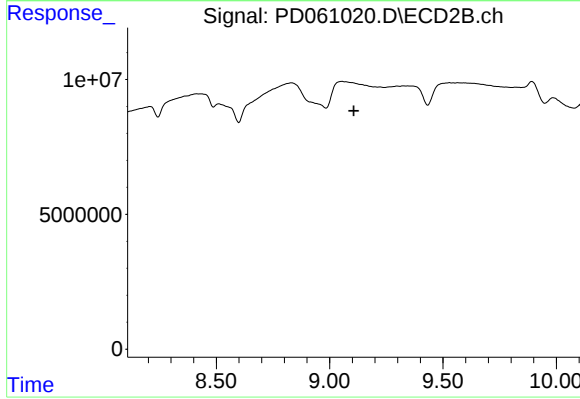

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.106 min
Response: 0
Conc: N.D.