

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 14:27
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:57:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 16:53:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	5400273	37002768	5.206	4.972
27)	SA Decachlor...	8.278	9.106	13505377	72718342	10.526	10.750
Target Compounds							
2)	A alpha-BHC	3.937	4.411	7550924	55689151	4.991	4.876
3)	MA gamma-BHC...	4.222	4.697	7834287	51280220	5.318	4.873
4)	MA Heptachlor	4.527	5.209	7739064	54536373	5.029	5.001
9)	A Endosulfan I	5.564	6.260	6714863	47548302	5.046	5.315
13)	MA Dieldrin	5.809	6.517	14818893	95107232	9.858	9.950
14)	MA Endrin	6.067	6.735	12761328	75656150	10.224	10.101
16)	A 4,4'-DDD	6.191	6.855	12414116	74048797	10.327	10.086
17)	MA 4,4'-DDT	6.434	7.155	12650326	76593871	9.969	10.190
20)	A Methoxychlor	6.981	7.611	33158637	178.4E6	51.748	53.062


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 14:27
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:57:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 16:53:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

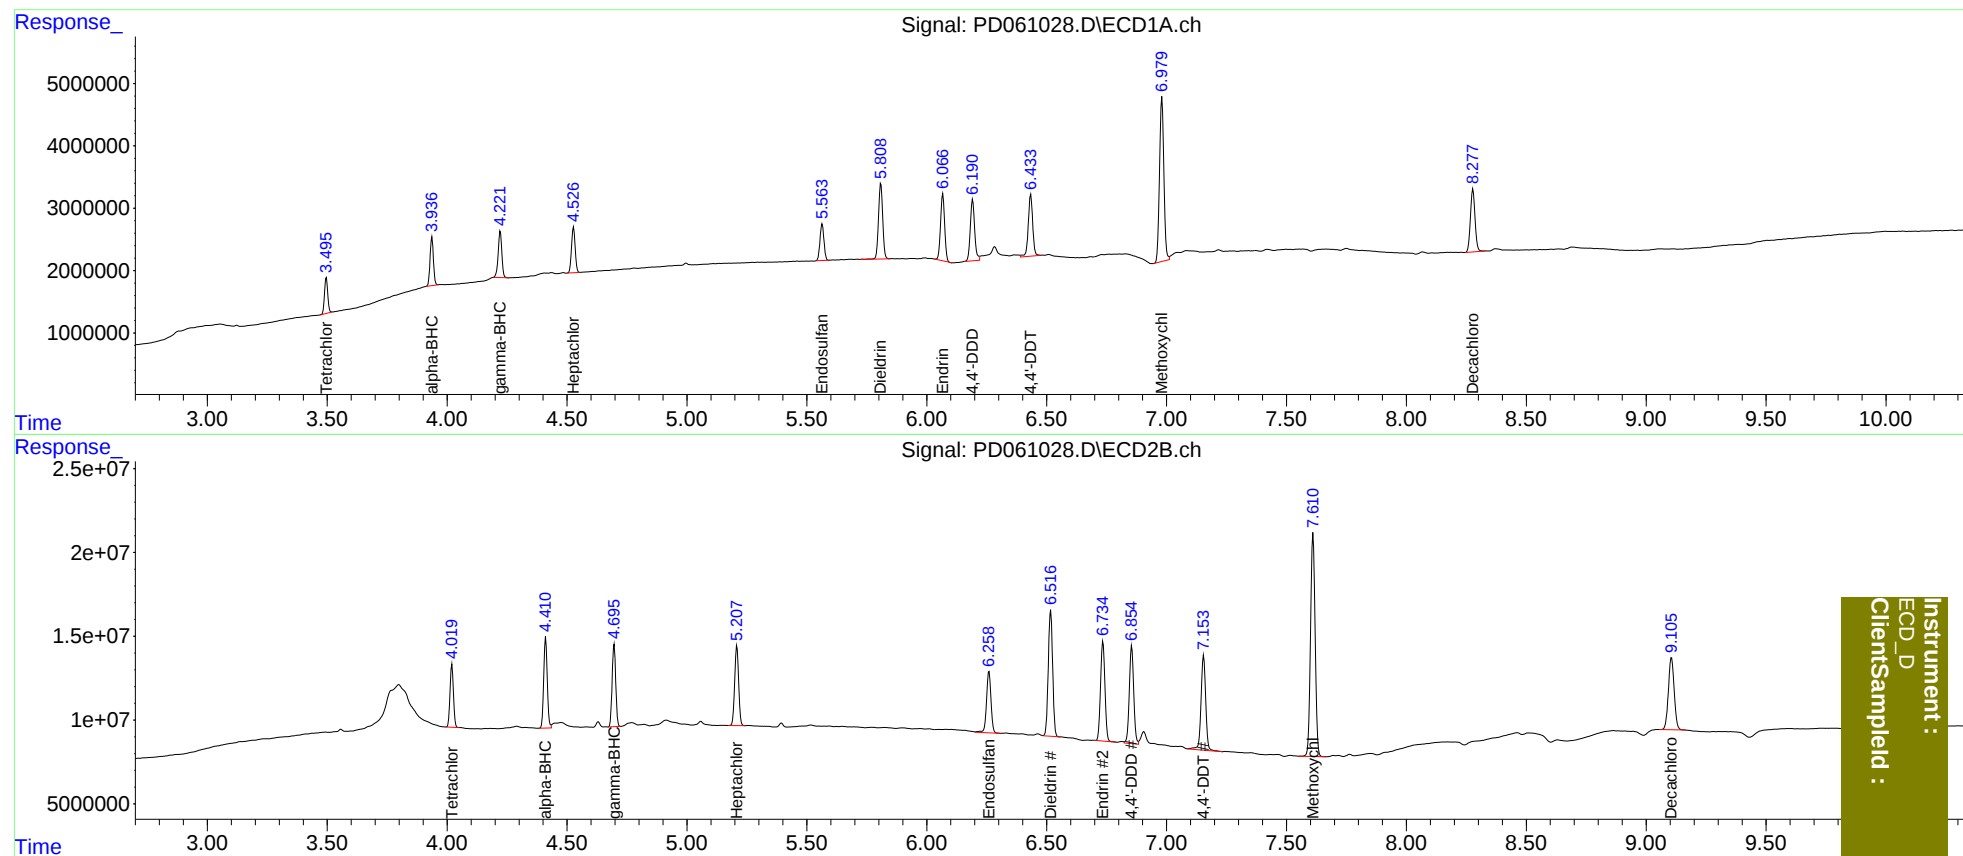


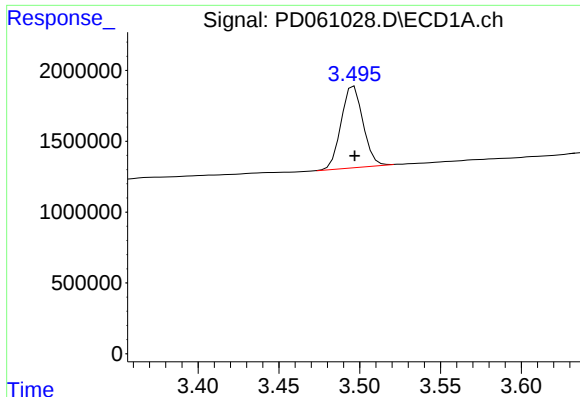

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 5400273
Conc: 5.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

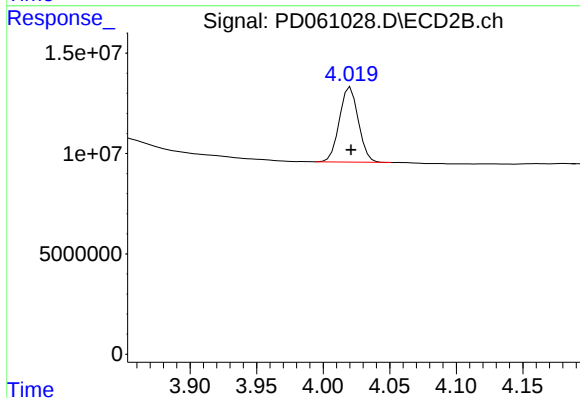


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 37002768
Conc: 4.97 ng/ml

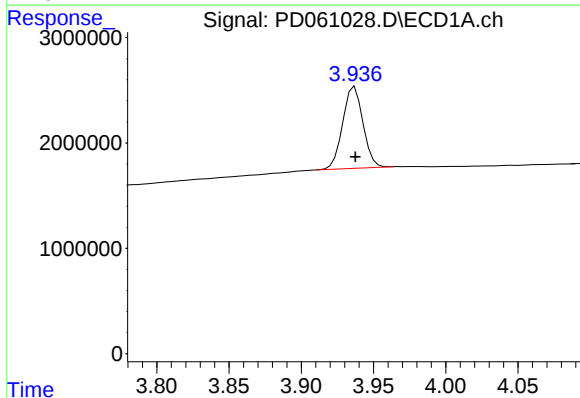


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 7550924
Conc: 4.99 ng/ml

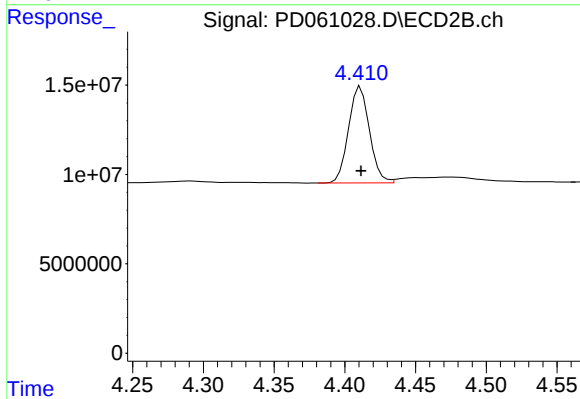

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 55689151
Conc: 4.88 ng/ml

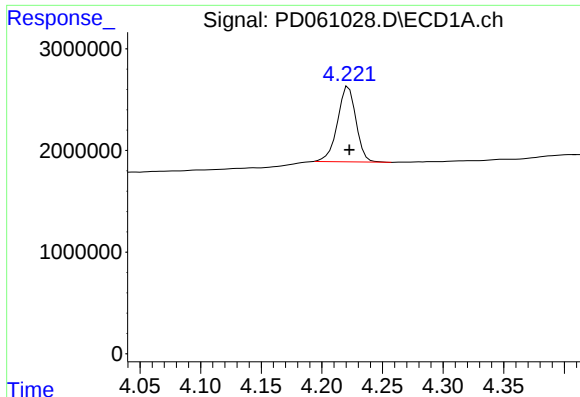

#3 gamma-BHC (Lindane)


R.T.: 4.222 min
Delta R.T.: 0.000 min
Response: 7834287
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

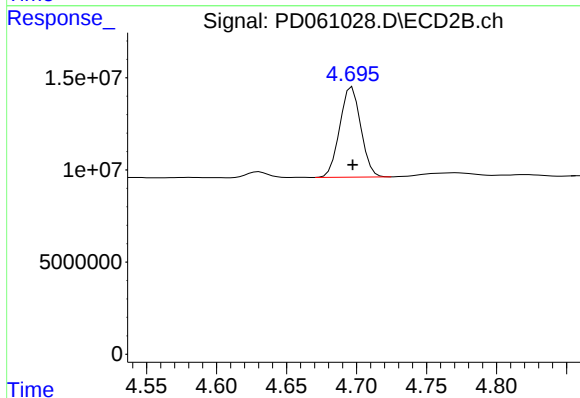


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 51280220
Conc: 4.87 ng/ml

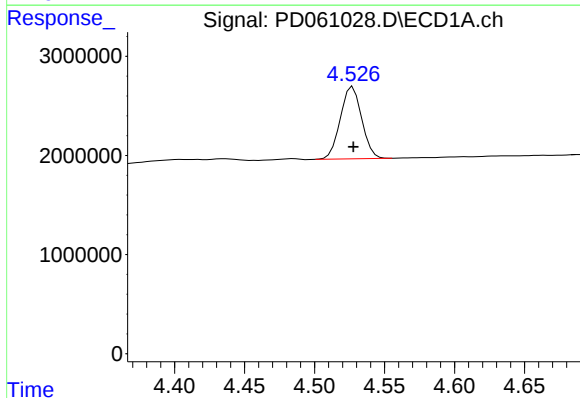


#4 Heptachlor

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 7739064
Conc: 5.03 ng/ml

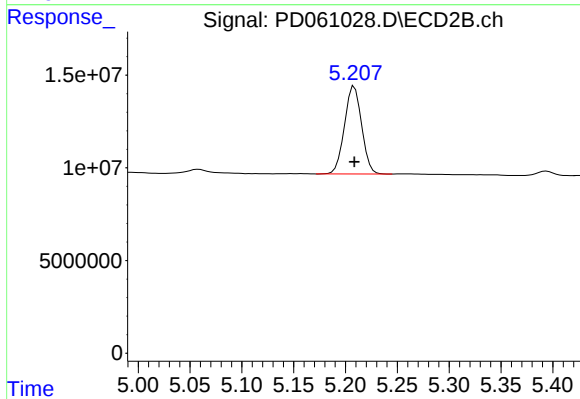

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 54536373
Conc: 5.00 ng/ml

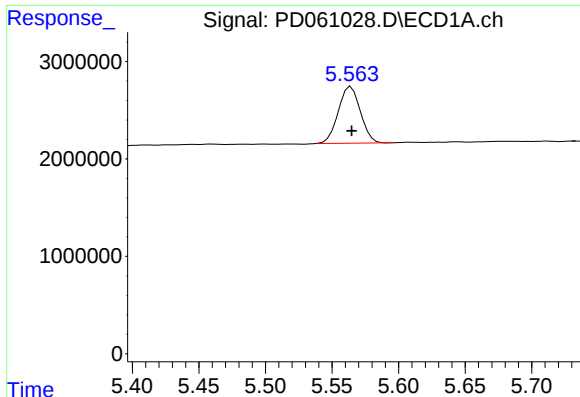

#9 Endosulfan I


R.T.: 5.564 min
Delta R.T.: 0.000 min
Response: 6714863
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

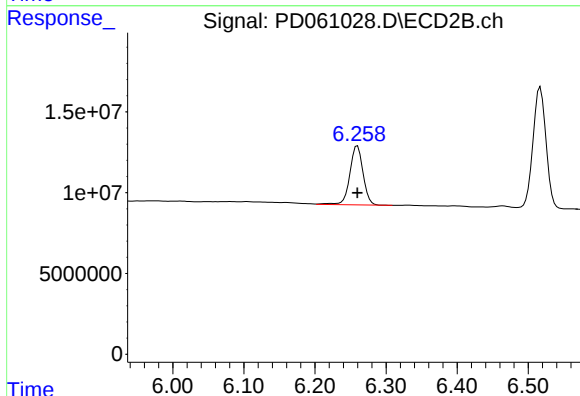


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 47548302
Conc: 5.31 ng/ml

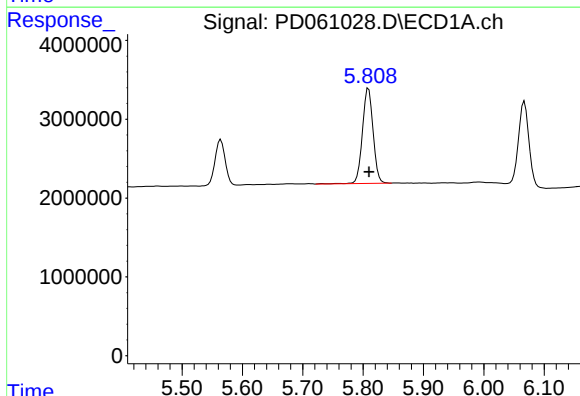


#13 Dieldrin

R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 14818893
Conc: 9.86 ng/ml

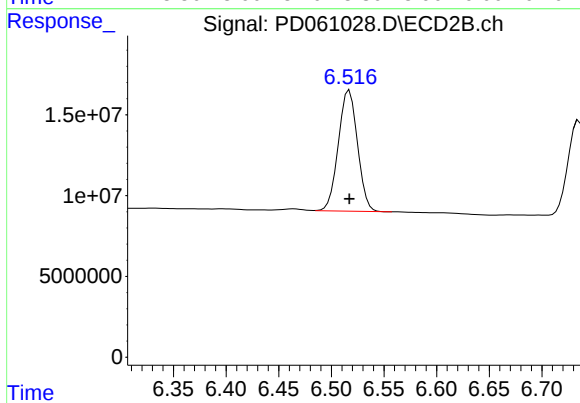

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 95107232
Conc: 9.95 ng/ml

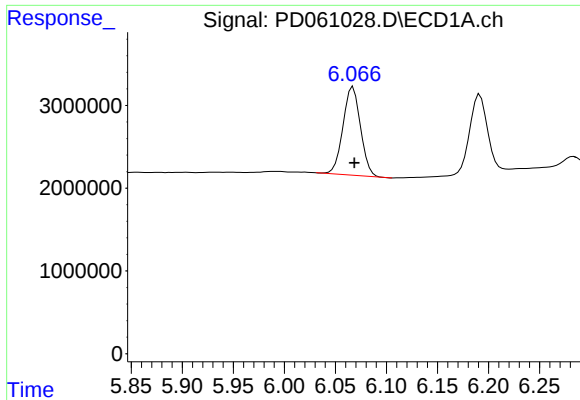

#14 Endrin


R.T.: 6.067 min
Delta R.T.: -0.001 min
Response: 12761328
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

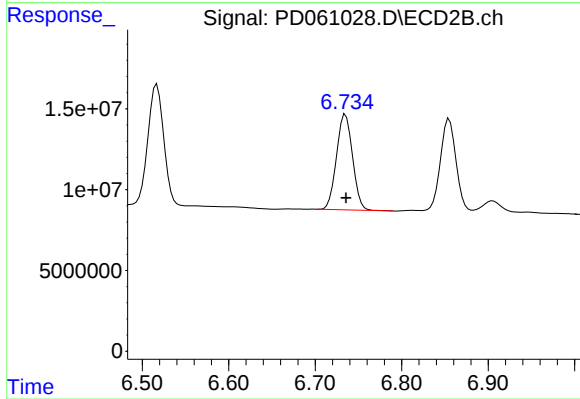


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 75656150
Conc: 10.10 ng/ml

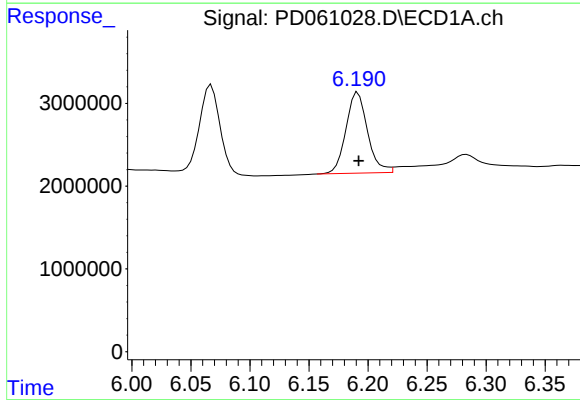


#16 4,4'-DDD

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 12414116
Conc: 10.33 ng/ml

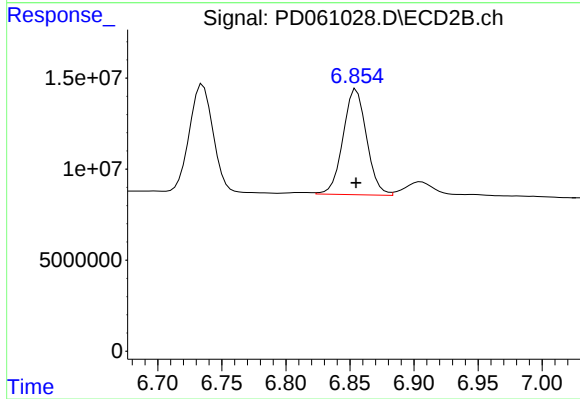

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 74048797
Conc: 10.09 ng/ml

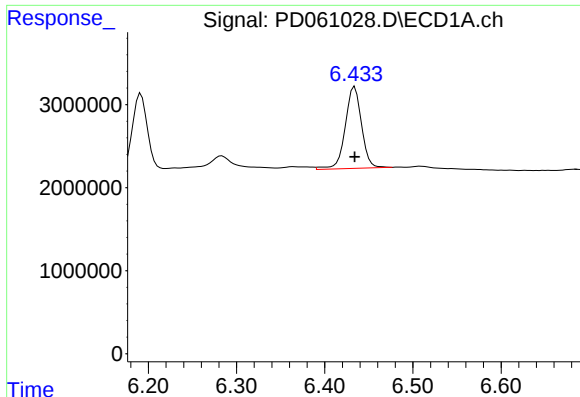

#17 4,4'-DDT


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 12650326
Conc: 9.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

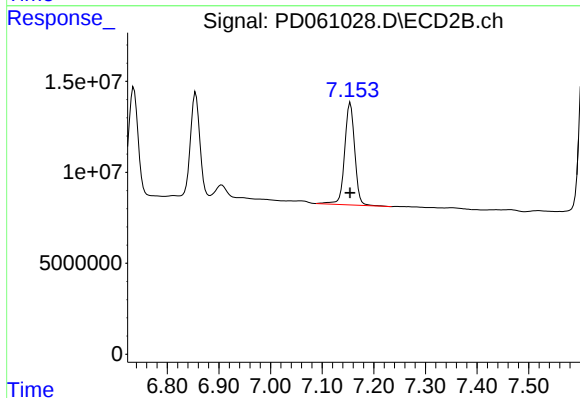


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 76593871
Conc: 10.19 ng/ml

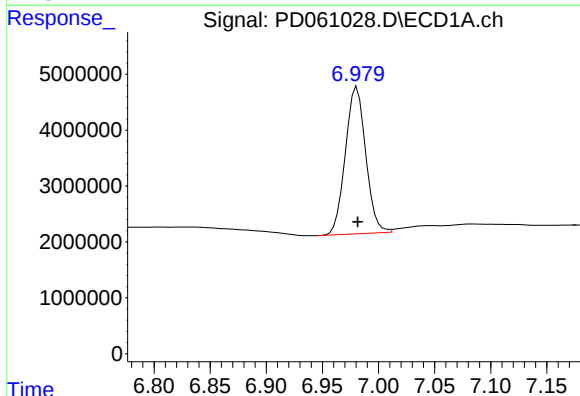


#20 Methoxychlor

R.T.: 6.981 min
Delta R.T.: 0.000 min
Response: 33158637
Conc: 51.75 ng/ml

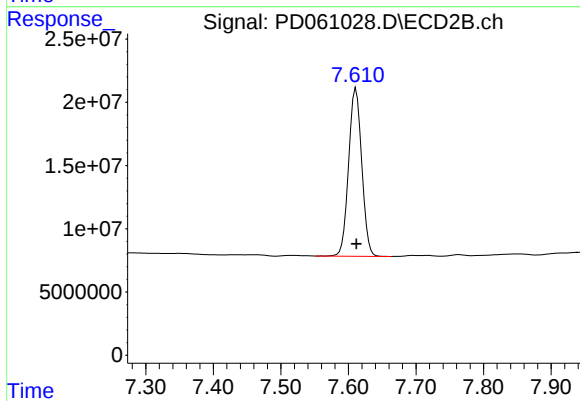

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 178402805
Conc: 53.06 ng/ml

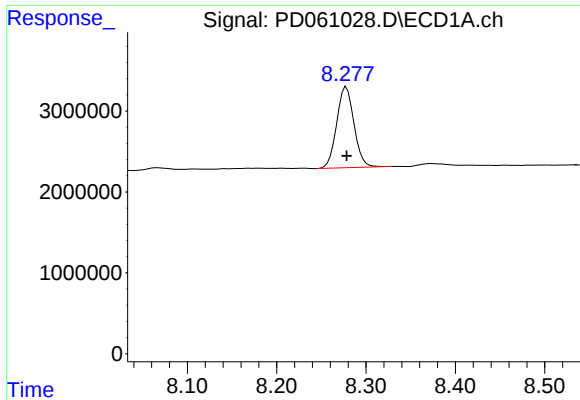

#27 Decachlorobiphenyl

R.T.: 8.278 min
Delta R.T.: 0.000 min
Response: 13505377
Conc: 10.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

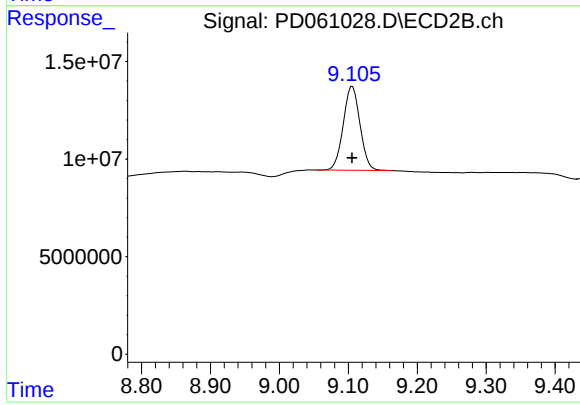

#27 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 72718342
Conc: 10.75 ng/ml