

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 14:56
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:57:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 16:53:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	10651301	75291479	10.269	10.118
27)	SA Decachlor...	8.279	9.105	26576134	143.6E6	20.712	21.225
Target Compounds							
2)	A alpha-BHC	3.937	4.411	15200690	114.1E6	10.047	9.987
3)	MA gamma-BHC...	4.223	4.697	15119498	105.2E6	10.263	9.997
4)	MA Heptachlor	4.528	5.208	15624620	109.7E6	10.153	10.057
9)	A Endosulfan I	5.565	6.260	13557453	98184653	10.187	10.975
13)	MA Dieldrin	5.810	6.517	29839702	194.4E6	19.849	20.343
14)	MA Endrin	6.068	6.736	25759371	154.5E6	20.638	20.624
16)	A 4,4'-DDD	6.192	6.856	24745119	149.2E6	20.586	20.329
17)	MA 4,4'-DDT	6.435	7.155	24428685	154.6E6	19.251	20.570
20)	A Methoxychlor	6.982	7.613	63765775	352.2E6	99.514	104.749

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 14:56
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:57:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 16:53:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

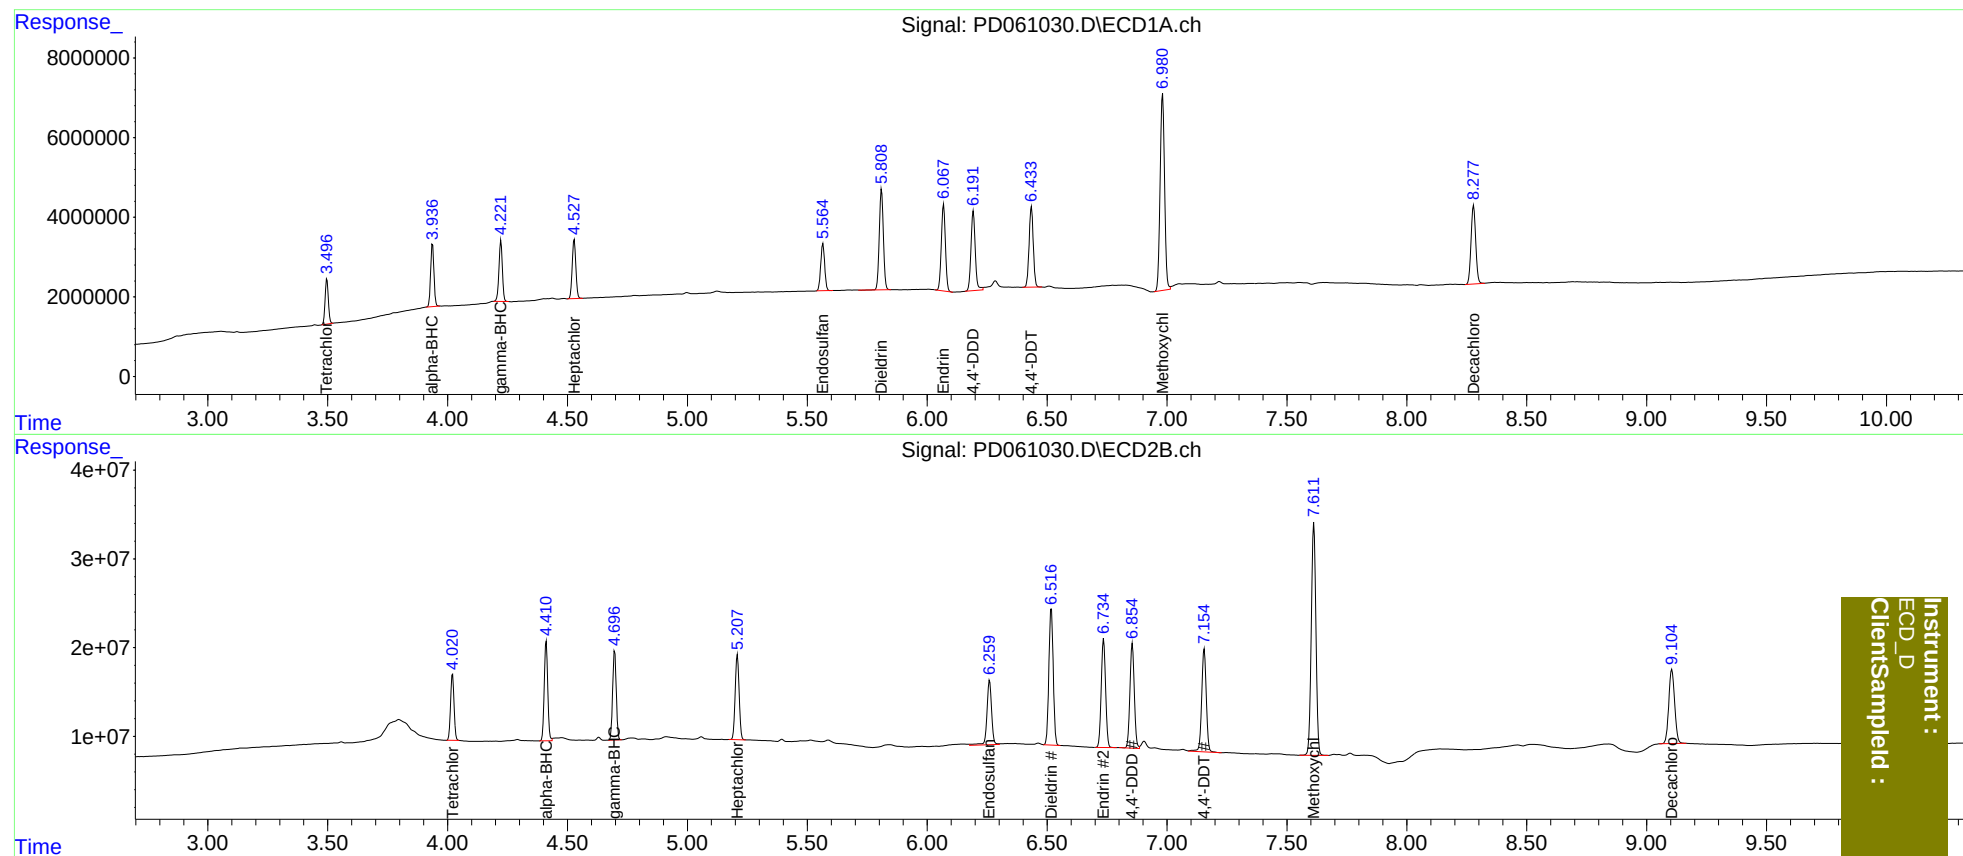


Instrument :
ECD_D
ClientSampled :

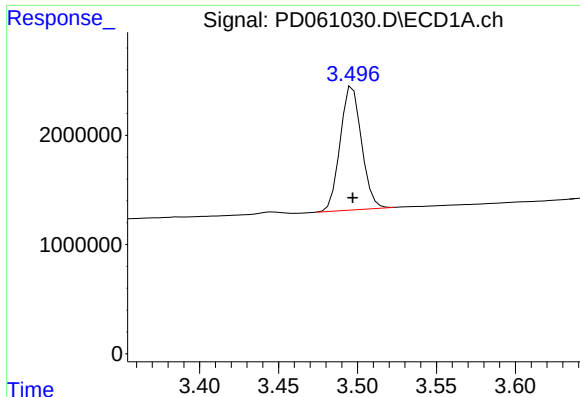

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 10651301
Conc: 10.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

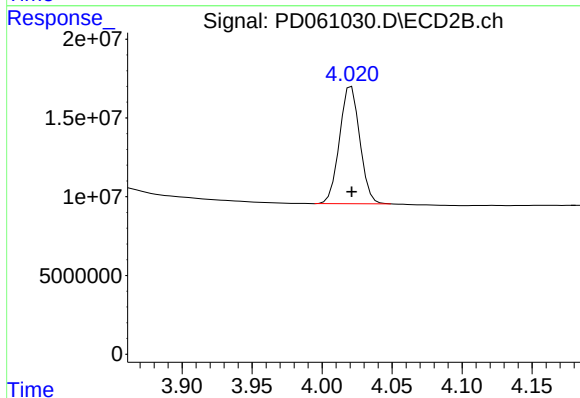


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 75291479
Conc: 10.12 ng/ml

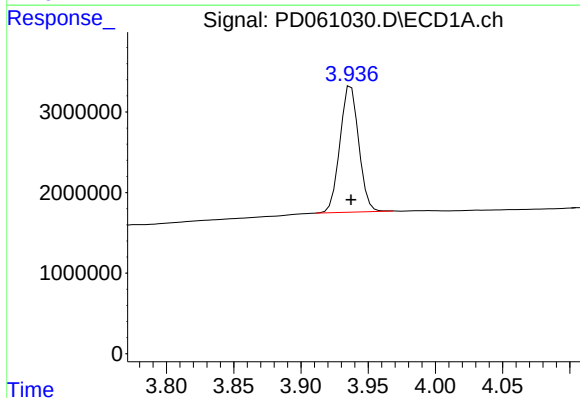


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 15200690
Conc: 10.05 ng/ml

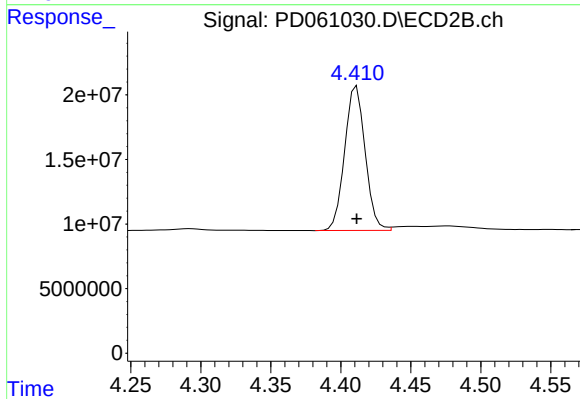

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 114064292
Conc: 9.99 ng/ml

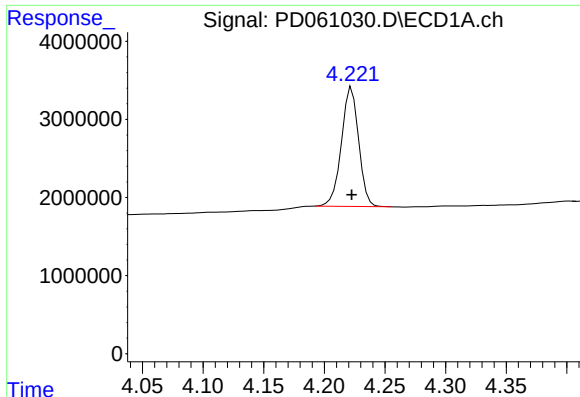

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 15119498
Conc: 10.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

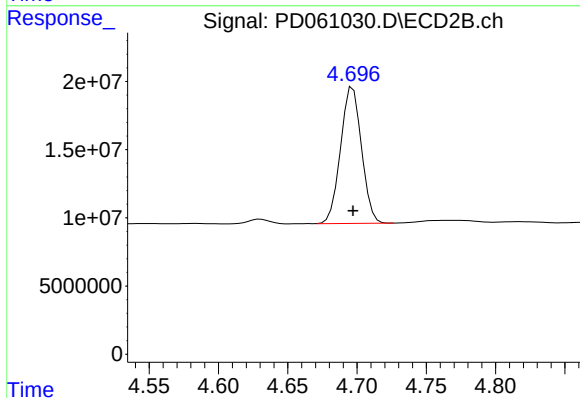


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 105192301
Conc: 10.00 ng/ml

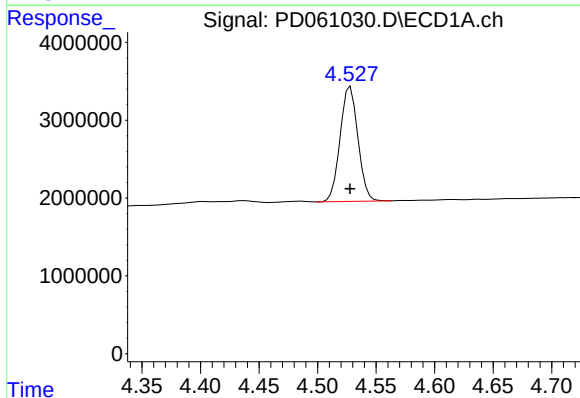


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 15624620
Conc: 10.15 ng/ml

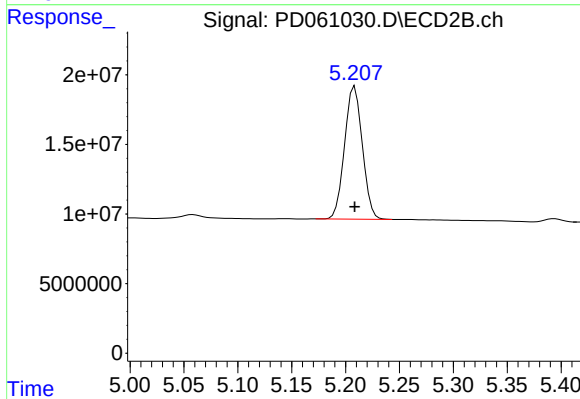

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 109677926
Conc: 10.06 ng/ml

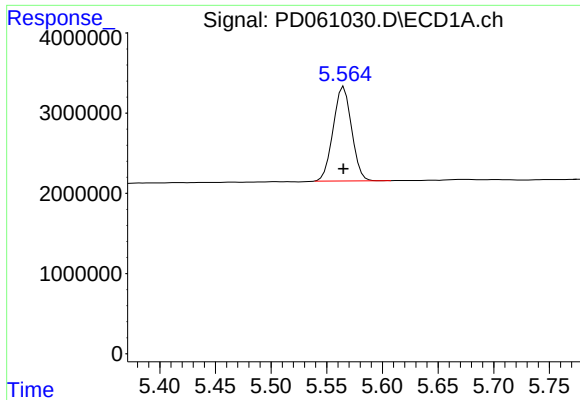

#9 Endosulfan I


R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 13557453
Conc: 10.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

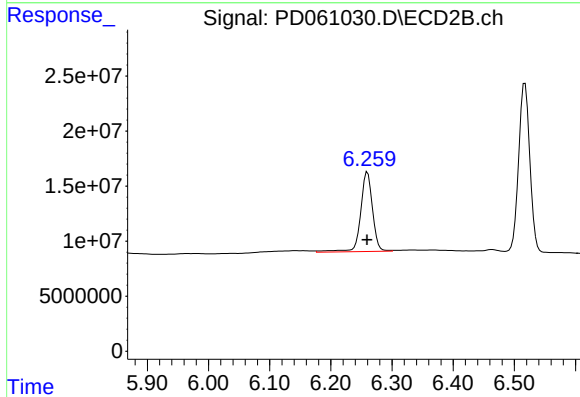


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 98184653
Conc: 10.97 ng/ml

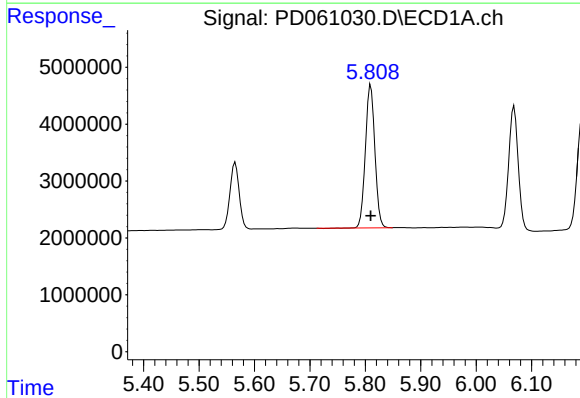


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 29839702
Conc: 19.85 ng/ml

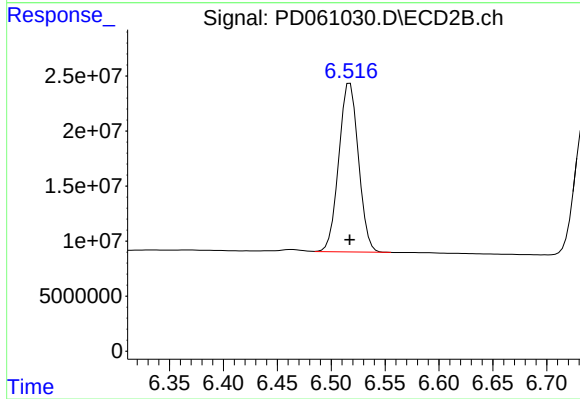

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 194443520
Conc: 20.34 ng/ml

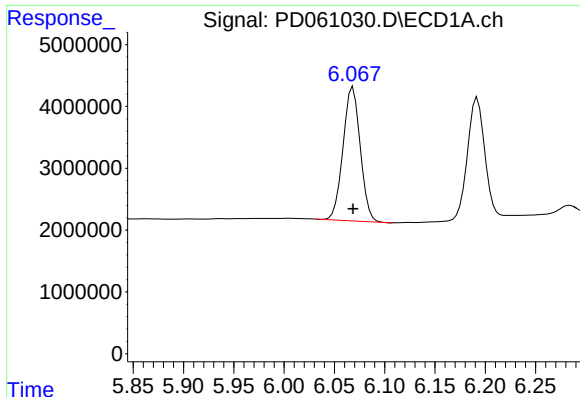

#14 Endrin


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 25759371
Conc: 20.64 ng/ml

Instrument :
ECD_D
ClientSampleId :

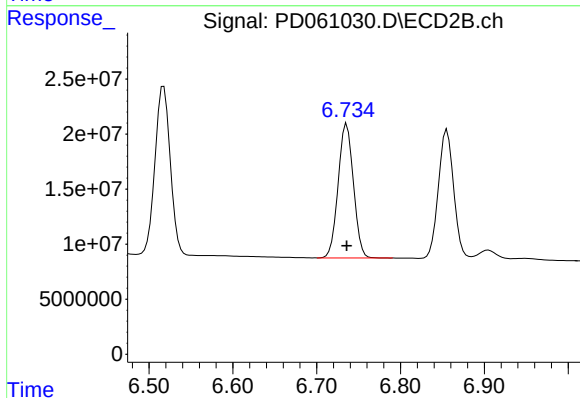


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 154462328
Conc: 20.62 ng/ml

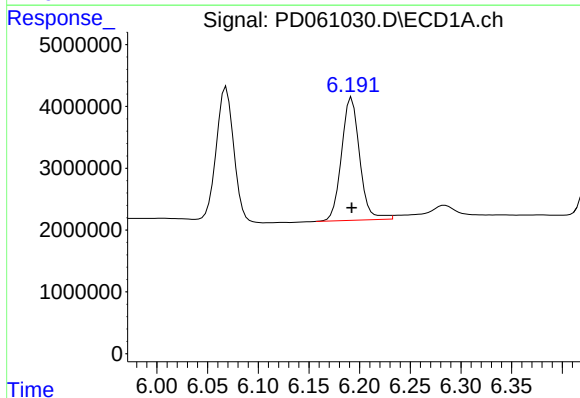


#16 4,4'-DDD

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 24745119
Conc: 20.59 ng/ml

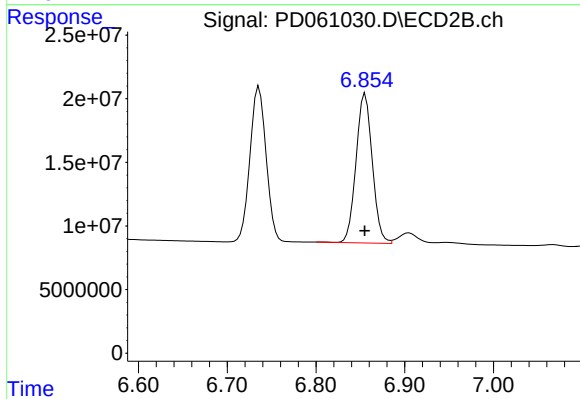

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 149240741
Conc: 20.33 ng/ml

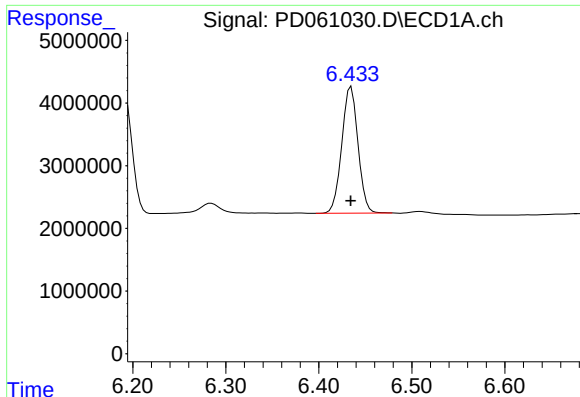

#17 4,4'-DDT


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 24428685
Conc: 19.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

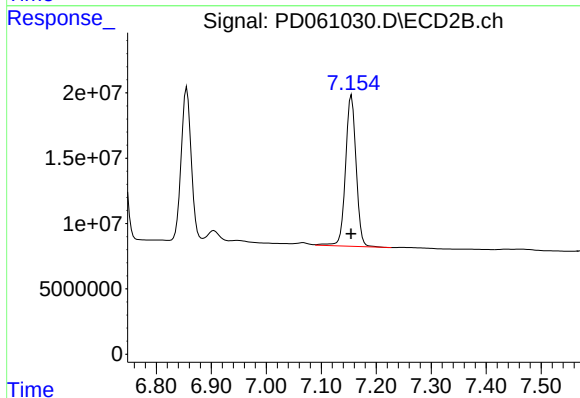


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 154611590
Conc: 20.57 ng/ml

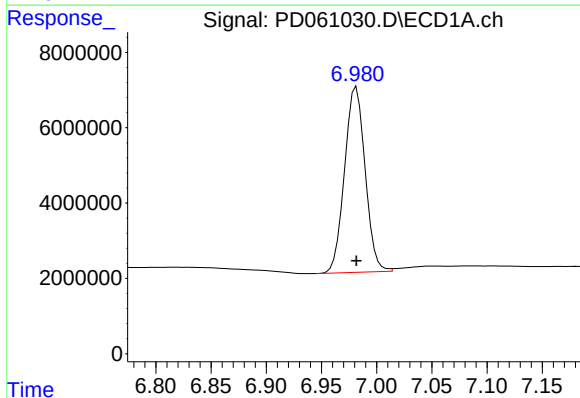


#20 Methoxychlor

R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 63765775
Conc: 99.51 ng/ml

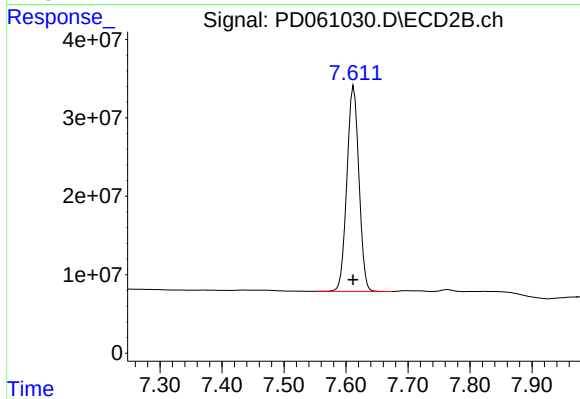

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 352183654
Conc: 104.75 ng/ml

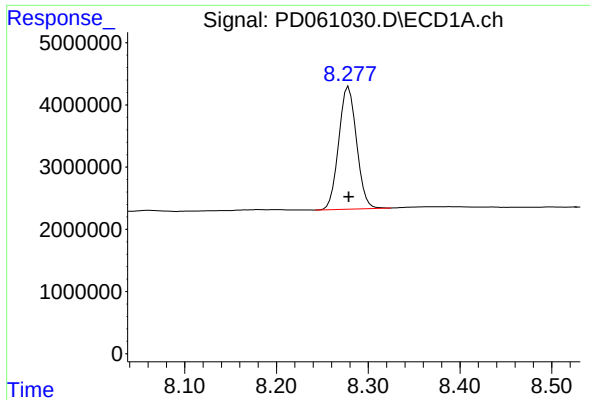

#27 Decachlorobiphenyl

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 26576134
Conc: 20.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

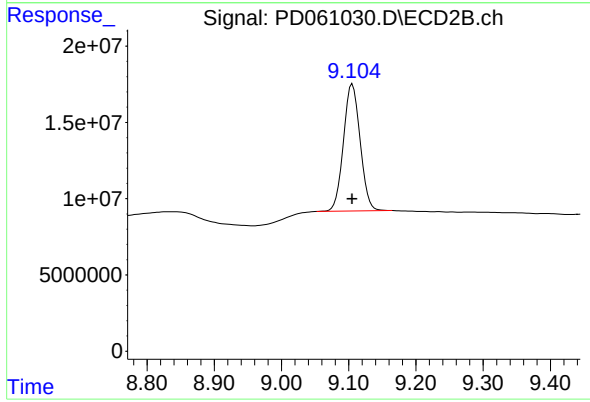

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 143582041
Conc: 21.23 ng/ml