

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 15:24
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:57:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 16:53:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	20744607	148.8E6	20.000	20.000
27)	SA Decachlor...	8.279	9.105	51324101	270.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.937	4.411	30257841	228.4E6	20.000	20.000
3)	MA gamma-BHC...	4.223	4.697	29465252	210.4E6	20.000	20.000
4)	MA Heptachlor	4.528	5.209	30778207	218.1E6	20.000	20.000
9)	A Endosulfan I	5.565	6.260	26616341	178.9E6	20.000	20.000
13)	MA Dieldrin	5.810	6.517	60132431	382.3E6	40.000	40.000
14)	MA Endrin	6.069	6.736	49926647	299.6E6	40.000	40.000
16)	A 4,4'-DDD	6.192	6.855	48082537	293.7E6	40.000	40.000
17)	MA 4,4'-DDT	6.434	7.154	50759275	300.7E6	40.000	40.000
20)	A Methoxychlor	6.982	7.612	128.2E6	672.4E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 15:24
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:57:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 16:53:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

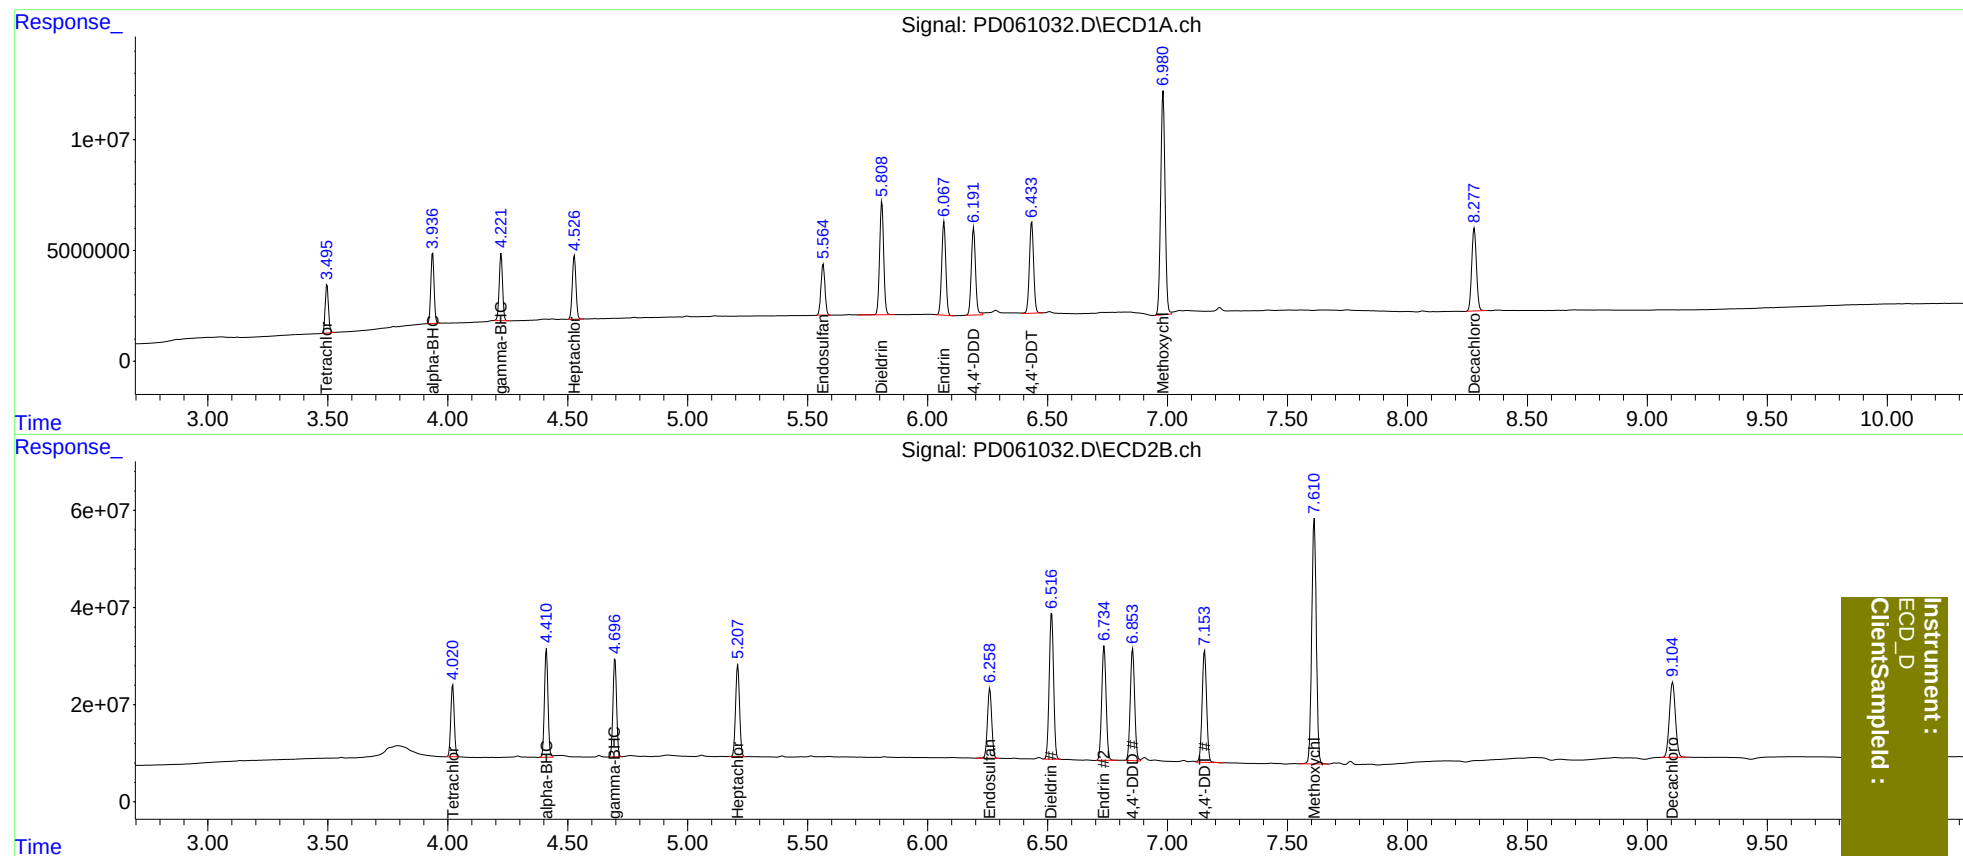


Instrument :
ECD_D
ClientSampled :

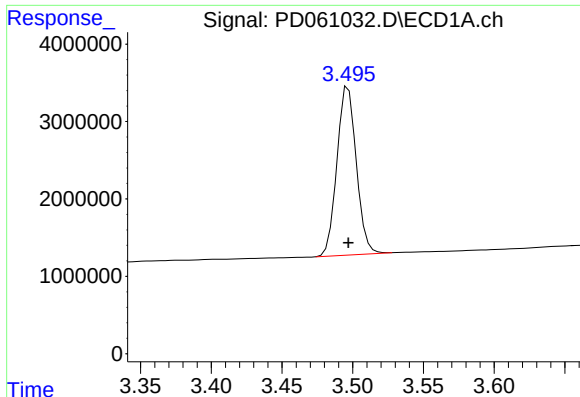

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 20744607
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

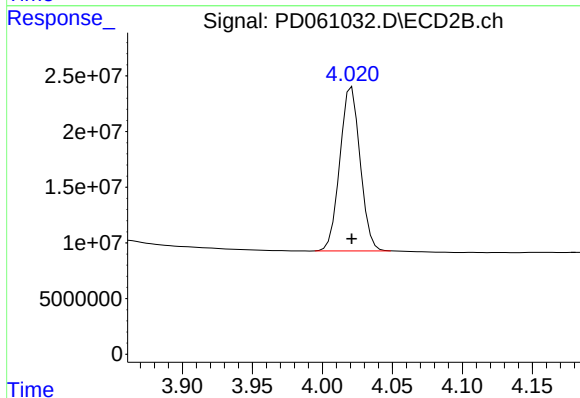


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 148830151
Conc: 20.00 ng/ml

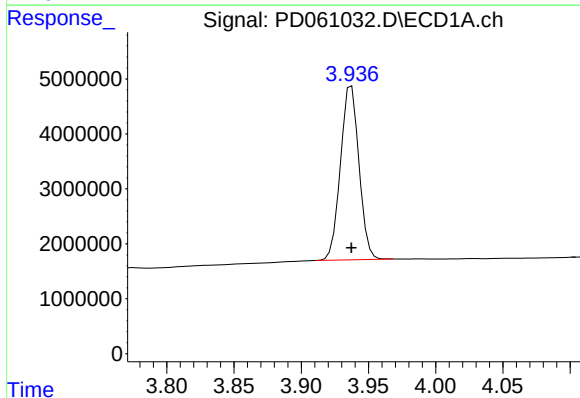


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 30257841
Conc: 20.00 ng/ml

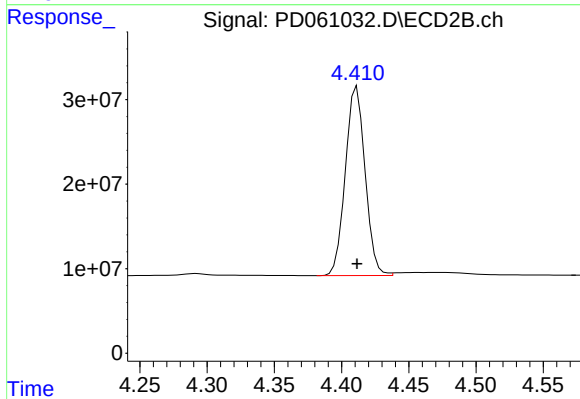

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 228426782
Conc: 20.00 ng/ml

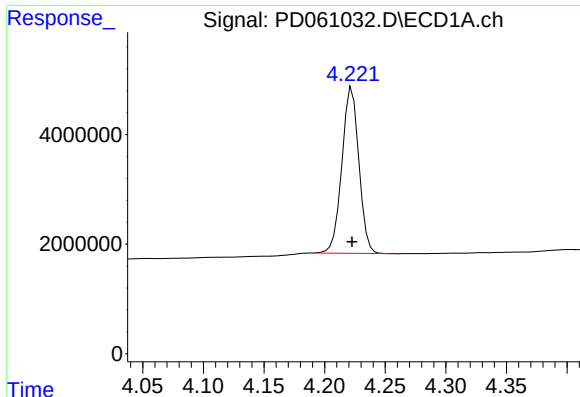

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 29465252
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

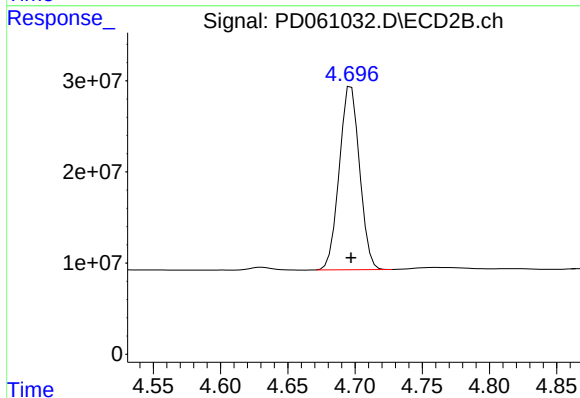


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 210448010
Conc: 20.00 ng/ml

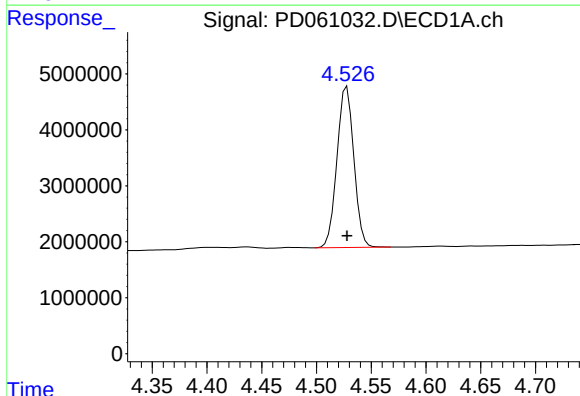


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 30778207
Conc: 20.00 ng/ml

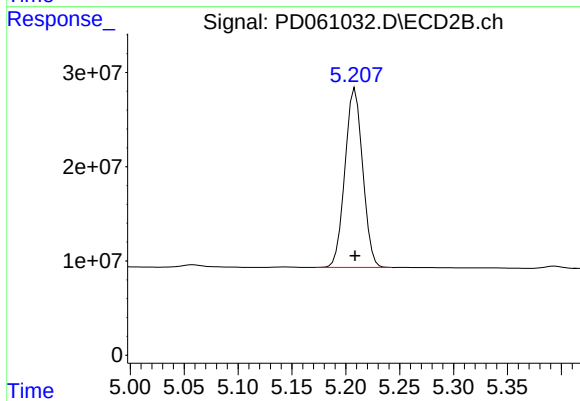

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 218108291
Conc: 20.00 ng/ml

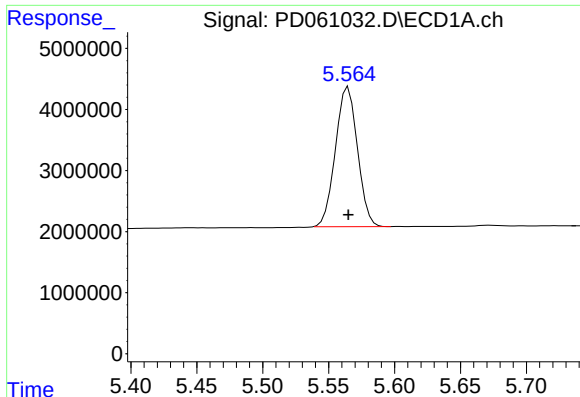

#9 Endosulfan I


R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 26616341
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

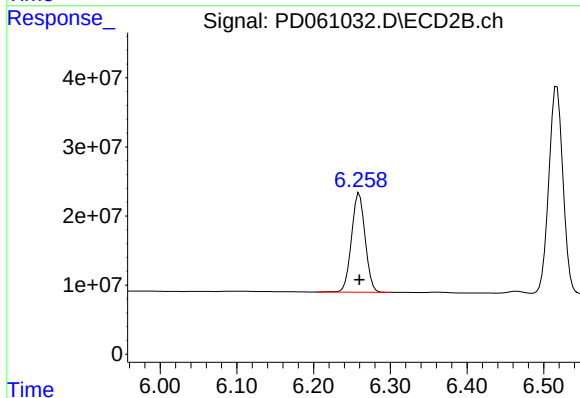


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 178927314
Conc: 20.00 ng/ml

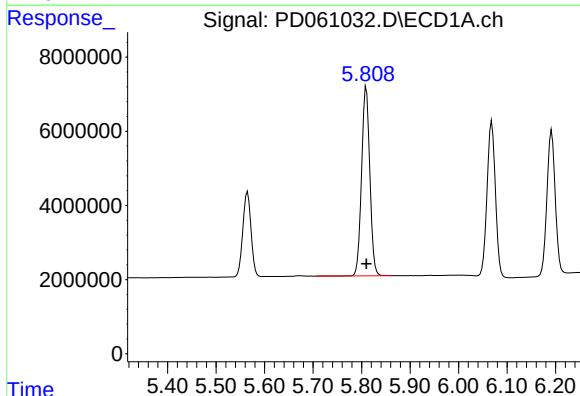


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 60132431
Conc: 40.00 ng/ml

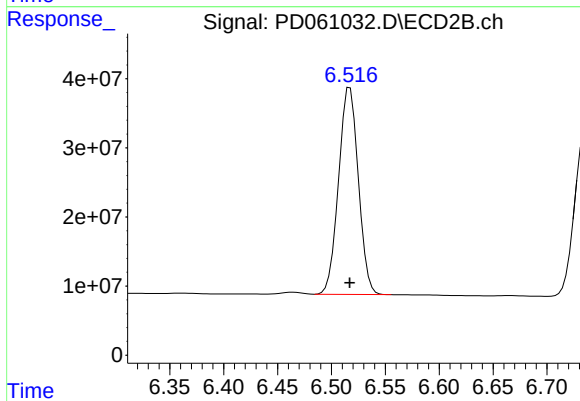

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 382327611
Conc: 40.00 ng/ml

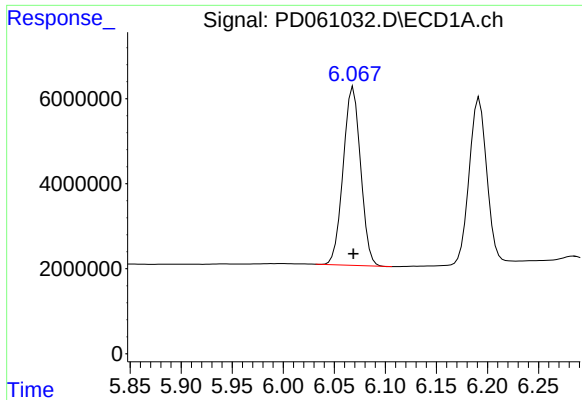

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 49926647
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

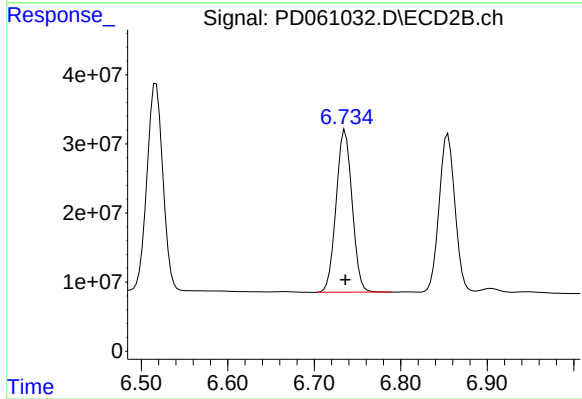


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 299584946
Conc: 40.00 ng/ml

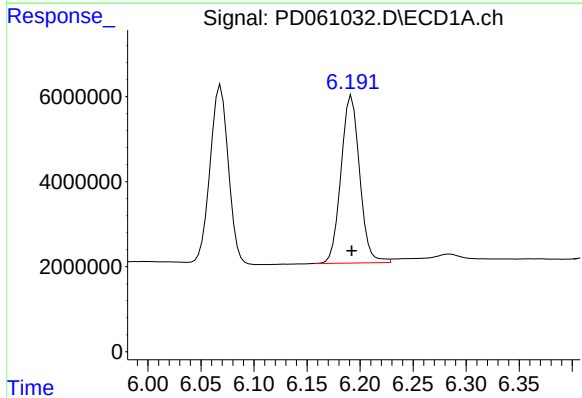


#16 4,4'-DDD

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 48082537
Conc: 40.00 ng/ml

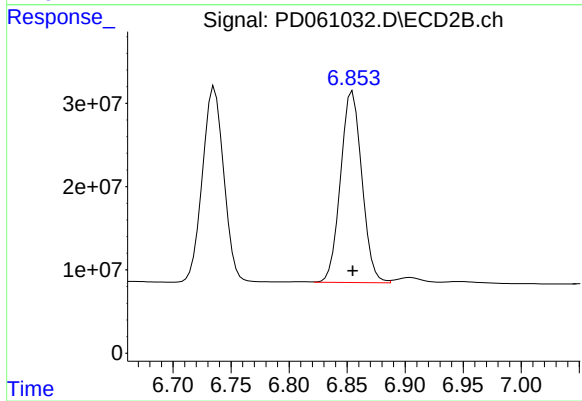

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 293656518
Conc: 40.00 ng/ml

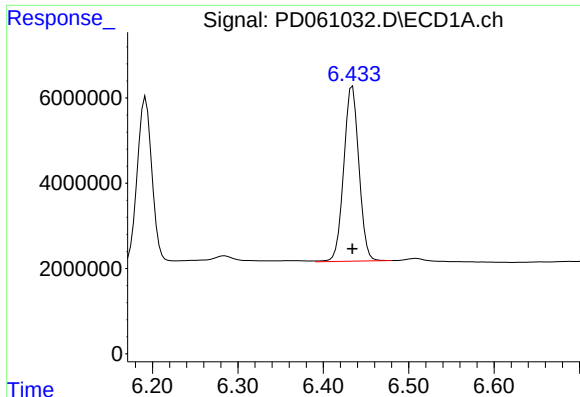

#17 4,4'-DDT


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 50759275
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

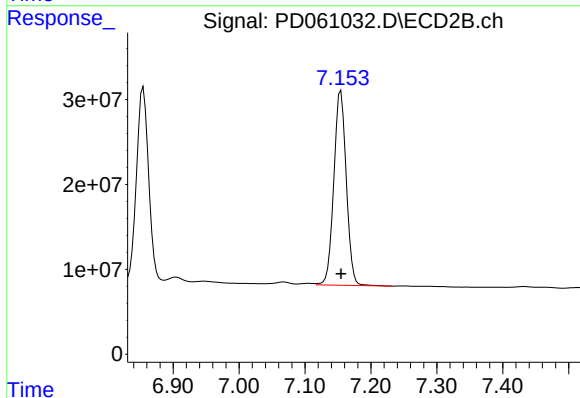


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 300659105
Conc: 40.00 ng/ml

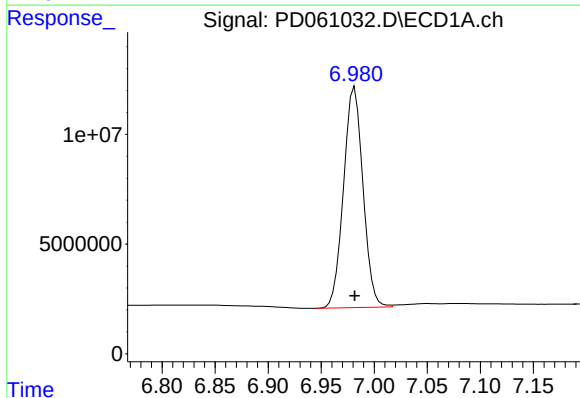


#20 Methoxychlor

R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 128153949
Conc: 200.00 ng/ml

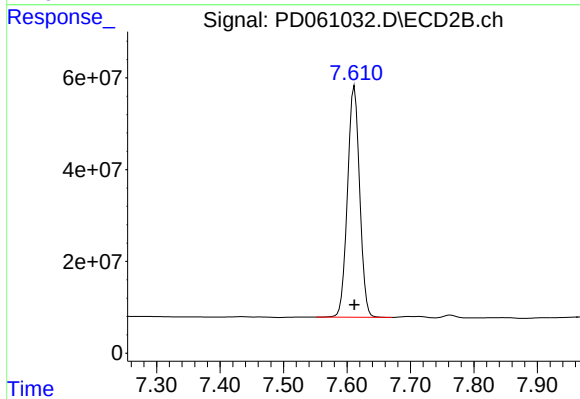

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 672432685
Conc: 200.00 ng/ml

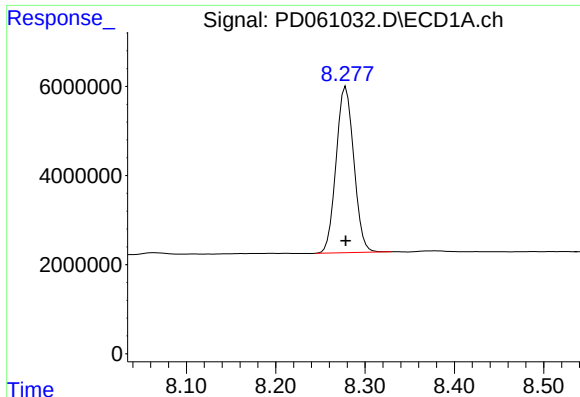

#27 Decachlorobiphenyl

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 51324101
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

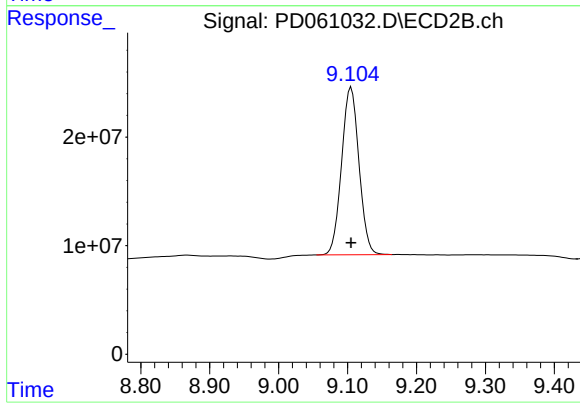

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 270585981
Conc: 40.00 ng/ml