

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 15:52
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:57:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 16:53:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	38926885	278.4E6	37.530	37.418
27)	SA Decachlor...	8.279	9.104	97008364	526.4E6	75.605	77.819
Target Compounds							
2)	A alpha-BHC	3.938	4.412	58952546	441.1E6	38.967	38.622
3)	MA gamma-BHC...	4.223	4.698	56287632	401.3E6	38.206	38.135
4)	MA Heptachlor	4.528	5.209	59288464	412.9E6	38.526	37.858
9)	A Endosulfan I	5.566	6.260	50783452	336.7E6	38.160	37.636
13)	MA Dieldrin	5.810	6.518	116.9E6	730.1E6	77.777	76.381
14)	MA Endrin	6.069	6.736	97883493	584.8E6	78.422	78.079
16)	A 4,4'-DDD	6.193	6.855	93021016	566.9E6	77.384	77.216
17)	MA 4,4'-DDT	6.435	7.155	99630791	585.3E6	78.512	77.872
20)	A Methoxychlor	6.981	7.612	242.6E6	1270.3E6	378.633	377.818

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 15:52
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:57:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 16:53:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

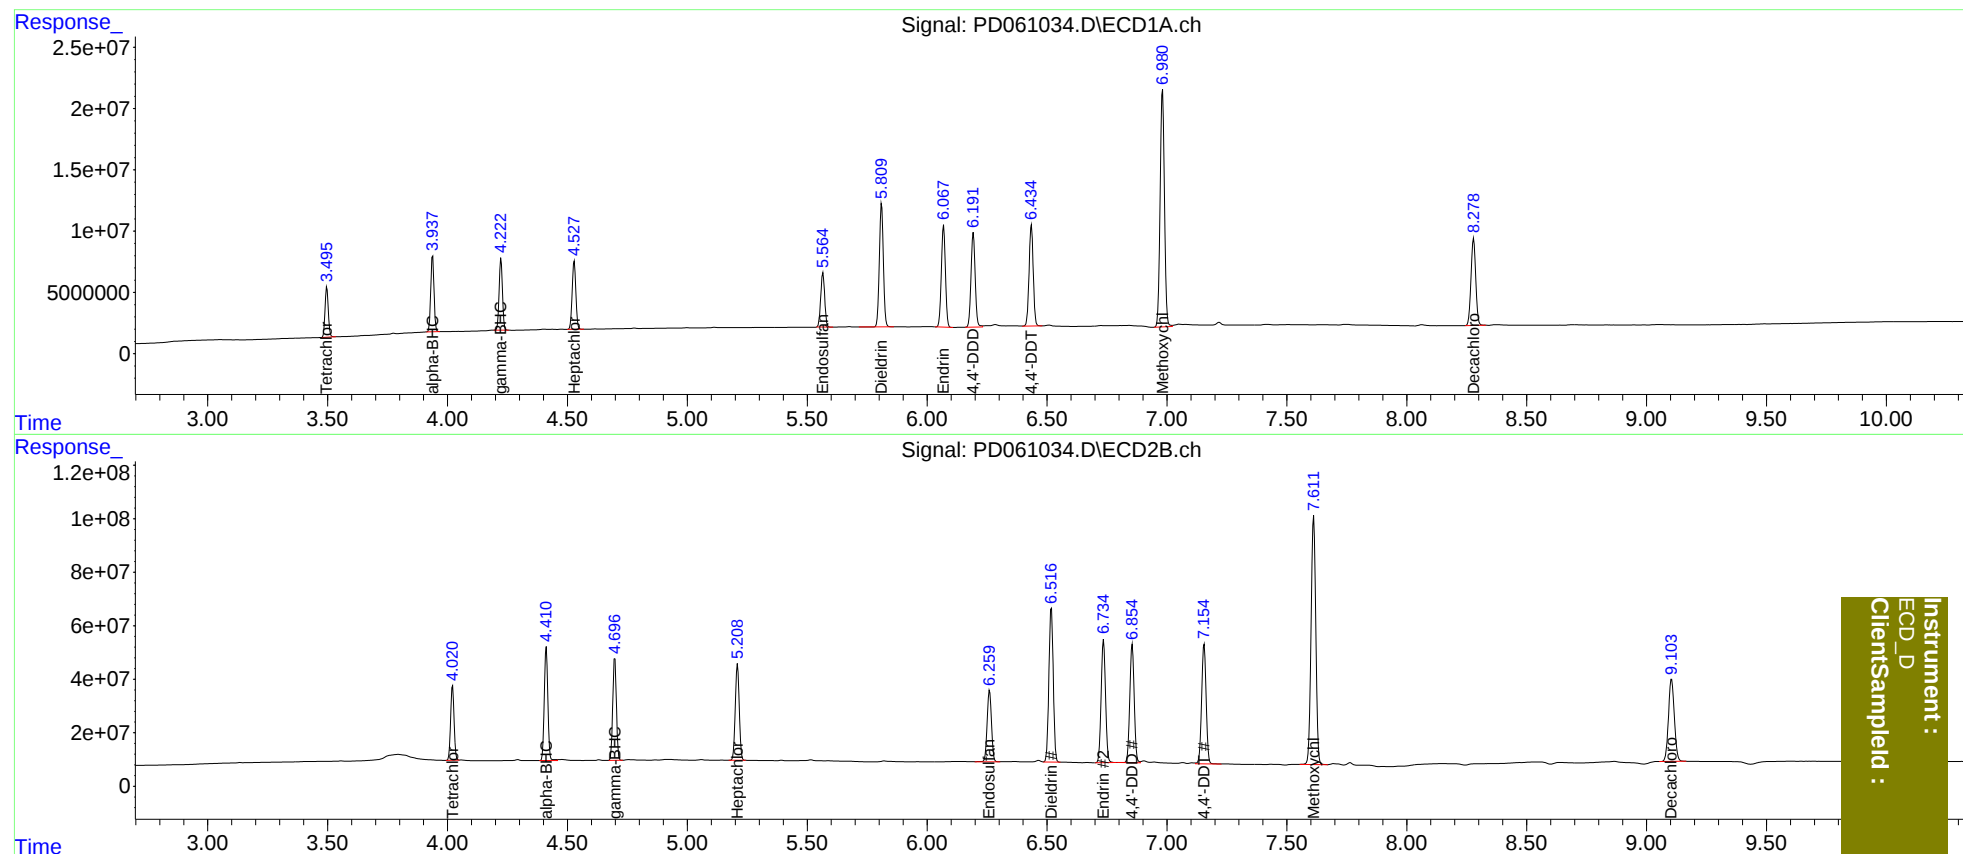


Instrument :
ECD_D
ClientSampled :

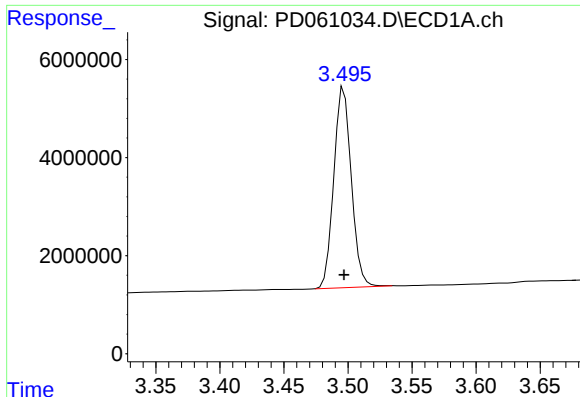

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 38926885
Conc: 37.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

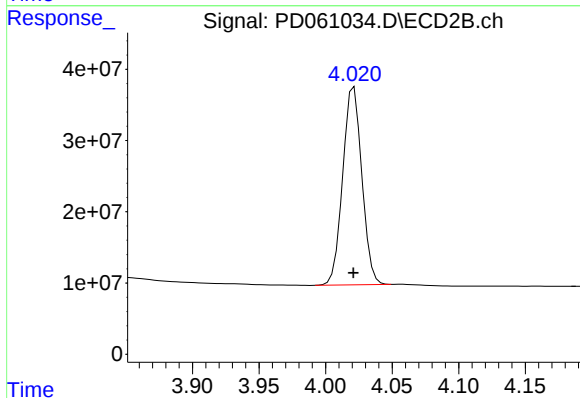


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 278447864
Conc: 37.42 ng/ml

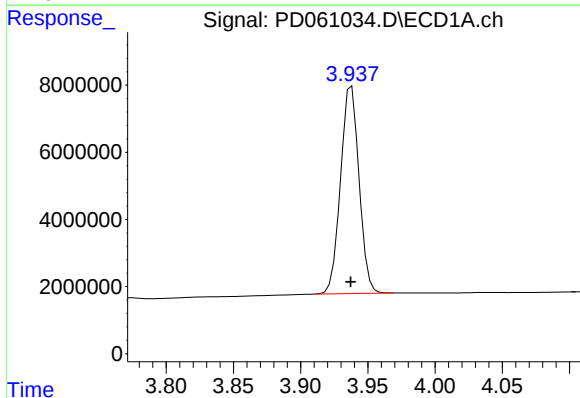


#2 alpha-BHC

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 58952546
Conc: 38.97 ng/ml

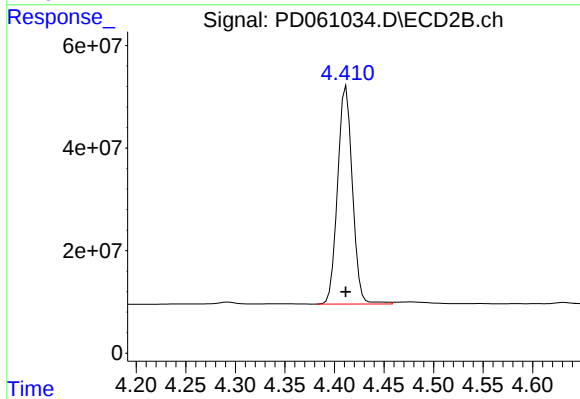

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.000 min
Response: 441110882
Conc: 38.62 ng/ml

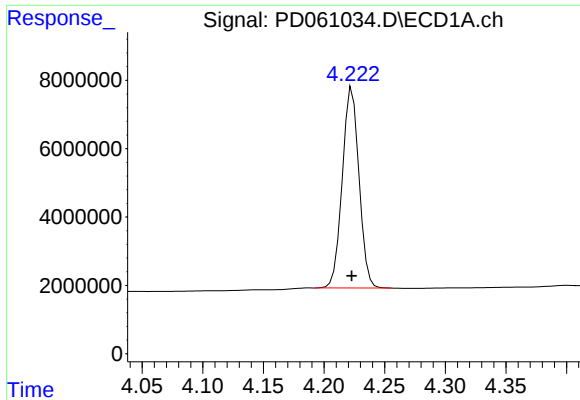

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 56287632
Conc: 38.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

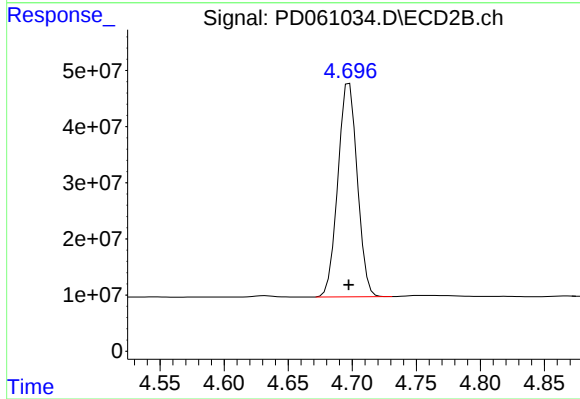


#3 gamma-BHC (Lindane)

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 401270108
Conc: 38.13 ng/ml

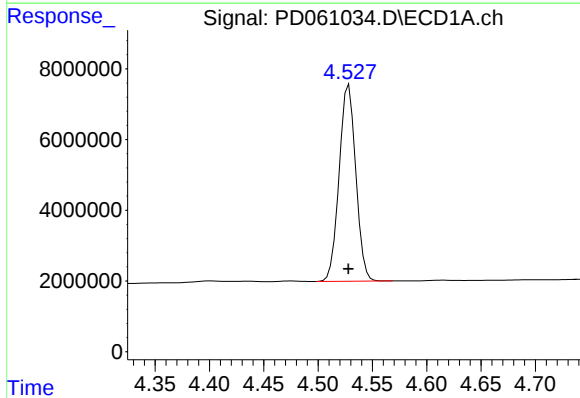


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 59288464
Conc: 38.53 ng/ml

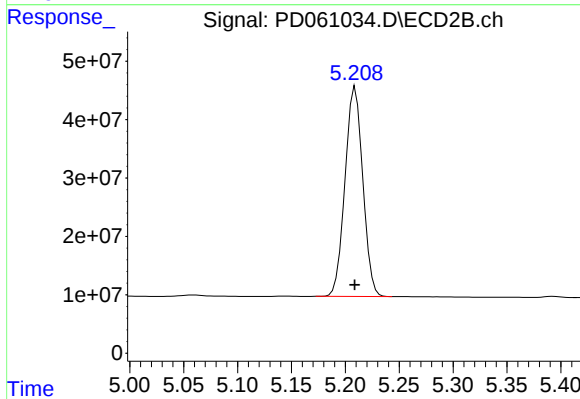

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 412862624
Conc: 37.86 ng/ml

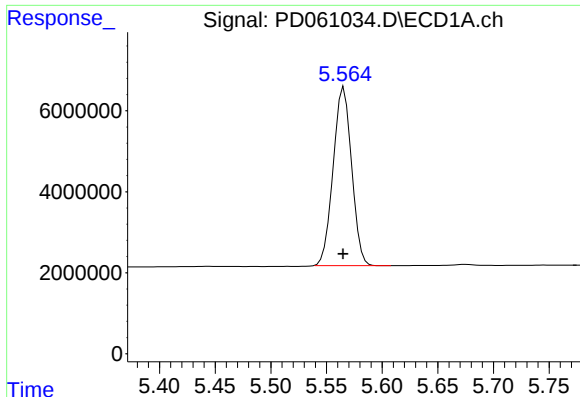

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 50783452
Conc: 38.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

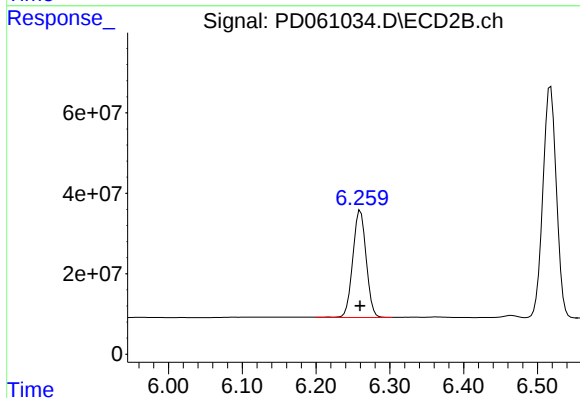


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 336705368
Conc: 37.64 ng/ml

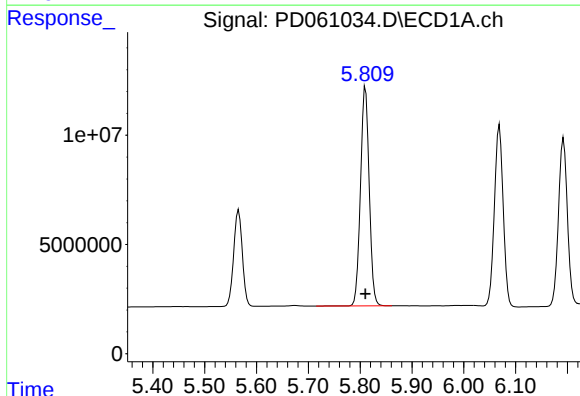


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 116923093
Conc: 77.78 ng/ml

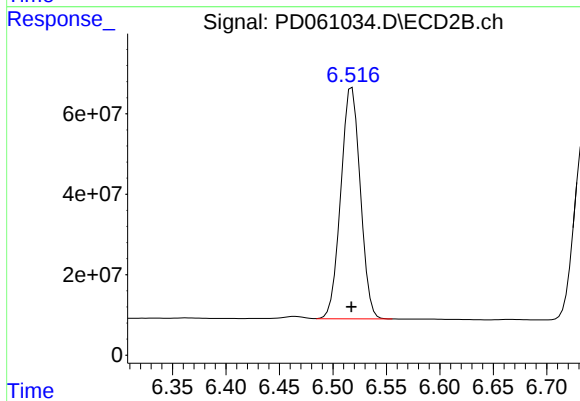

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 730065933
Conc: 76.38 ng/ml

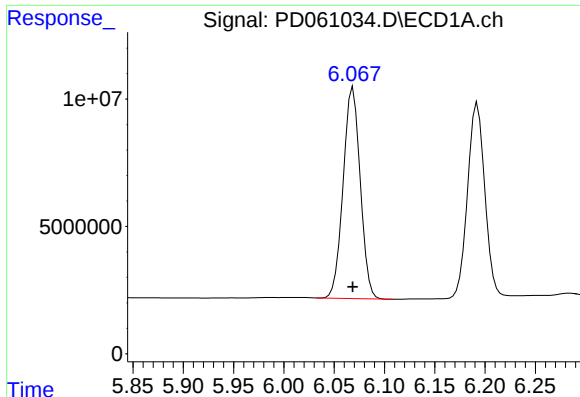

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 97883493
Conc: 78.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

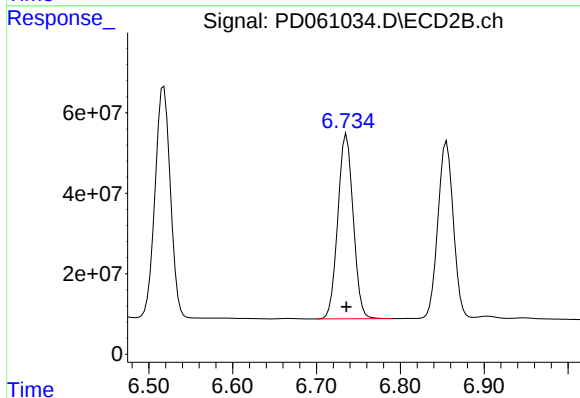


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 584781209
Conc: 78.08 ng/ml

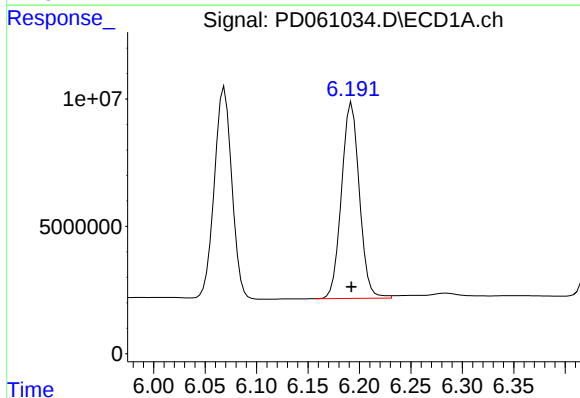


#16 4,4'-DDD

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 93021016
Conc: 77.38 ng/ml

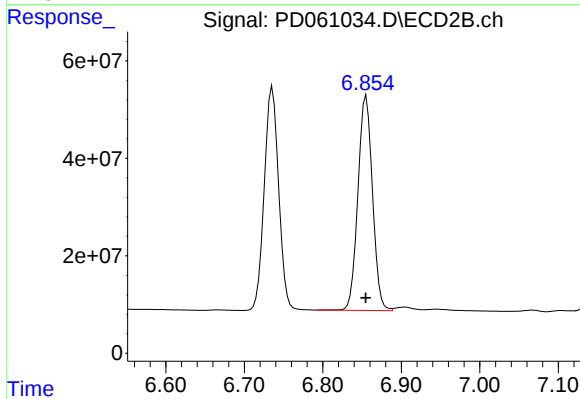

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 566875837
Conc: 77.22 ng/ml

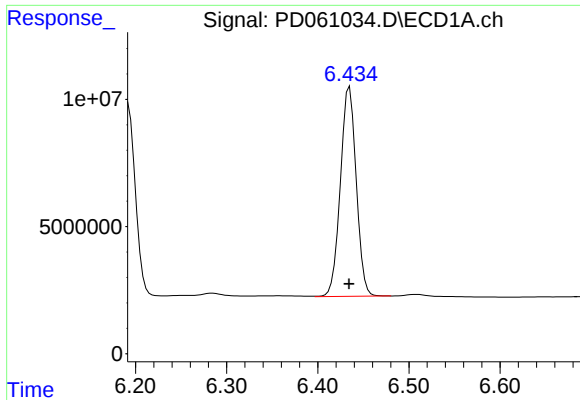

#17 4,4'-DDT


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 99630791
Conc: 78.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

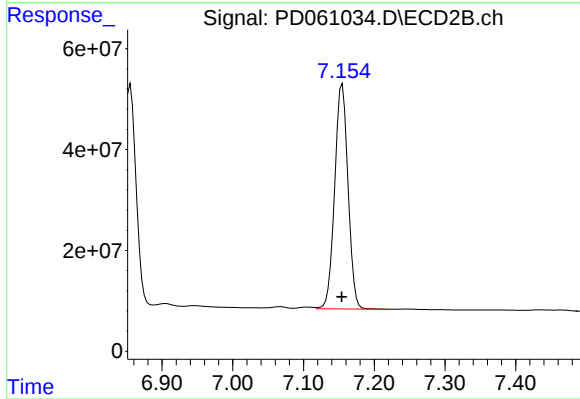


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 585320952
Conc: 77.87 ng/ml

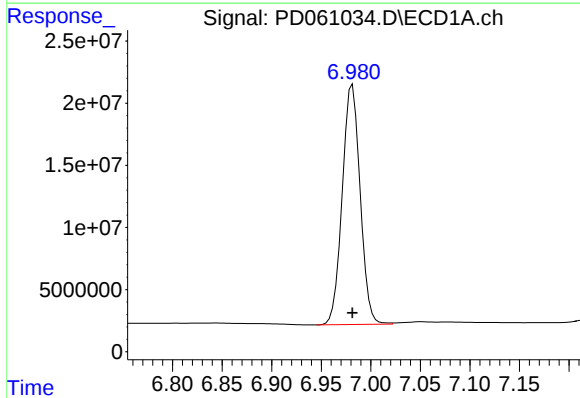


#20 Methoxychlor

R.T.: 6.981 min
Delta R.T.: 0.000 min
Response: 242616789
Conc: 378.63 ng/ml

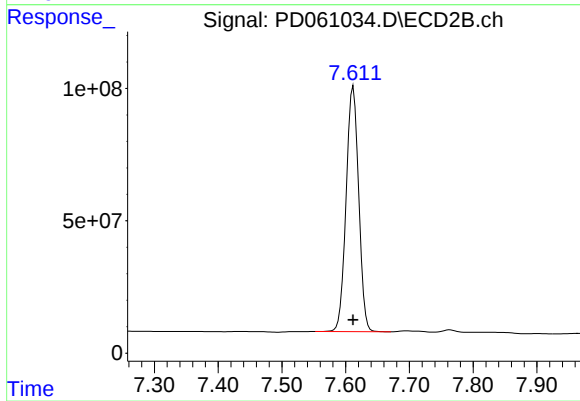

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 1270286600
Conc: 377.82 ng/ml

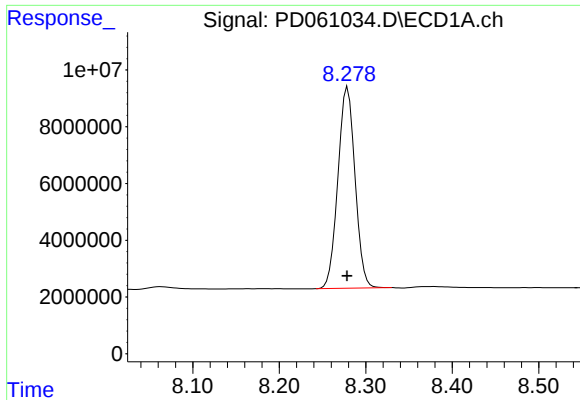

#27 Decachlorobiphenyl

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 97008364
Conc: 75.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

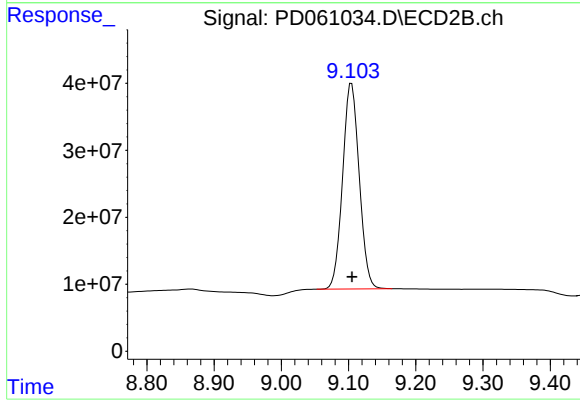

#27 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 526415181
Conc: 77.82 ng/ml