

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 16:20
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 16:58:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 25 16:53:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	73551644	515.7E6	70.912	69.304
27)	SA Decachlor...	8.279	9.105	180.0E6	985.4E6	140.297	145.666
Target Compounds							
2)	A alpha-BHC	3.937	4.411	115.0E6	826.6E6	75.982	72.377
3)	MA gamma-BHC...	4.223	4.696	108.5E6	755.0E6	73.647	71.756
4)	MA Heptachlor	4.528	5.208	114.0E6	769.6E6	74.073	70.570
9)	A Endosulfan I	5.566	6.260	96107788	634.3E6	72.217	70.899
13)	MA Dieldrin	5.810	6.517	227.1E6	1370.4E6	151.066	143.374
14)	MA Endrin	6.069	6.736	188.7E6	1095.6E6	151.189	146.282
16)	A 4,4'-DDD	6.192	6.855	178.1E6	1059.8E6	148.192	144.357
17)	MA 4,4'-DDT	6.434	7.154	192.5E6	1109.8E6	151.729	147.655
20)	A Methoxychlor	6.981	7.612	458.3E6	2300.8E6	715.164	684.323

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 16:20
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 16:58:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jan 25 16:53:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

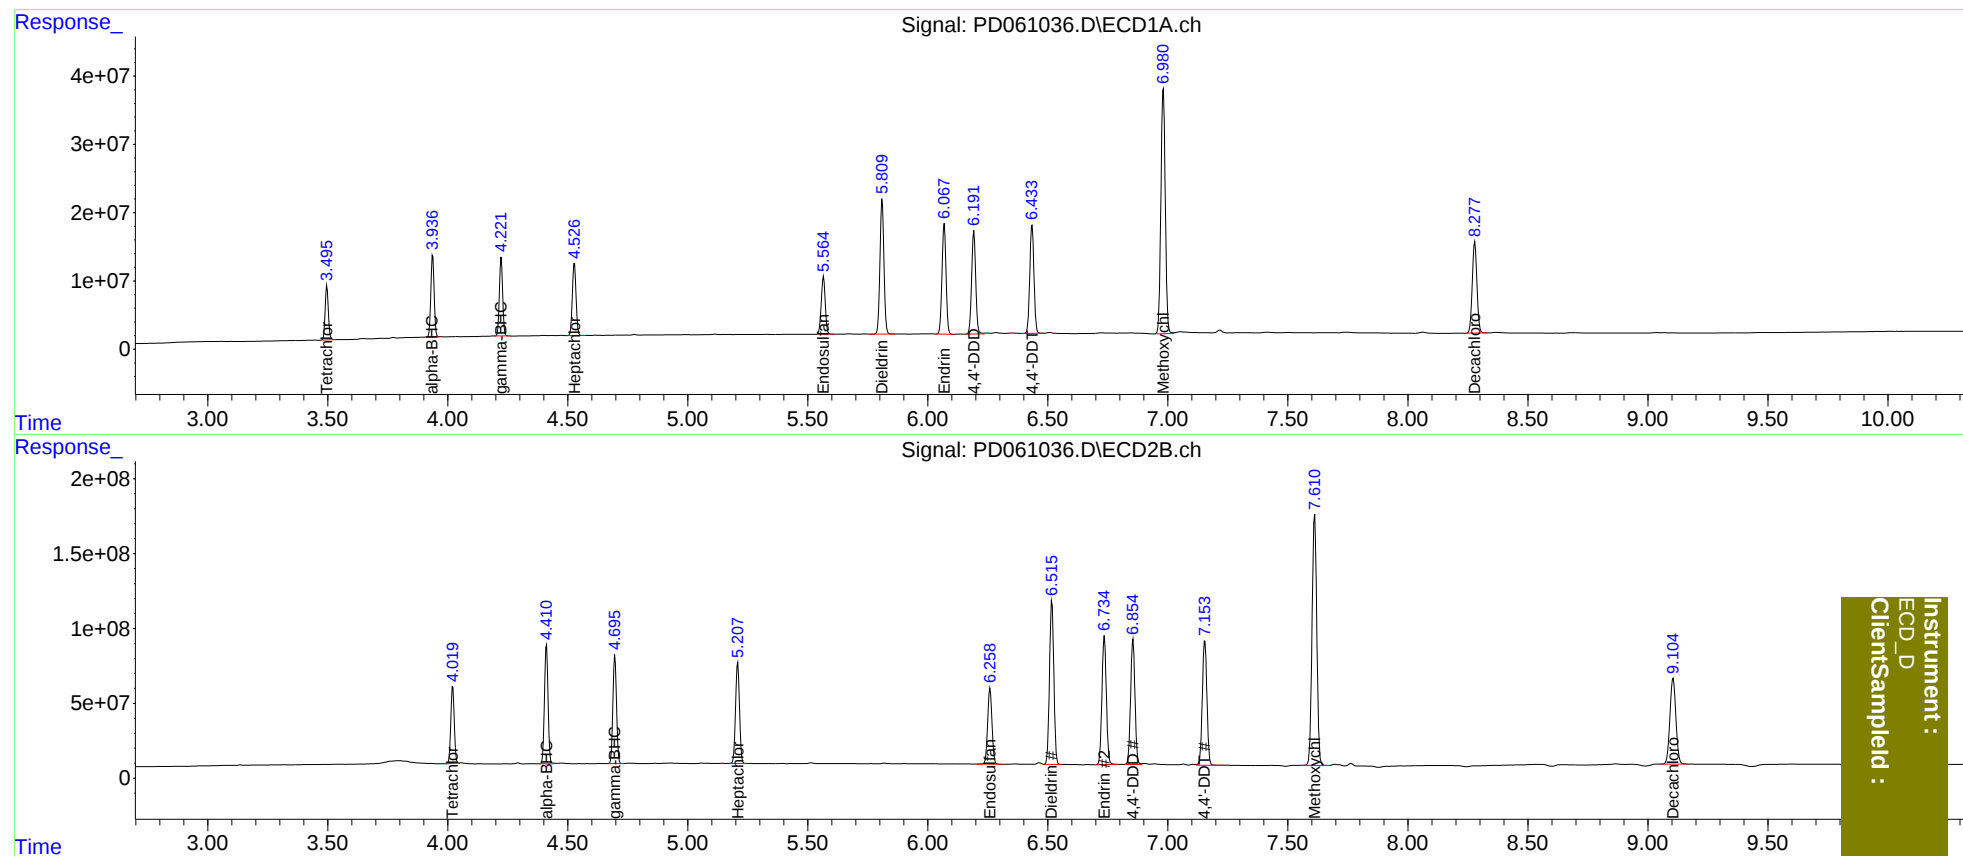


Instrument :
ECD_D
ClientSampled :

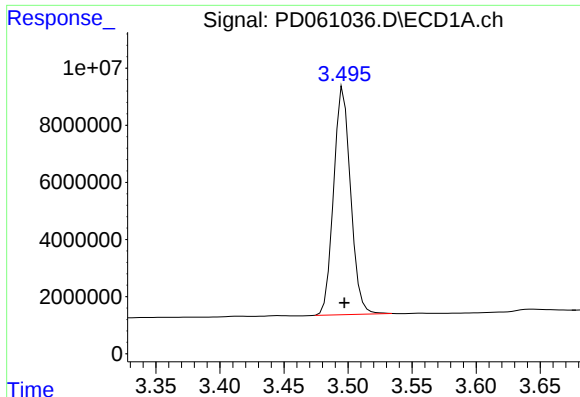

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 73551644
Conc: 70.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

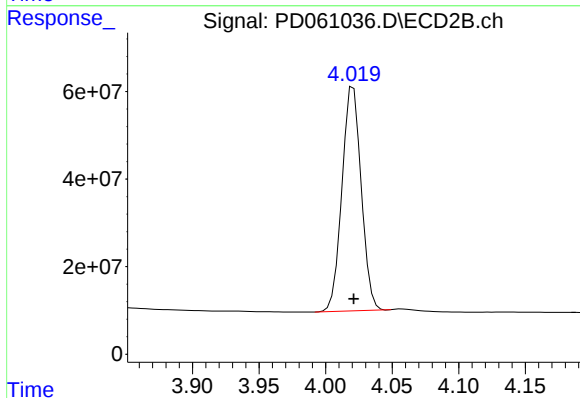


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 515725605
Conc: 69.30 ng/ml

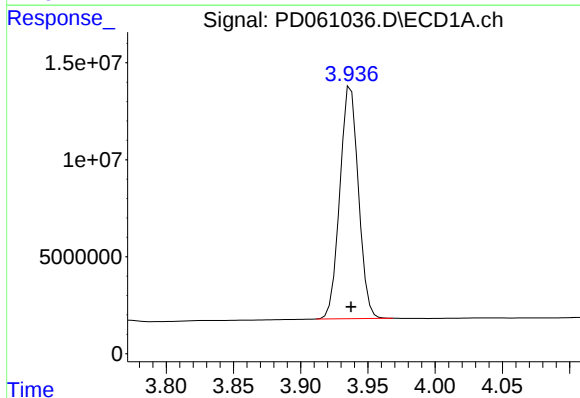


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 114952571
Conc: 75.98 ng/ml

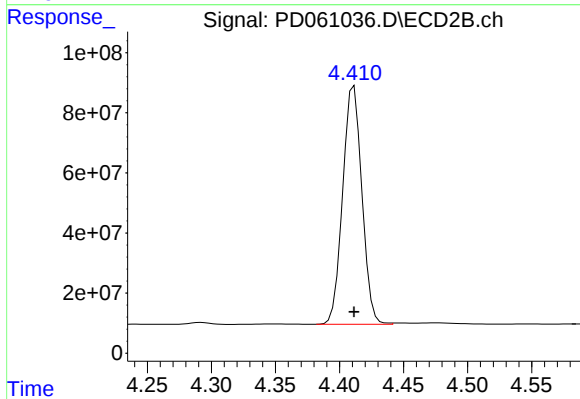

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 826639775
Conc: 72.38 ng/ml

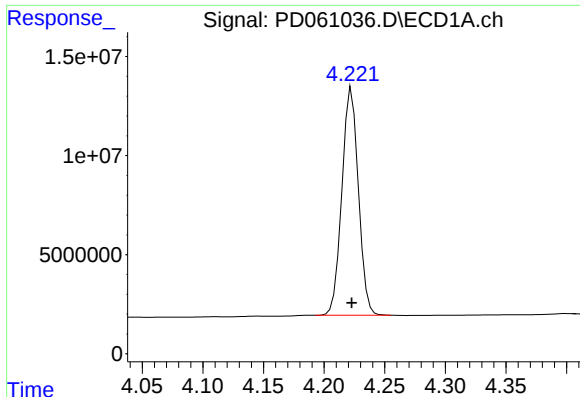

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 108501959
Conc: 73.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

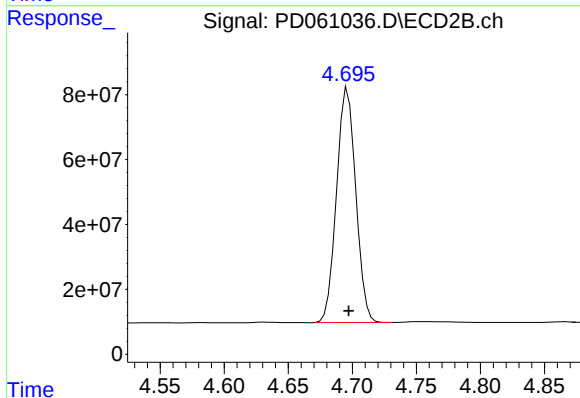


#3 gamma-BHC (Lindane)

R.T.: 4.696 min
Delta R.T.: 0.000 min
Response: 755047046
Conc: 71.76 ng/ml

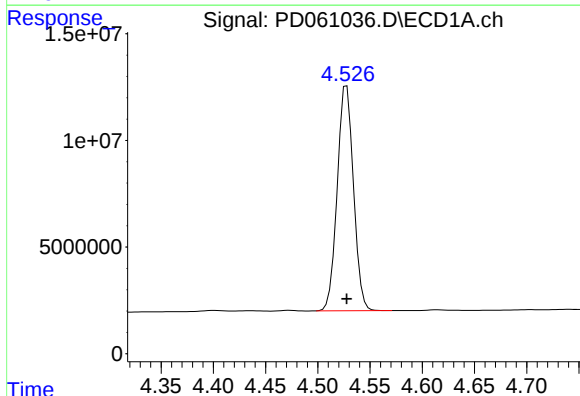


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 113992285
Conc: 74.07 ng/ml

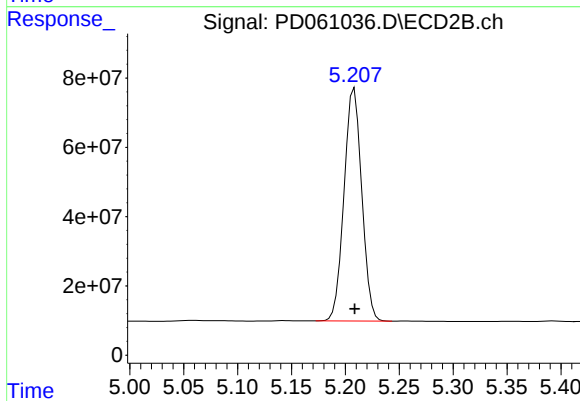

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 769593686
Conc: 70.57 ng/ml

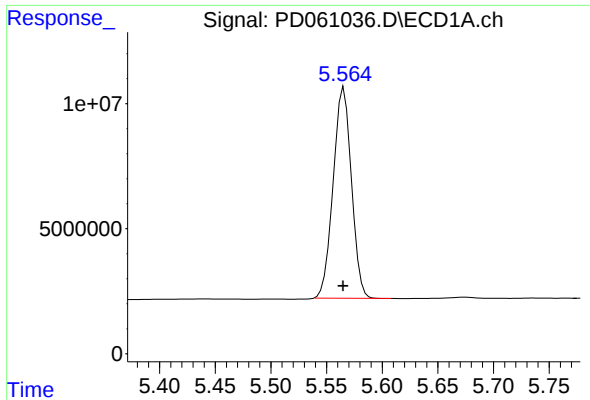

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 96107788
Conc: 72.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

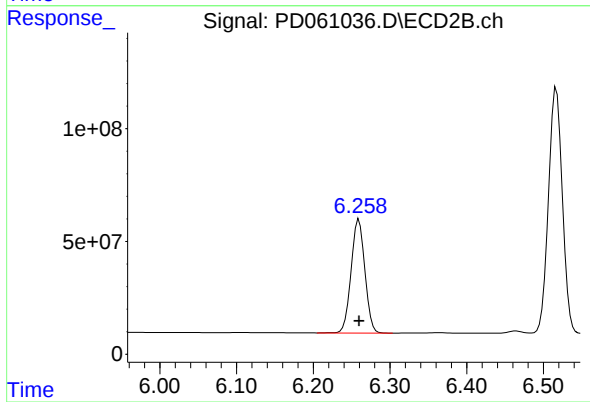


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 634290255
Conc: 70.90 ng/ml

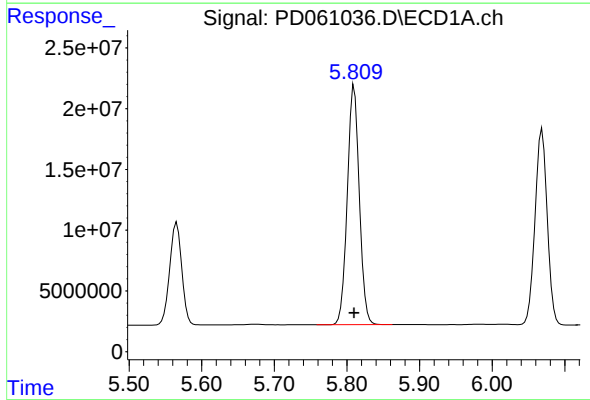


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 227098608
Conc: 151.07 ng/ml

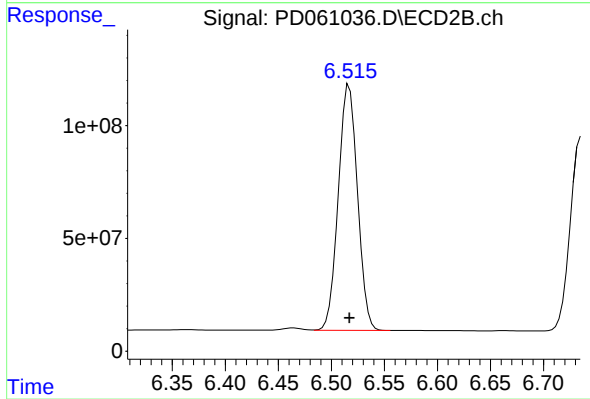

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 1370396790
Conc: 143.37 ng/ml

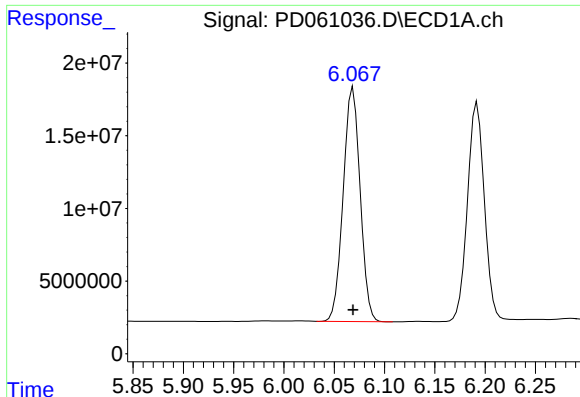

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 188709457
Conc: 151.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

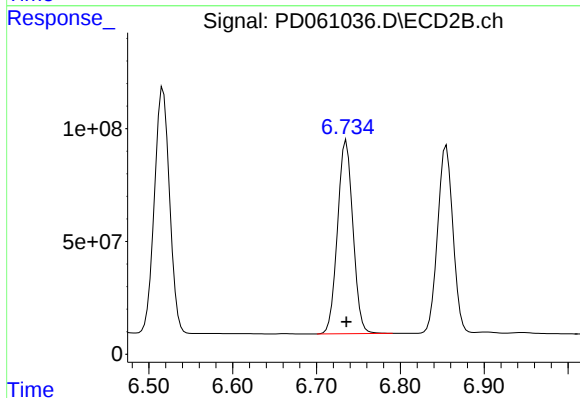


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 1095600838
Conc: 146.28 ng/ml

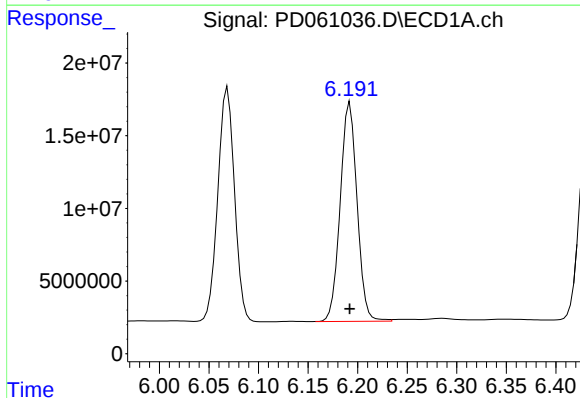


#16 4,4'-DDD

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 178136755
Conc: 148.19 ng/ml

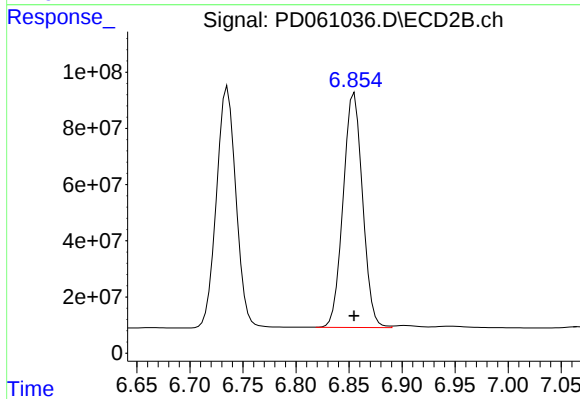

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 1059782432
Conc: 144.36 ng/ml

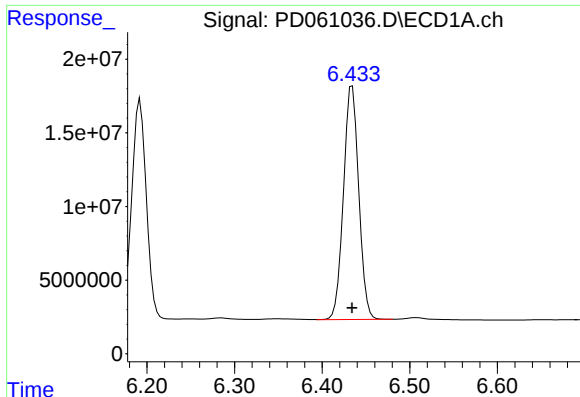

#17 4,4'-DDT


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 192541515
Conc: 151.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

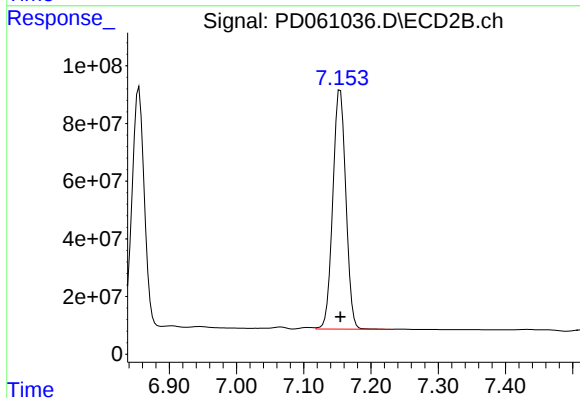


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 1109845501
Conc: 147.65 ng/ml

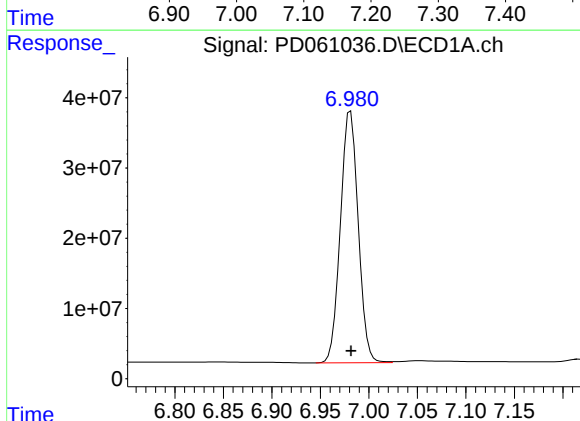


#20 Methoxychlor

R.T.: 6.981 min
Delta R.T.: 0.000 min
Response: 458255613
Conc: 715.16 ng/ml

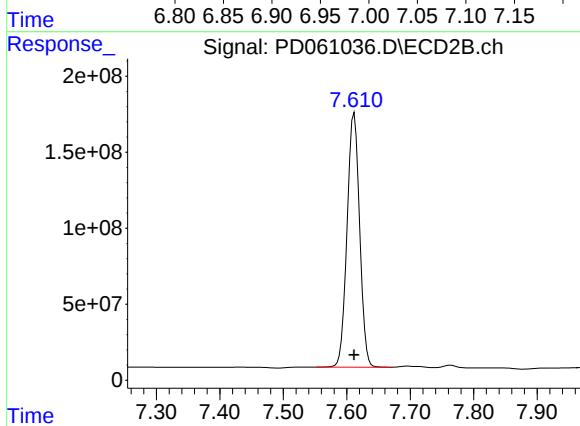

#20 Methoxychlor

R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 2300806395
Conc: 684.32 ng/ml

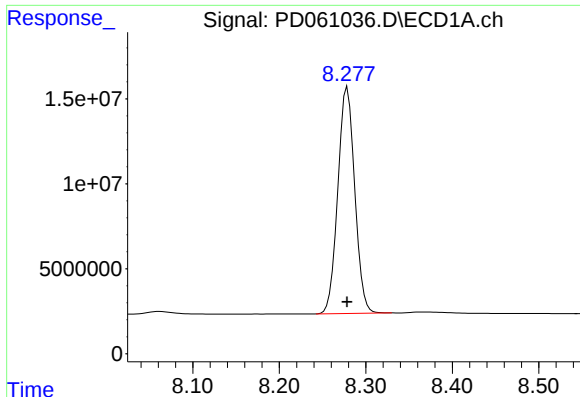

#27 Decachlorobiphenyl


R.T.: 8.279 min

Delta R.T.: 0.000 min

Response: 180016053

Conc: 140.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

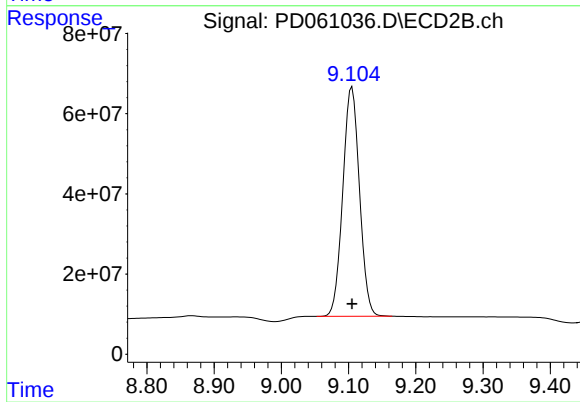

#27 Decachlorobiphenyl

R.T.: 9.105 min

Delta R.T.: 0.000 min

Response: 985379391

Conc: 145.67 ng/ml