

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
 Data File : PD061044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2021 18:54
 Operator : DD\AJ
 Sample : INDA306
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 03:04:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	19011680	140.9E6	18.731	19.694
27)	SA Decachlor...	8.278	9.104	44955541	265.7E6	35.678	39.120
Target Compounds							
2)	A alpha-BHC	3.938	4.411	27787955	215.8E6	18.640	19.505
3)	MA gamma-BHC...	4.223	4.697	26899863	199.0E6	18.385	19.621
4)	MA Heptachlor	4.528	5.208	27947848	208.2E6	18.493	19.744
9)	A Endosulfan I	5.564	6.259	24561570	171.3E6	18.730	19.885
13)	MA Dieldrin	5.810	6.517	53981989	361.9E6	36.763	38.928
14)	MA Endrin	6.068	6.735	45450665	283.2E6	36.564	38.341
16)	A 4,4'-DDD	6.192	6.855	43152448	278.3E6	36.764	39.111
17)	MA 4,4'-DDT	6.434	7.154	44191614	285.9E6	36.091	39.376
20)	A Methoxychlor	6.981	7.611	113.7E6	647.8E6	182.180	196.254

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012521\
Data File : PD061044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2021 18:54
Operator : DD\AJ
Sample : INDA306
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 03:04:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

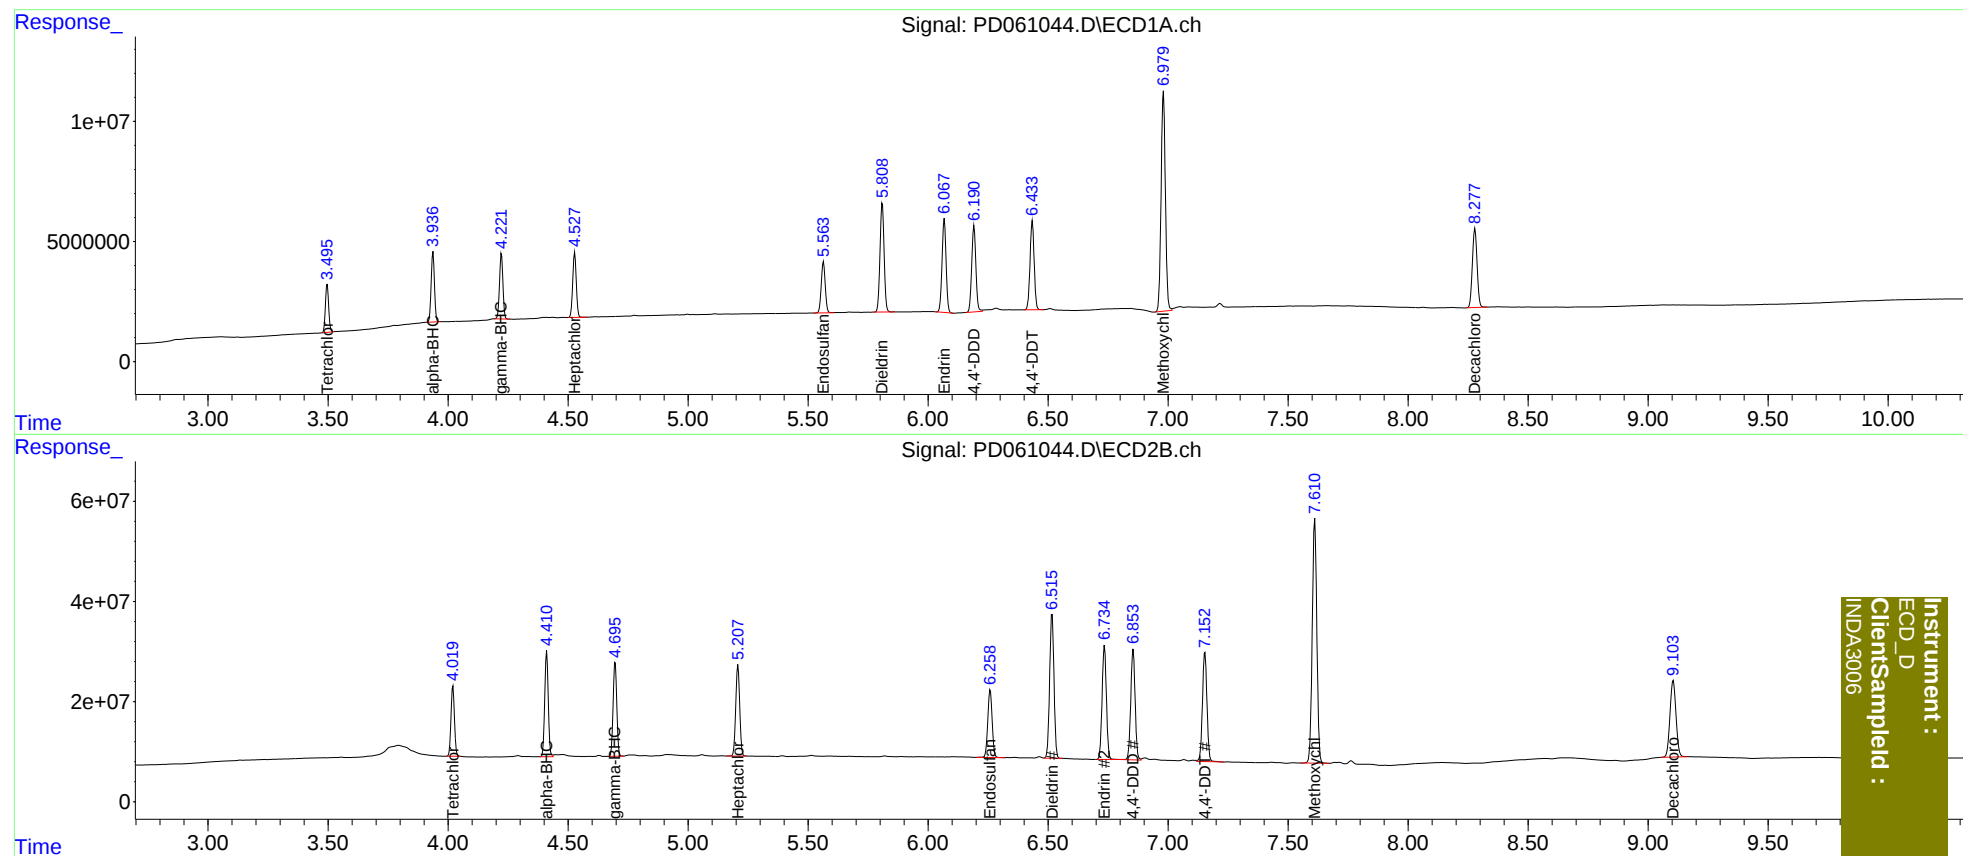

Instrument :
ECD_D
ClientSampled :
INDA3006