

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012522\
 Data File : PD067794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2022 13:56
 Operator : AR\AJ
 Sample : INDA363
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3116

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 03:01:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.960	44172755	171.6E6	19.497	21.176
27)	SA Decachlor...	8.158	9.016	38810637	212.4E6	40.522	42.043
Target Compounds							
2)	A alpha-BHC	3.872	4.353	67022525	226.0E6	20.222	21.565
3)	MA gamma-BHC...	4.154	4.638	63398550	214.5E6	20.041	21.744
4)	MA Heptachlor	4.447	5.139	63288046	184.8E6	20.418	20.667
9)	A Endosulfan I	5.468	6.188	53802268	154.5E6	20.327	21.510
13)	MA Dieldrin	5.711	6.447	117.9E6	319.2E6	41.829	42.450
14)	MA Endrin	5.967	6.663	99947102	228.1E6	44.862	40.888
16)	A 4,4'-DDD	6.093	6.792	87560449	256.0E6	43.952	43.561
17)	MA 4,4'-DDT	6.331	7.090	85095589	254.4E6	41.323	43.788
20)	A Methoxychlor	6.879	7.553	192.3E6	601.4E6	217.995	218.131


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012522\
Data File : PD067794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2022 13:56
Operator : AR\AJ
Sample : INDA363
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 03:01:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

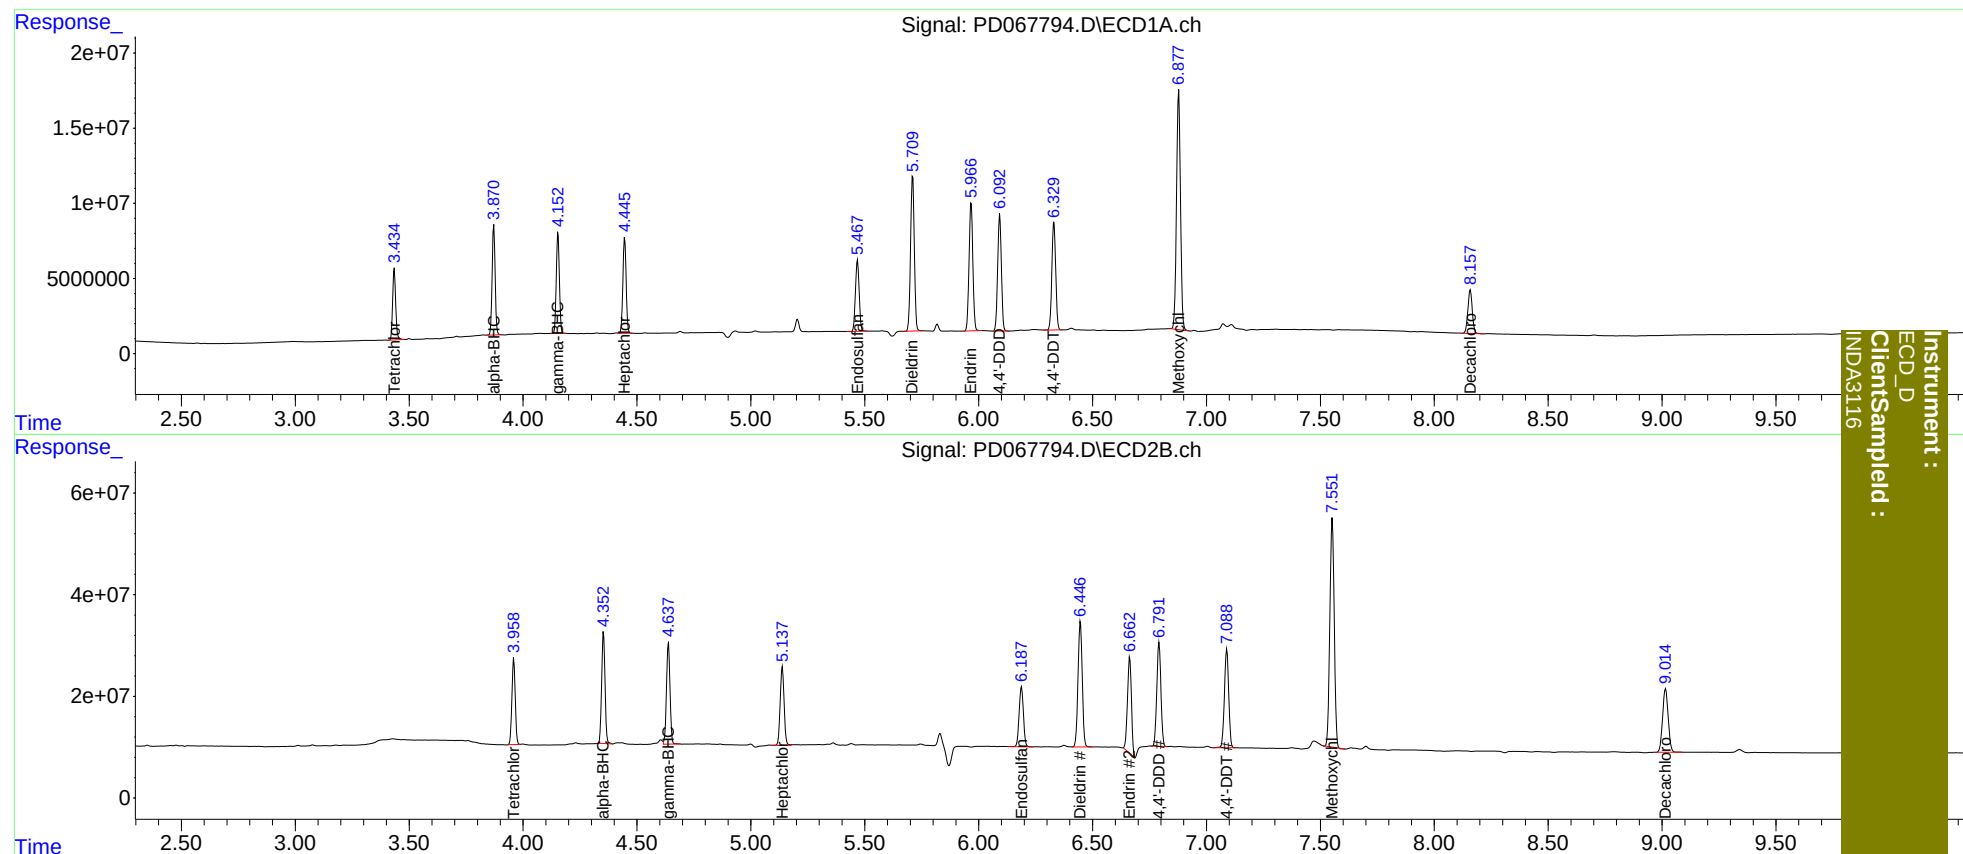


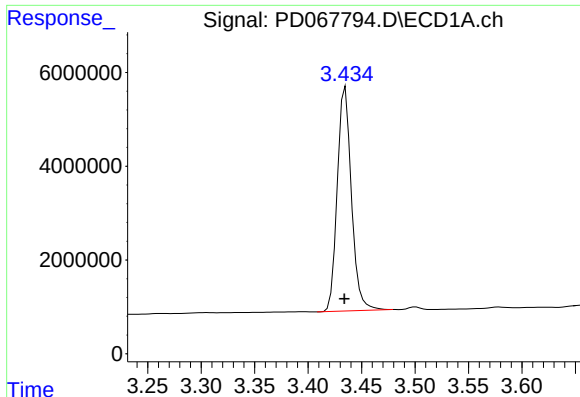

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 44172755
Conc: 19.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

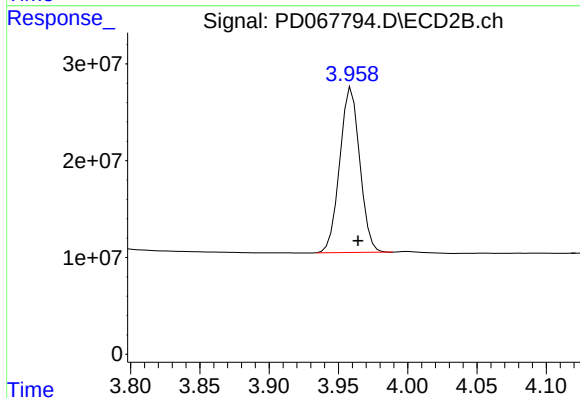


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.005 min
Response: 171629202
Conc: 21.18 ng/ml

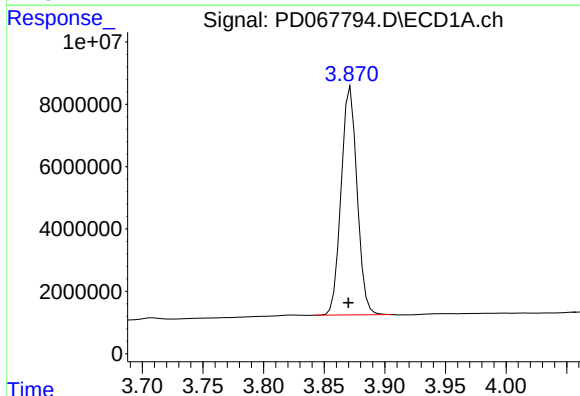


#2 alpha-BHC

R.T.: 3.872 min
Delta R.T.: 0.002 min
Response: 67022525
Conc: 20.22 ng/ml

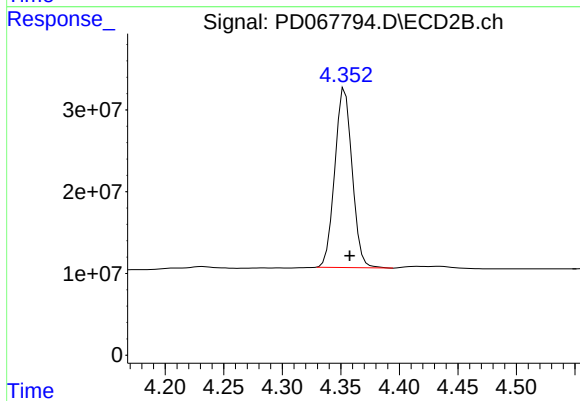

#2 alpha-BHC


R.T.: 4.353 min
Delta R.T.: -0.004 min
Response: 225999411
Conc: 21.57 ng/ml

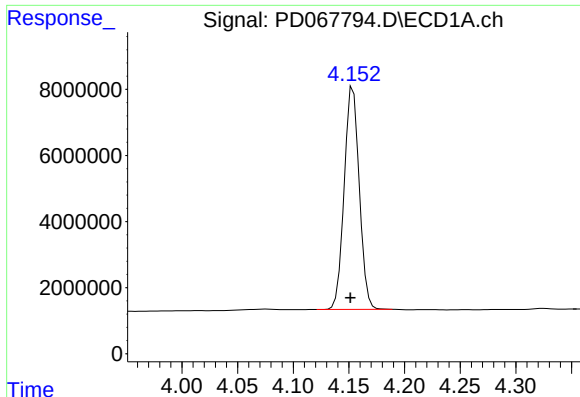

#3 gamma-BHC (Lindane)


R.T.: 4.154 min
Delta R.T.: 0.002 min
Response: 63398550
Conc: 20.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

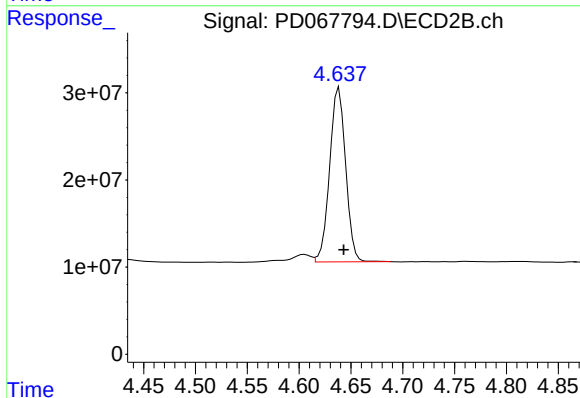


#3 gamma-BHC (Lindane)

R.T.: 4.638 min
Delta R.T.: -0.004 min
Response: 214538126
Conc: 21.74 ng/ml

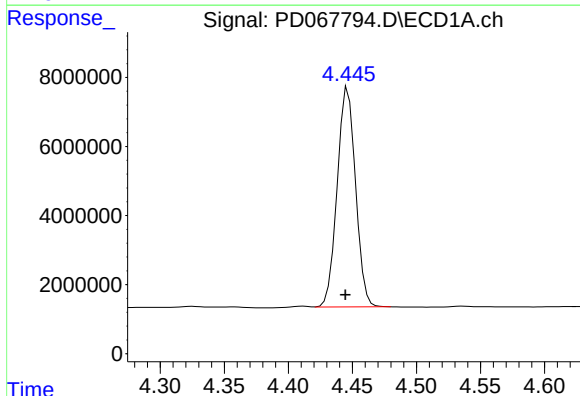


#4 Heptachlor

R.T.: 4.447 min
Delta R.T.: 0.002 min
Response: 63288046
Conc: 20.42 ng/ml

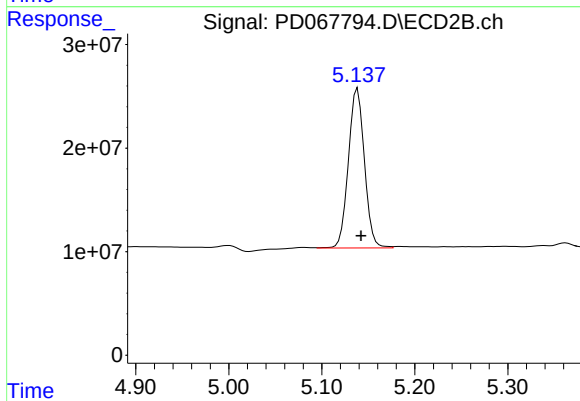

#4 Heptachlor


R.T.: 5.139 min
Delta R.T.: -0.004 min
Response: 184816739
Conc: 20.67 ng/ml

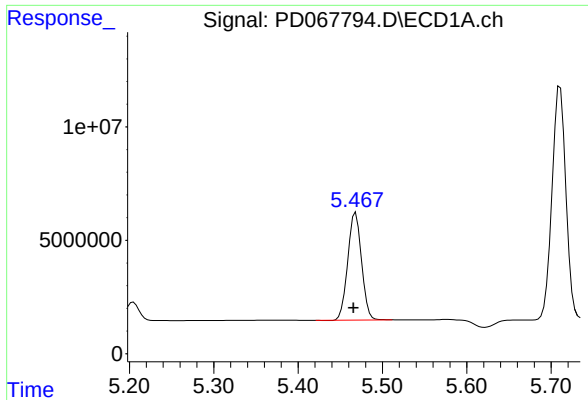

#9 Endosulfan I


R.T.: 5.468 min
Delta R.T.: 0.003 min
Response: 53802268
Conc: 20.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

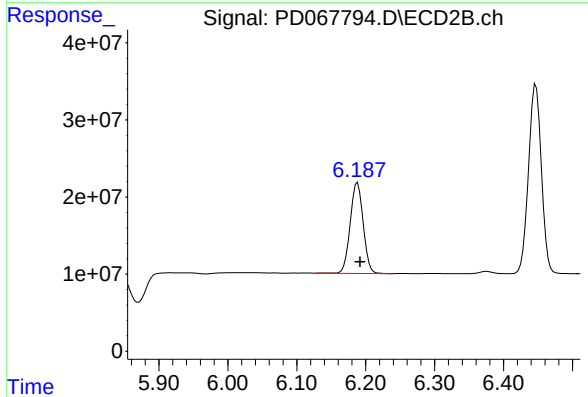


#9 Endosulfan I

R.T.: 6.188 min
Delta R.T.: -0.004 min
Response: 154547747
Conc: 21.51 ng/ml

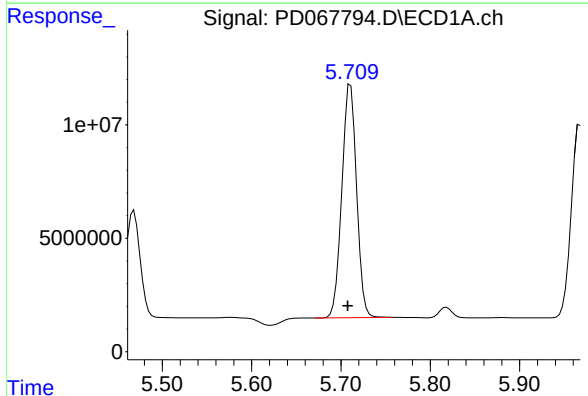


#13 Dieldrin

R.T.: 5.711 min
Delta R.T.: 0.003 min
Response: 117897284
Conc: 41.83 ng/ml

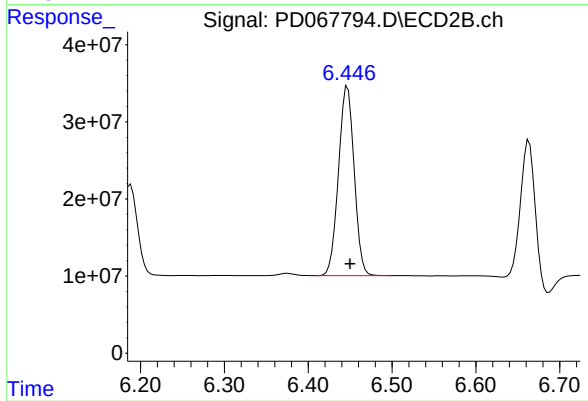

#13 Dieldrin


R.T.: 6.447 min
Delta R.T.: -0.003 min
Response: 319200344
Conc: 42.45 ng/ml

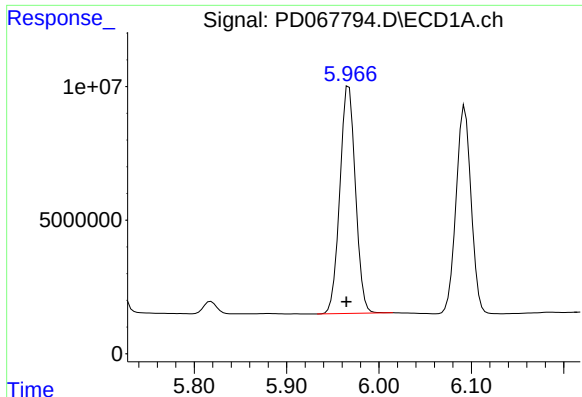

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.003 min
Response: 99947102
Conc: 44.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

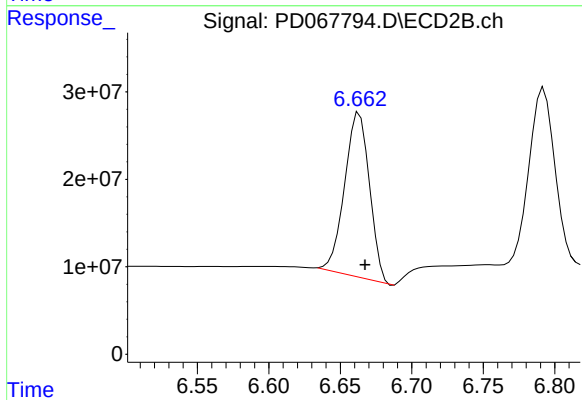


#14 Endrin

R.T.: 6.663 min
Delta R.T.: -0.004 min
Response: 228085144
Conc: 40.89 ng/ml

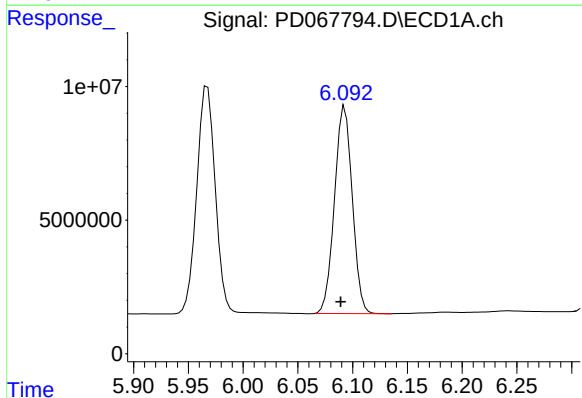


#16 4,4'-DDD

R.T.: 6.093 min
Delta R.T.: 0.004 min
Response: 87560449
Conc: 43.95 ng/ml

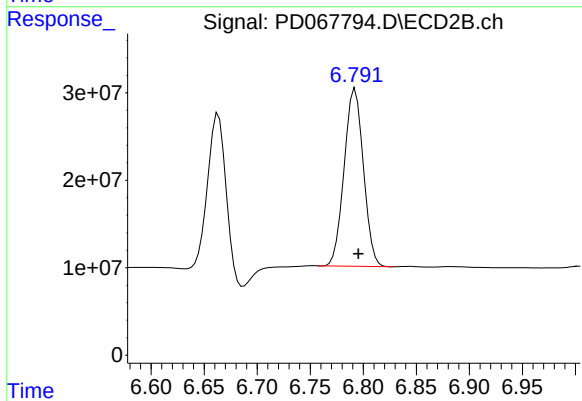

#16 4,4'-DDD


R.T.: 6.792 min
Delta R.T.: -0.003 min
Response: 256027443
Conc: 43.56 ng/ml

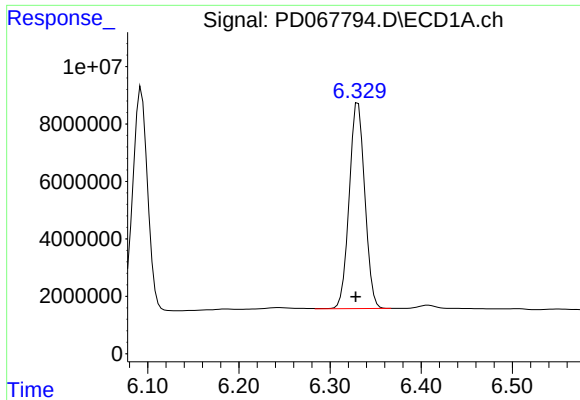

#17 4,4'-DDT


R.T.: 6.331 min
Delta R.T.: 0.003 min
Response: 85095589
Conc: 41.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

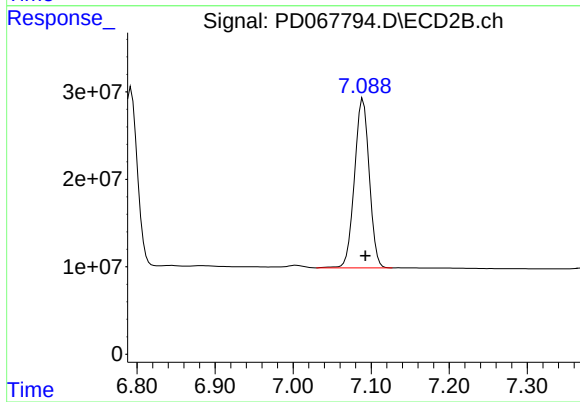


#17 4,4'-DDT

R.T.: 7.090 min
Delta R.T.: -0.003 min
Response: 254397550
Conc: 43.79 ng/ml

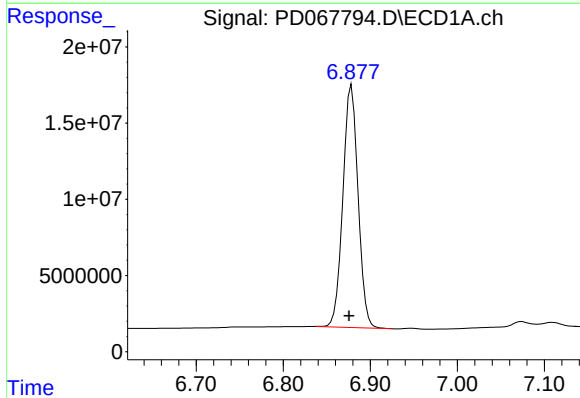


#20 Methoxychlor

R.T.: 6.879 min
Delta R.T.: 0.003 min
Response: 192266745
Conc: 218.00 ng/ml

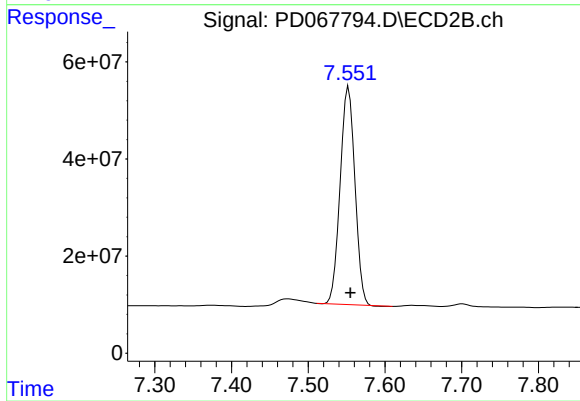

#20 Methoxychlor


R.T.: 7.553 min
Delta R.T.: -0.002 min
Response: 601426610
Conc: 218.13 ng/ml

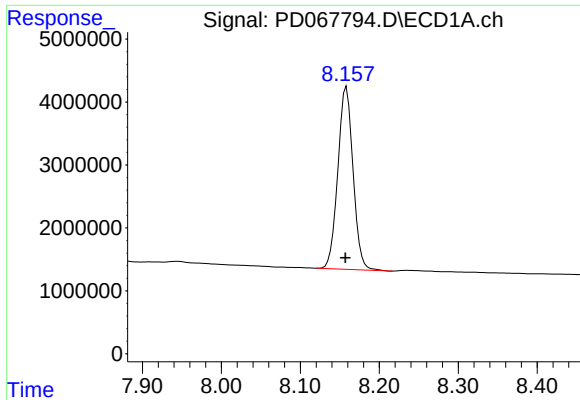

#27 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: 0.001 min
Response: 38810637
Conc: 40.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3116

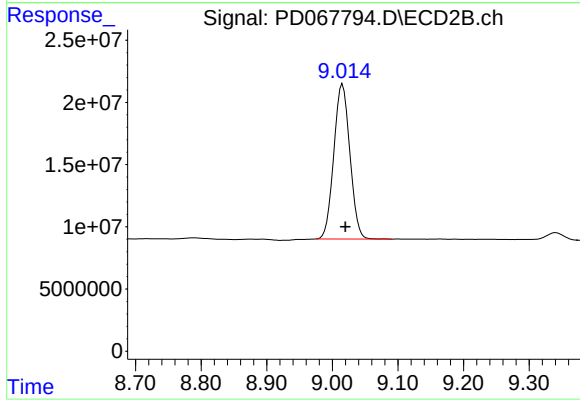

#27 Decachlorobiphenyl

R.T.: 9.016 min
Delta R.T.: -0.004 min
Response: 212446219
Conc: 42.04 ng/ml