

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
 Data File : PD073755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2023 00:07
 Operator : AR\AJ
 Sample : 01226-10MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EX9G4MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/25/2023
 Supervised By : Ankita Jodhani 01/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 04:13:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	43141863	23959409	18.218	18.875
27)	SA Decachlor...	9.098	7.931	71606026	29960278	25.954	24.894
Target Compounds							
2)	A alpha-BHC	4.010	3.280	189.9E6	86284619	49.864	48.690
3)	MA gamma-BHC...	4.344	3.610	176.3E6	79405048	48.407	47.232
4)	MA Heptachlor	4.936	3.952	165.1E6	66982223	45.365	44.413
5)	MB Aldrin	5.280	4.233	164.6E6	74386528	45.999	43.819
6)	B beta-BHC	4.537	3.905	72768028	33418844	43.326	40.883
7)	B delta-BHC	4.785	4.135	153.0E6	72105322	46.826m	41.571m
8)	B Heptachlo...	5.706	4.736	145.4E6	66272987	44.702	42.562
9)	A Endosulfan I	6.094	5.107	140.2E6	62603919	45.699	43.624
10)	B trans-Chl...	5.962	4.987	145.0E6	66952479	45.025	42.871
11)	B cis-Chlor...	6.042	5.052	144.6E6	66630536	43.383	41.452
12)	B 4,4'-DDE	6.214	5.242	297.3E6	125.7E6	94.310	85.624
13)	MA Dieldrin	6.369	5.371	324.4E6	138.8E6	96.527	89.196m
14)	MA Endrin	6.599	5.648	273.1E6	120.7E6	97.608	93.793
15)	B Endosulfa...	6.817	5.942	272.9E6	120.9E6	92.330	87.836
16)	A 4,4'-DDD	6.732	5.797	238.9E6	104.1E6	93.871	86.267
17)	MA 4,4'-DDT	7.047	6.048	266.0E6	104.0E6	97.479	88.079
18)	B Endrin al...	6.947	6.122	202.9E6	87856600	84.843	80.477
19)	B Endosulfa...	7.182	6.344	260.8E6	109.4E6	93.849	86.991
20)	A Methoxychlor	7.522	6.625	735.2E6	255.5E6	493.951	463.168
21)	B Endrin ke...	7.669	6.851	314.5E6	135.0E6	98.659	89.742

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
Data File : PD073755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2023 00:07
Operator : AR\AJ
Sample : 01226-10MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 04:13:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

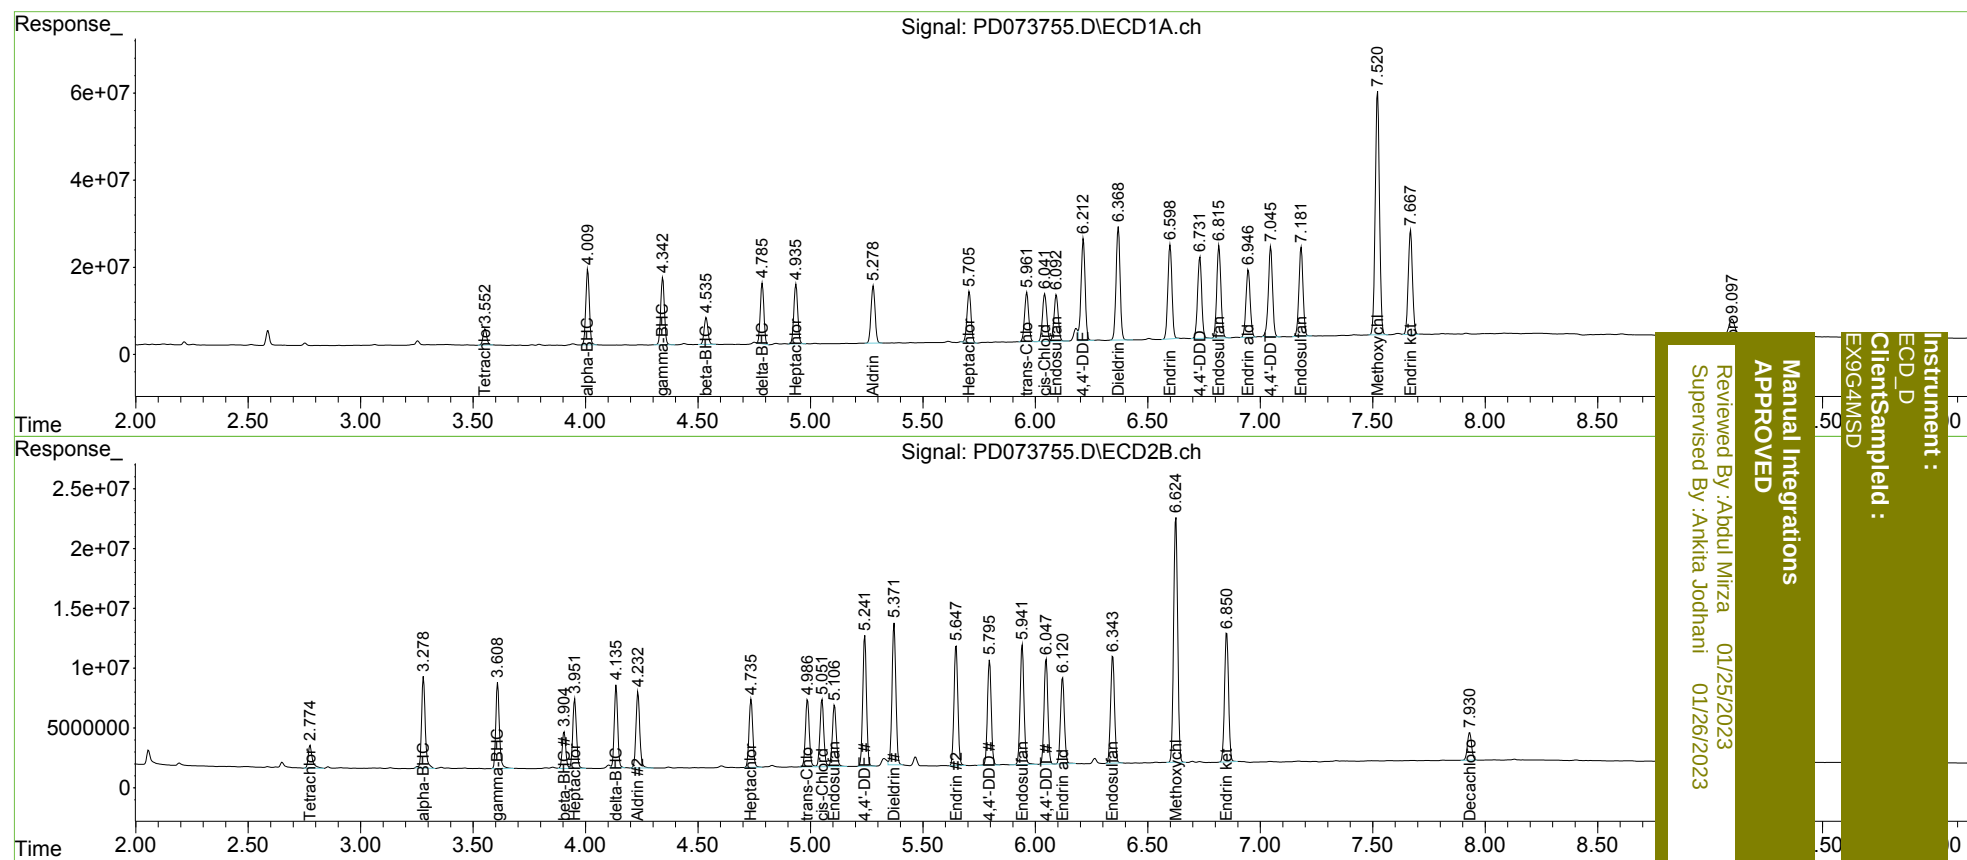

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/25/2023
Supervised By: Ankita Jodhani 01/26/2023

Instrument :
ECD_D
Client Sampled :
EX9G4MSD