

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
 Data File : PD073756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2023 00:20
 Operator : AR\AJ
 Sample : 01226-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EX9G5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/25/2023
 Supervised By : Ankita Jodhani 01/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 04:13:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	48787566	26333788	20.602	20.746
27)	SA Decachlor...	9.098	7.931	91209213	38855165	33.059	32.284
Target Compounds							
5)	MB Aldrin	5.277	4.233	2168398	665009	0.606	0.392m#
10)	B trans-Chl...	5.961	4.987	5138072	2327501	1.596m	1.490
11)	B cis-Chlor...	6.045	5.050	3253033	692484	0.976	0.431m#
13)	MA Dieldrin	6.368	5.371	11445484	4956526	3.406m	3.185m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
Data File : PD073756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2023 00:20
Operator : AR\AJ
Sample : 01226-11
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 04:13:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

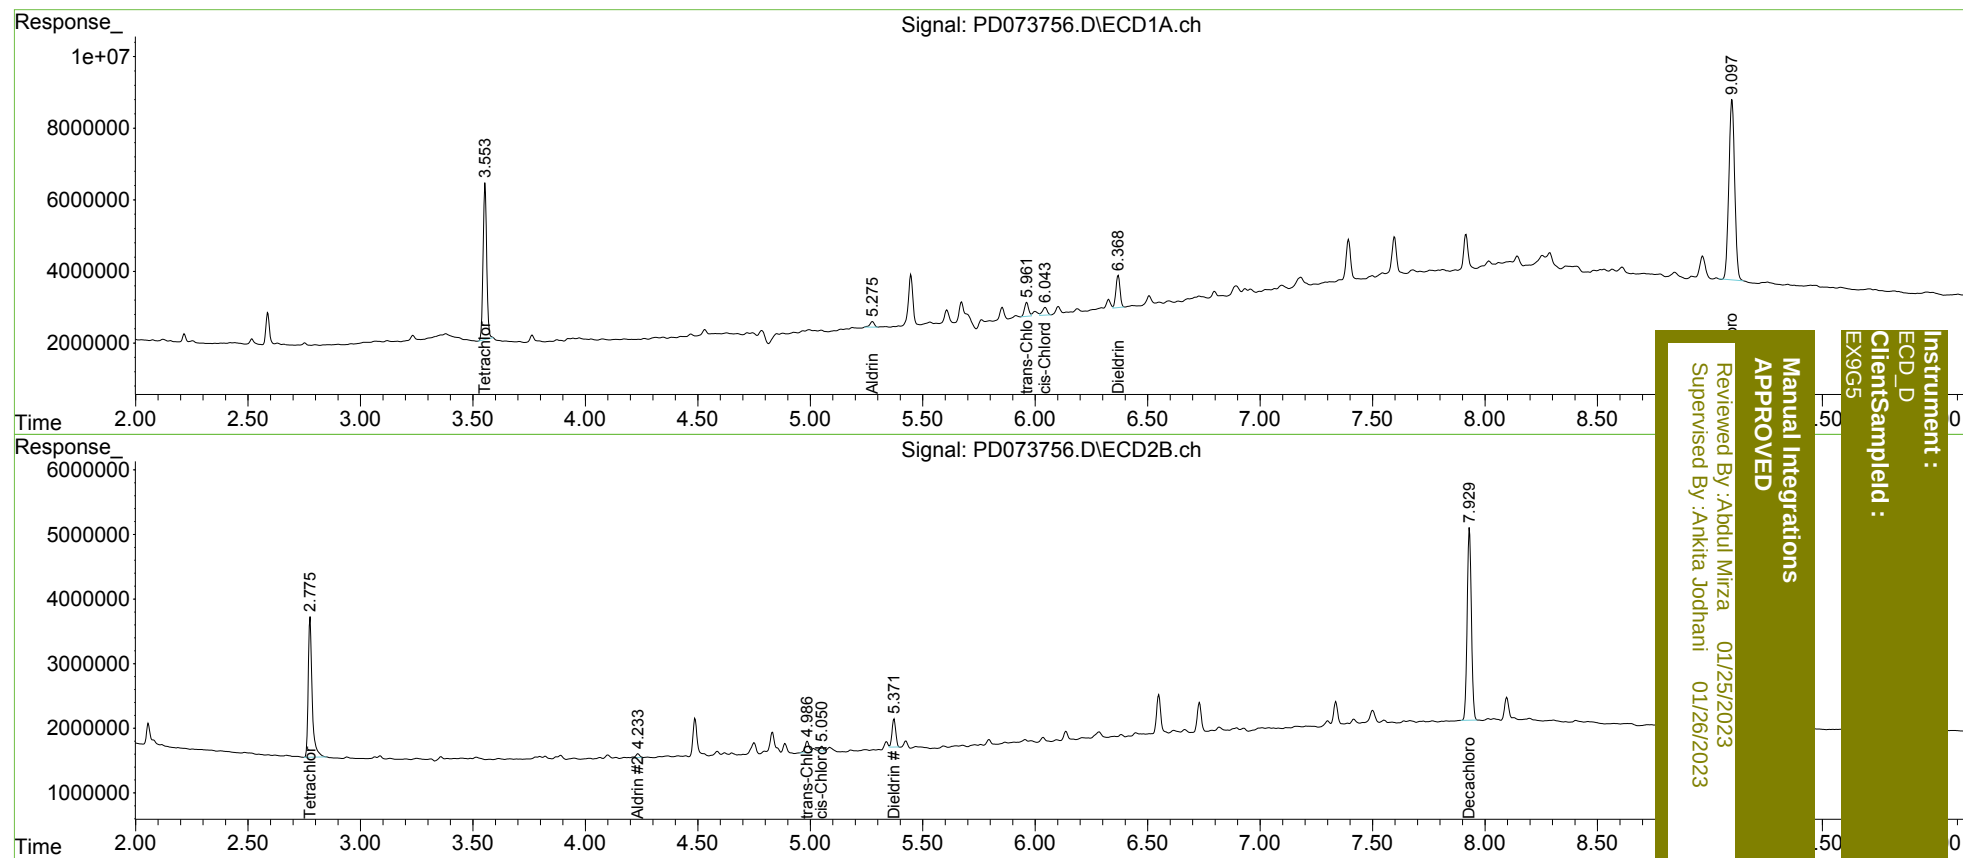

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/25/2023
Supervised By: Ankita Jodhani 01/26/2023

Instrument :
ECD_D
ClientSampled :
EX9G5