

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
 Data File : PD073754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 23:53
 Operator : AR\AJ
 Sample : 01226-09MS
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EX9G4MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/25/2023
 Supervised By :Ankita Jodhani 01/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 04:07:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	42374308	23765357	17.894	18.722
27)	SA Decachlor...	9.098	7.931	73113255	30368614	26.500	25.233
Target Compounds							
2)	A alpha-BHC	4.011	3.280	189.3E6	86456869	49.710	48.788
3)	MA gamma-BHC...	4.344	3.610	176.3E6	79014818	48.407	47.000
4)	MA Heptachlor	4.936	3.953	164.0E6	66827007	45.081	44.310
5)	MB Aldrin	5.280	4.234	165.1E6	74344066	46.151	43.794
6)	B beta-BHC	4.537	3.905	72101823	33067274	42.929	40.453
7)	B delta-BHC	4.785	4.135	154.1E6	72043197	47.173m	41.536m
8)	B Heptachlo...	5.707	4.736	146.4E6	66274486	45.011	42.563
9)	A Endosulfan I	6.094	5.108	142.2E6	62704512	46.345	43.695
10)	B trans-Chl...	5.963	4.988	145.6E6	67047885	45.225	42.932
11)	B cis-Chlor...	6.043	5.052	145.7E6	66657877	43.698	41.469
12)	B 4,4'-DDE	6.214	5.242	284.4E6	126.0E6	90.210	85.798
13)	MA Dieldrin	6.370	5.373	326.0E6	138.7E6	97.025	89.106
14)	MA Endrin	6.600	5.648	273.5E6	120.5E6	97.750	93.590
15)	B Endosulfa...	6.817	5.941	274.6E6	121.2E6	92.921	88.090
16)	A 4,4'-DDD	6.732	5.797	240.7E6	104.2E6	94.615	86.401
17)	MA 4,4'-DDT	7.047	6.049	267.5E6	104.5E6	97.994	88.502
18)	B Endrin al...	6.948	6.121	203.4E6	87686237	85.045	80.321
19)	B Endosulfa...	7.182	6.344	262.8E6	110.2E6	94.578	87.632
20)	A Methoxychlor	7.522	6.624	743.4E6	256.2E6	499.487	464.427
21)	B Endrin ke...	7.668	6.851	317.1E6	135.3E6	99.482	89.932

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012523\
Data File : PD073754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 23:53
Operator : AR\AJ
Sample : 01226-09MS
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 04:07:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

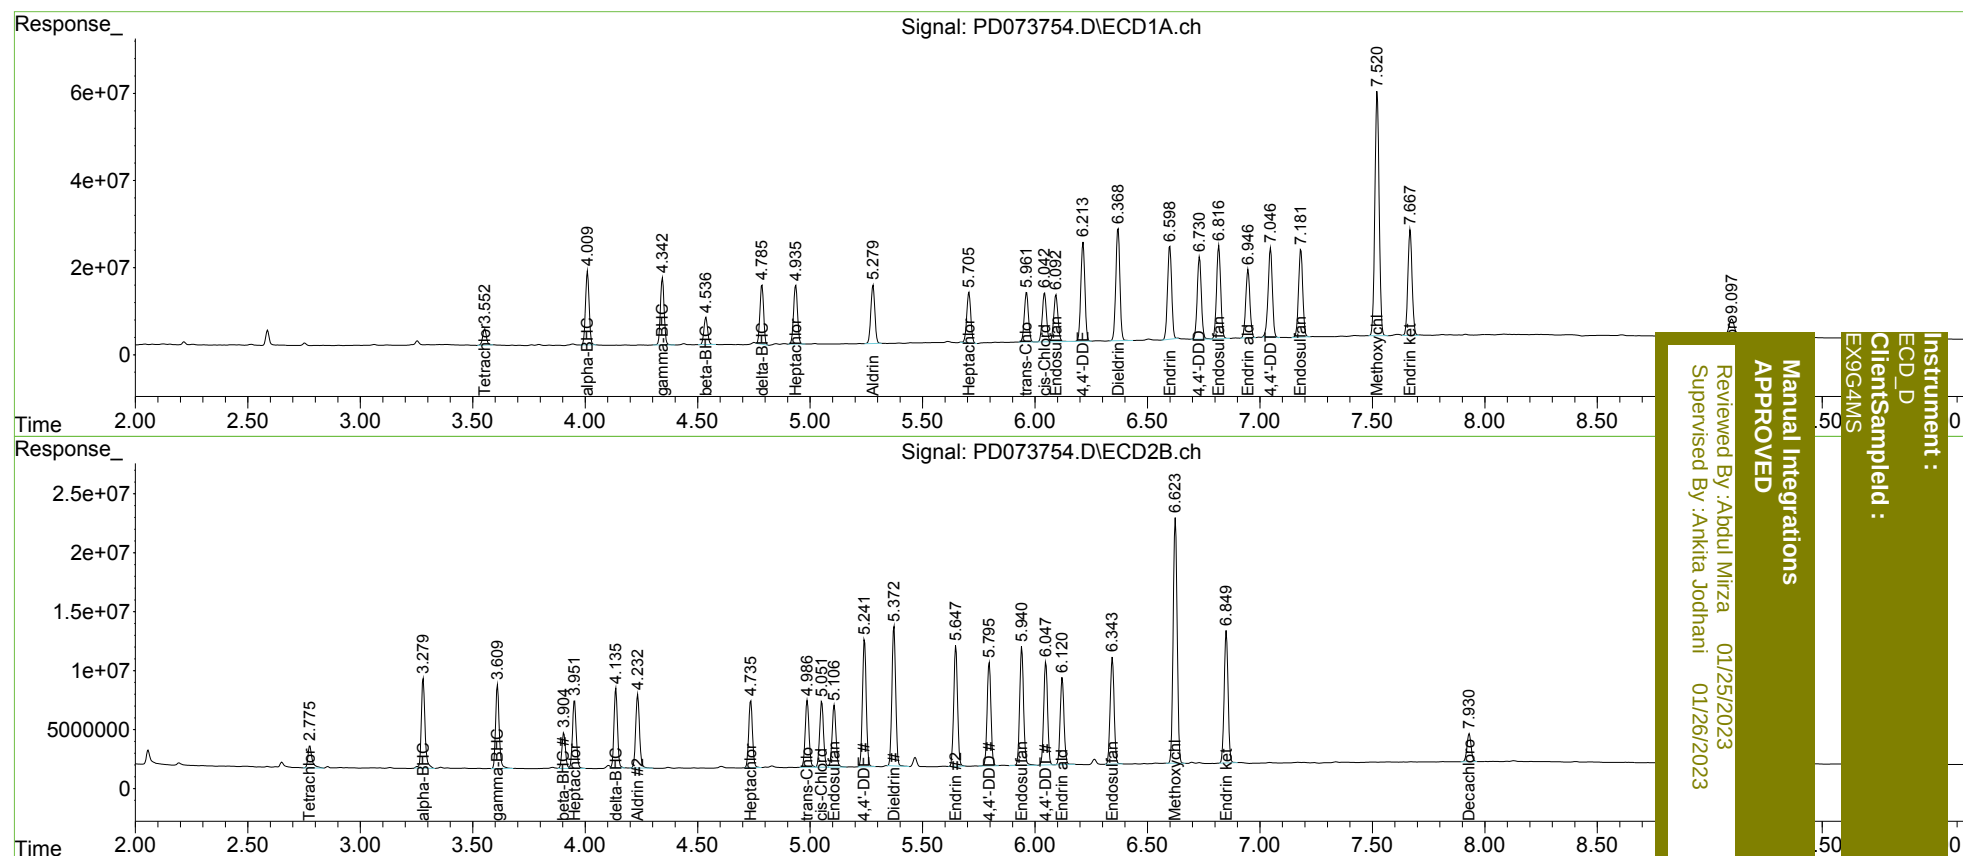

Instrument :
ECD_D
ClientSampled :
EX9G4MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/25/2023
Supervised By :Ankita Jodhani 01/26/2023