

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
 Data File : PD080897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2024 15:04
 Operator : AR\AJ
 Sample : PB158619BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB158619BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:46:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.572	2.795	32765436	56066205	23.081	23.438
28)	SA Decachlor...	9.117	7.935	49060991	67066192	24.379	25.179
Target Compounds							
2)	A alpha-BHC	0.000	3.311	0	128568	N.D.	0.034 #
3)	MA gamma-BHC...	0.000	3.640	0	741281	N.D.	0.198 #
7)	B delta-BHC	4.800	0.000	1084124	0	0.432	N.D. #
8)	B Heptachlo...	0.000	4.777f	0	3138081	N.D.	0.937 #
13)	MA Dieldrin	6.394	0.000	302279	0	0.137	N.D. #
15)	B Endosulfa...	6.828	0.000	263139	0	0.136	N.D. #
18)	B Endrin al...	0.000	6.140	0	308771	N.D.	0.137 #
21)	B Endrin ke...	7.703f	0.000	293187	0	0.140	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
Data File : PD080897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2024 15:04
Operator : AR\AJ
Sample : PB158619BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB158619BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:46:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

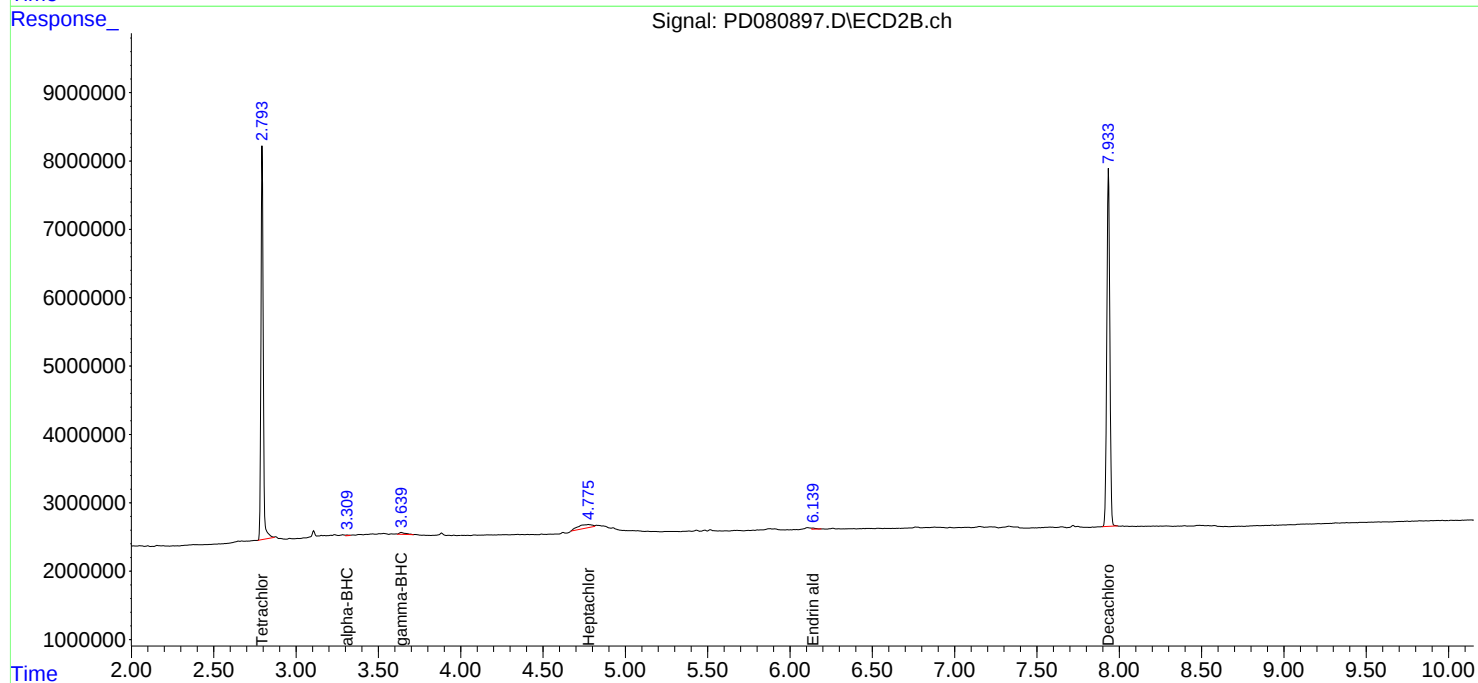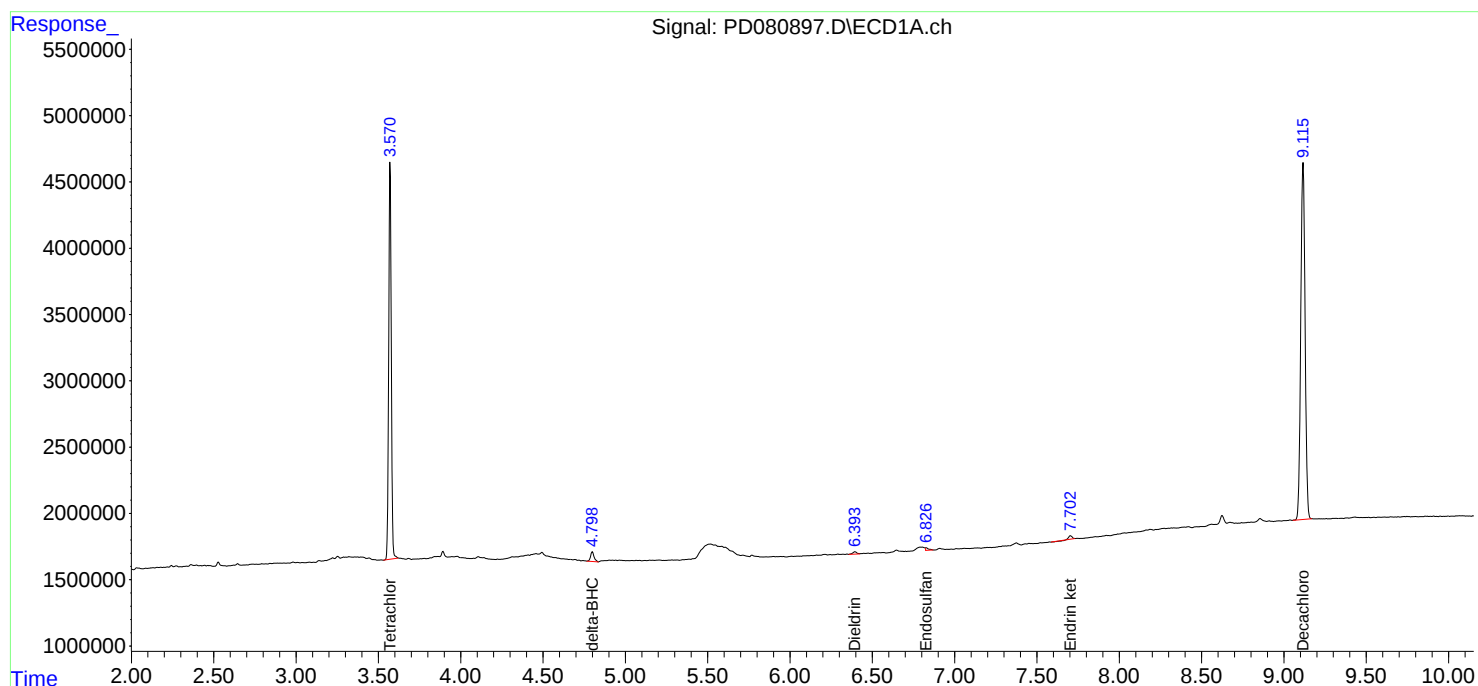


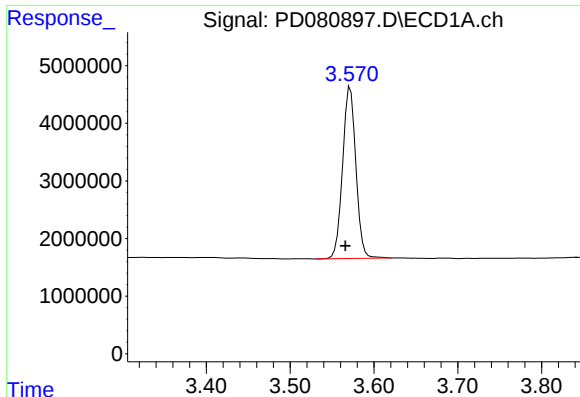

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: 0.006 min
Response: 32765436
Conc: 23.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158619BL

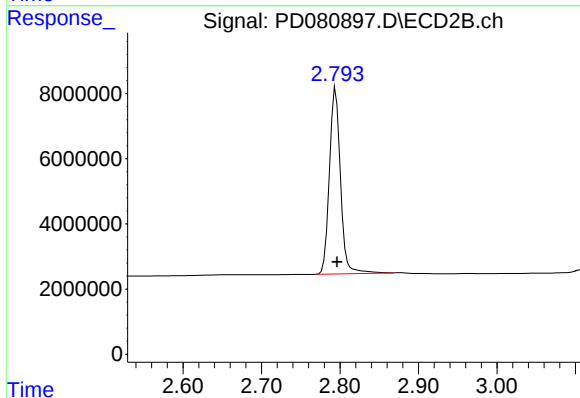


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.001 min
Response: 56066205
Conc: 23.44 ng/ml

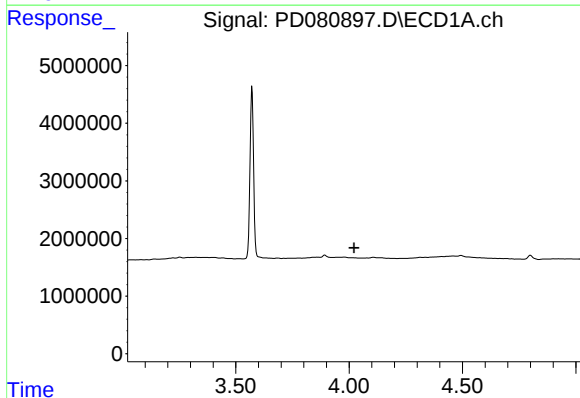


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

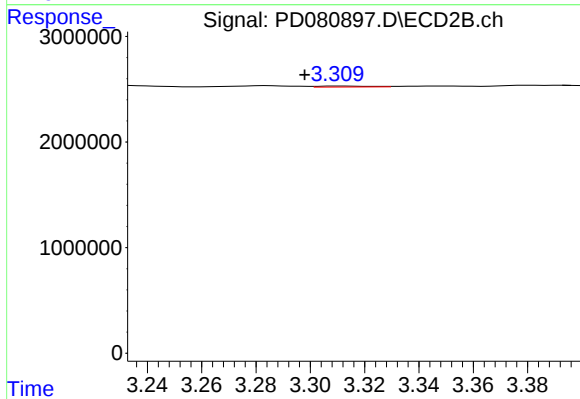

#2 alpha-BHC


R.T.: 3.311 min
Delta R.T.: 0.013 min
Response: 128568
Conc: 0.03 ng/ml

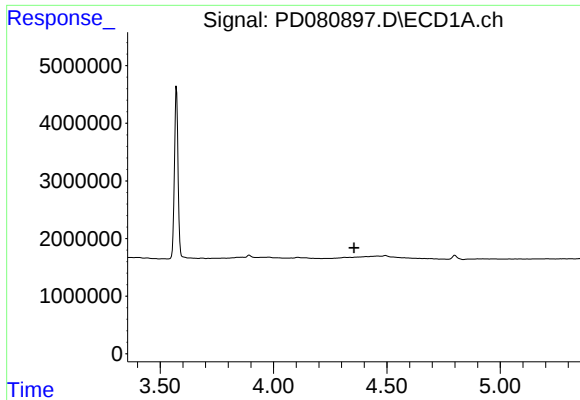

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158619BL

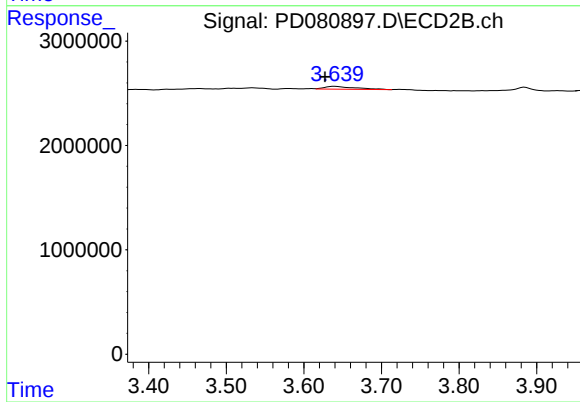


#3 gamma-BHC (Lindane)

R.T.: 3.640 min
Delta R.T.: 0.013 min
Response: 741281
Conc: 0.20 ng/ml

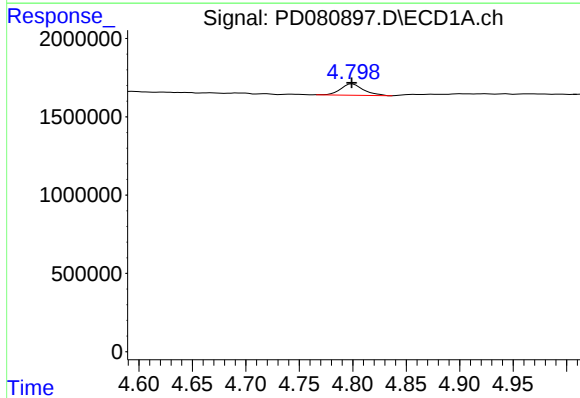


#7 delta-BHC

R.T.: 4.800 min
Delta R.T.: 0.000 min
Response: 1084124
Conc: 0.43 ng/ml

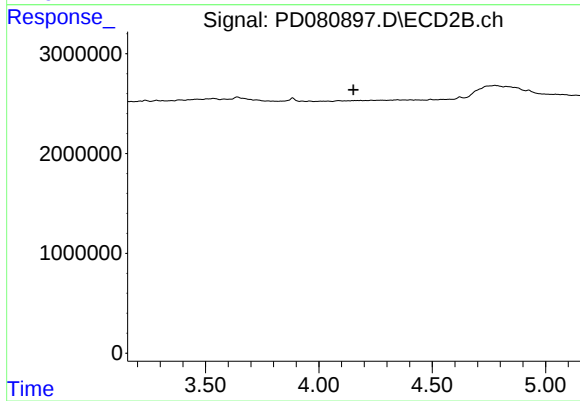

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.153 min
Response: 0
Conc: N.D.

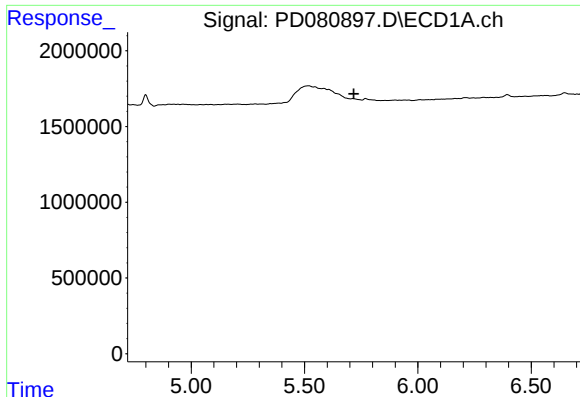

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.717 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB158619BL

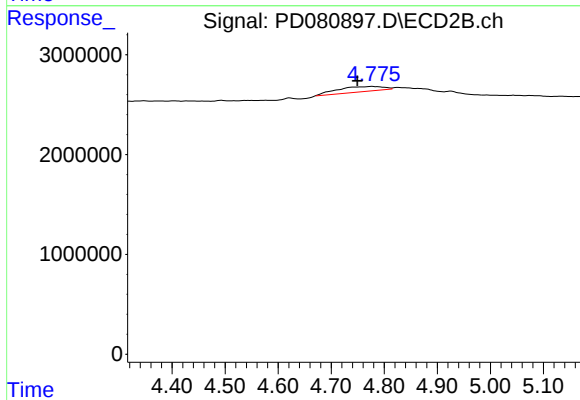


#8 Heptachlor epoxide

R.T.: 4.777 min
Delta R.T.: 0.027 min
Response: 3138081
Conc: 0.94 ng/ml

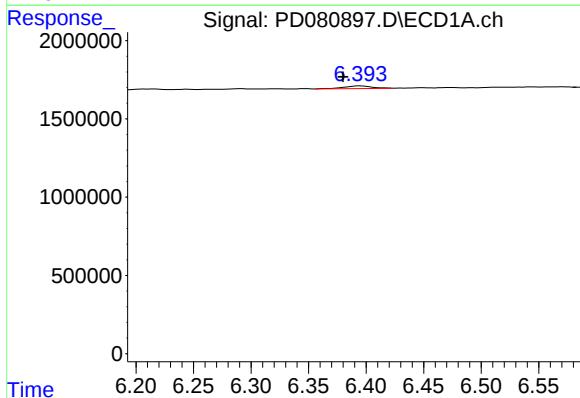


#13 Dieldrin

R.T.: 6.394 min
Delta R.T.: 0.014 min
Response: 302279
Conc: 0.14 ng/ml

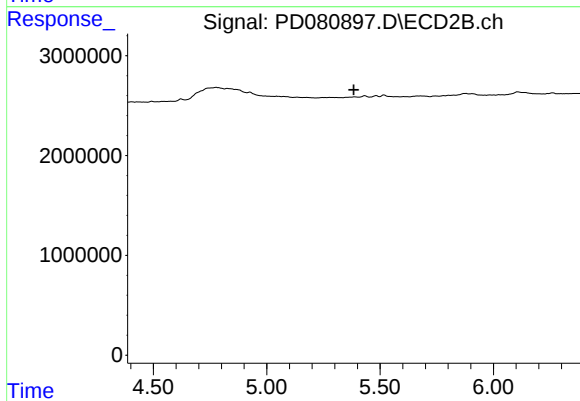

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.384 min
Response: 0
Conc: N.D.

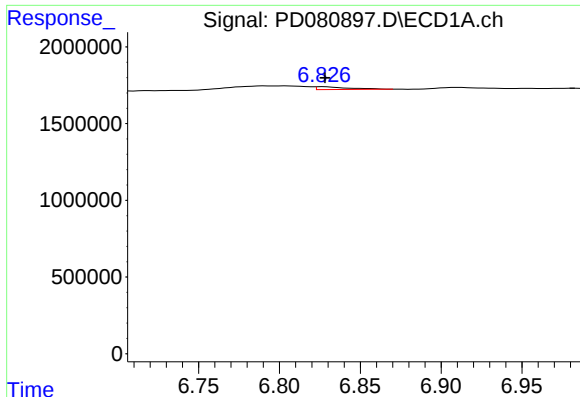

#15 Endosulfan II


R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 263139
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158619BL

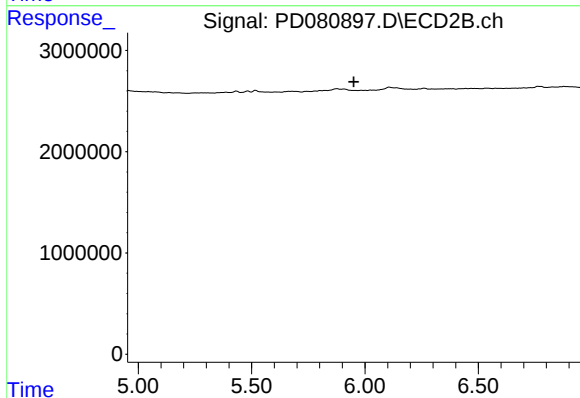


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.951 min
Response: 0
Conc: N.D.

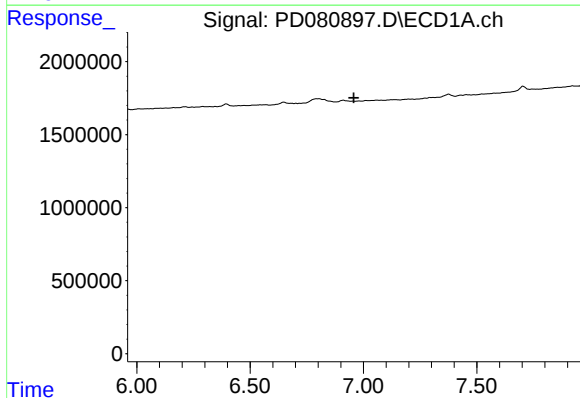


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.958 min
Response: 0
Conc: N.D.

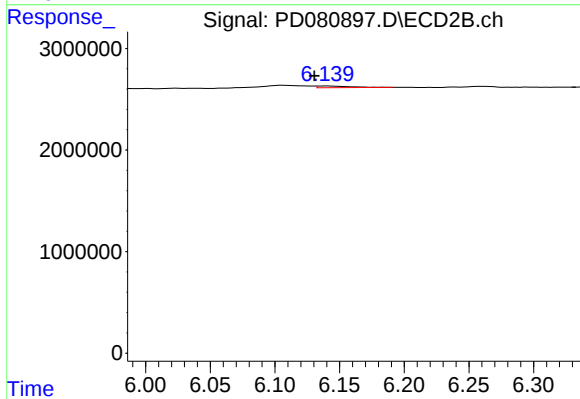

#18 Endrin aldehyde


R.T.: 6.140 min
Delta R.T.: 0.010 min
Response: 308771
Conc: 0.14 ng/ml

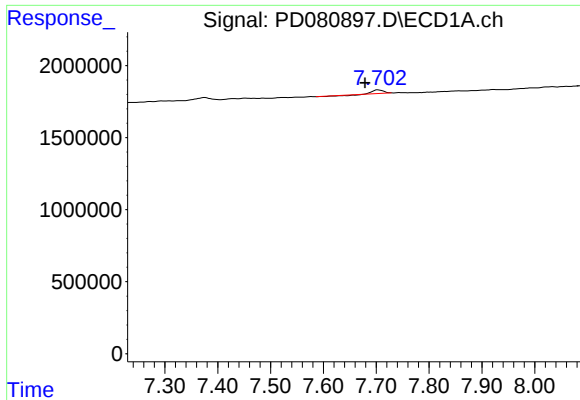

#21 Endrin ketone


R.T.: 7.703 min
Delta R.T.: 0.025 min
Response: 293187
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB158619BL

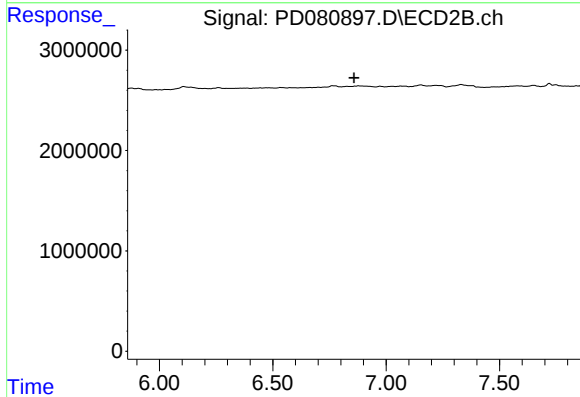


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

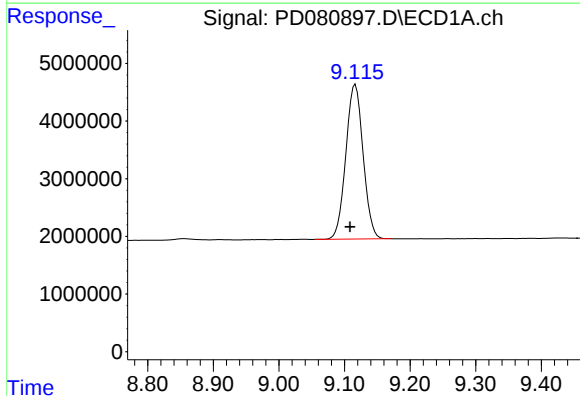

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.008 min
Response: 49060991
Conc: 24.38 ng/ml

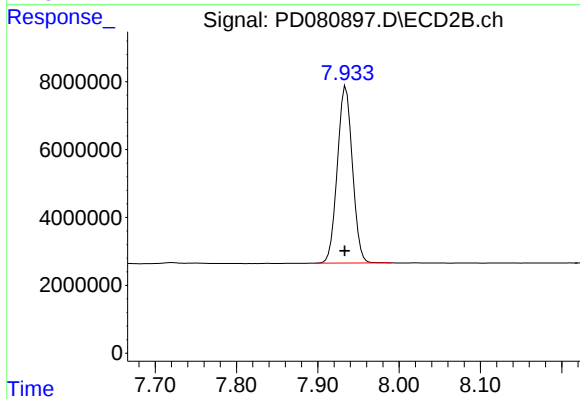

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.002 min
Response: 67066192
Conc: 25.18 ng/ml