

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
 Data File : PD080895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2024 14:31
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:45:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.795	60898943	124.0E6	42.900	51.818
28)	SA Decachlor...	9.112	7.934	84723549	118.8E6	42.100	44.608
Target Compounds							
23)	Chlordane-1	4.733	3.794	31926052	42723653	413.487	420.118
24)	Chlordane-2	5.264	4.370	33768152	50769747	407.917	414.207
25)	Chlordane-3	5.975	5.000	130.1E6	140.8E6	411.845	419.665
26)	Chlordane-4	6.058	5.064	156.4E6	132.7E6	410.878	417.566
27)	Chlordane-5	6.909	5.958	28954402	51672416	414.759	426.194



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
Data File : PD080895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2024 14:31
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:45:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

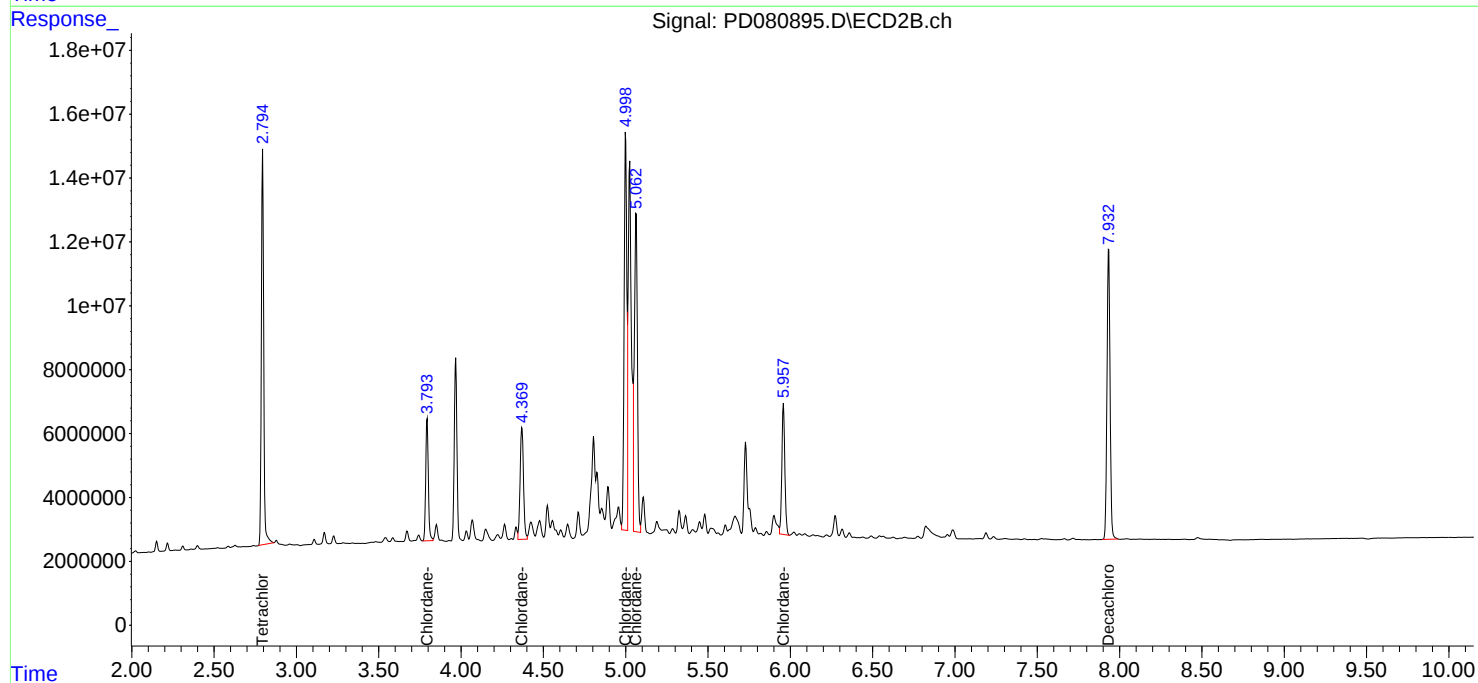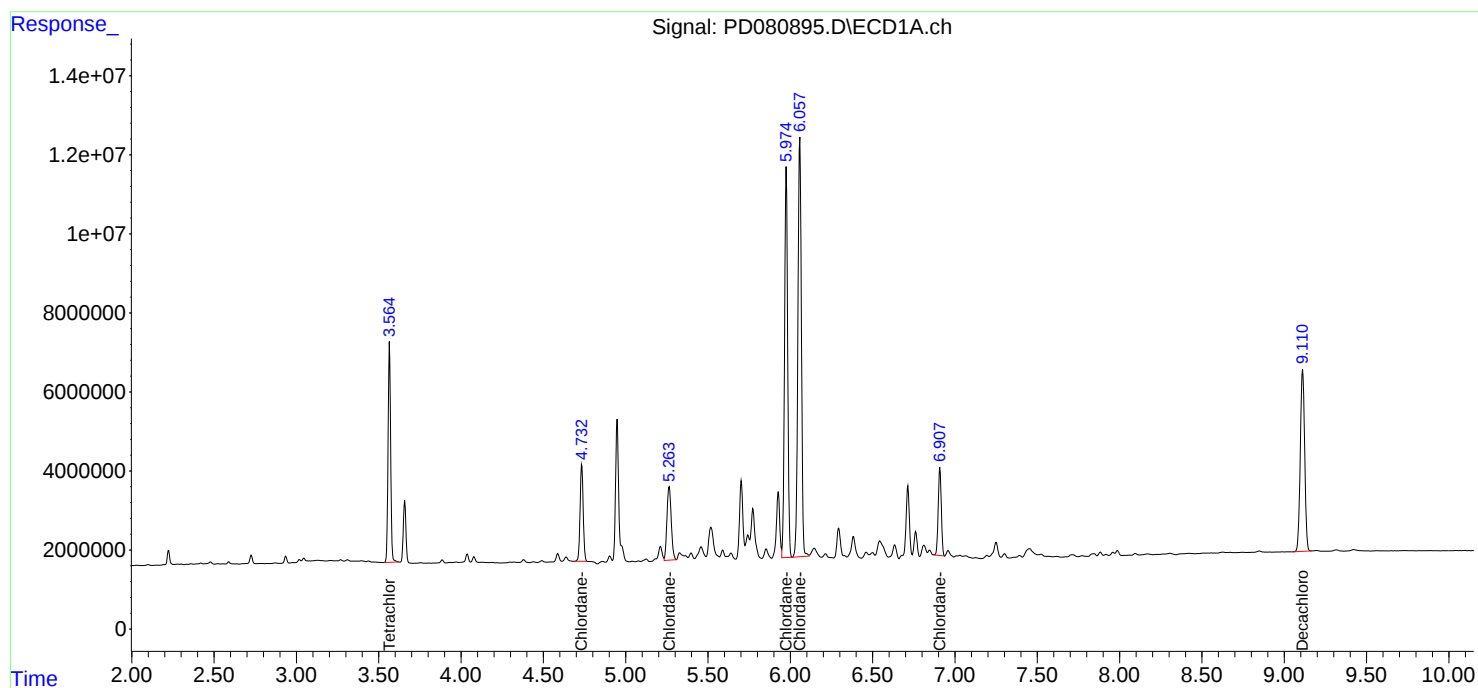


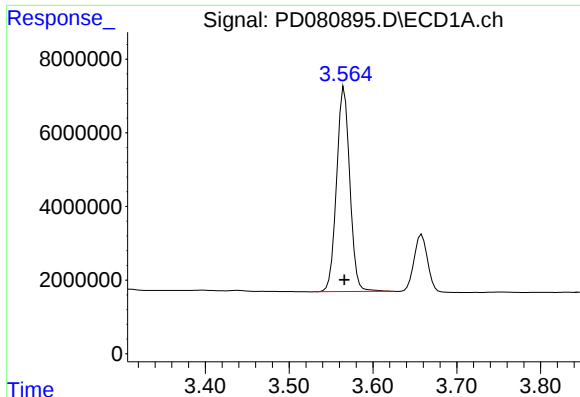

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 60898943
Conc: 42.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

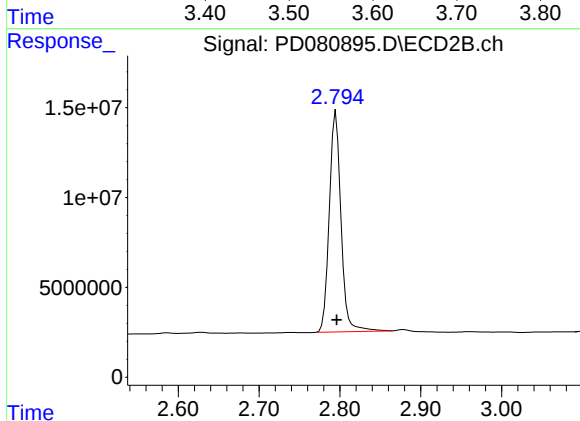


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.000 min
Response: 123955635
Conc: 51.82 ng/ml

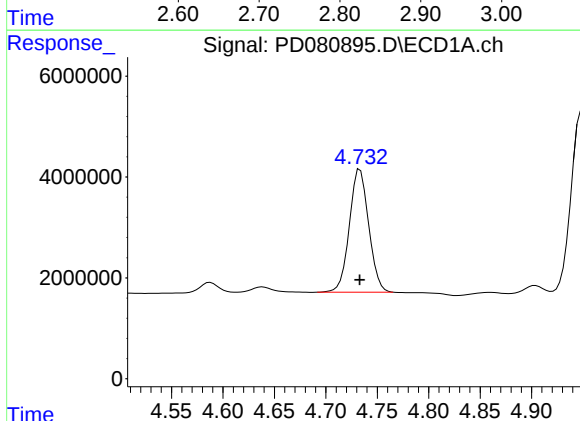


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 31926052
Conc: 413.49 ng/ml

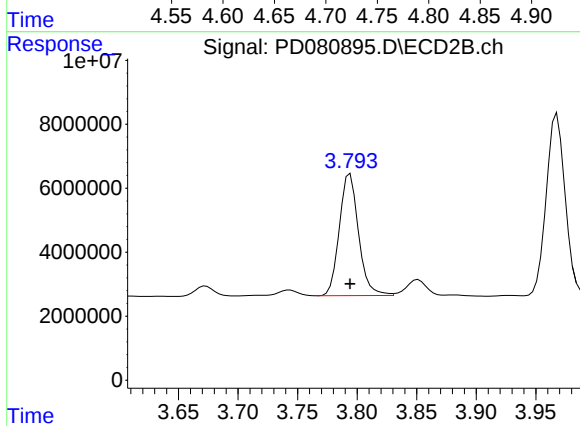

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 42723653
Conc: 420.12 ng/ml

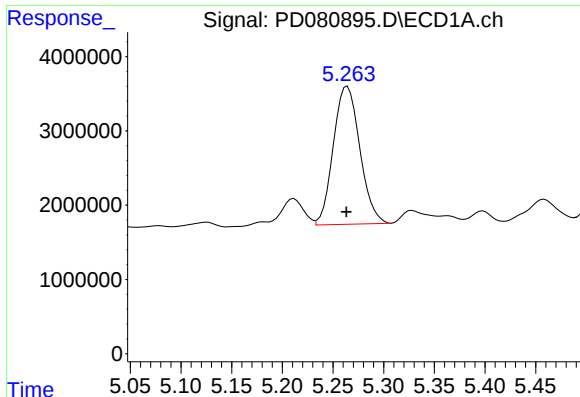

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.001 min
Response: 33768152
Conc: 407.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

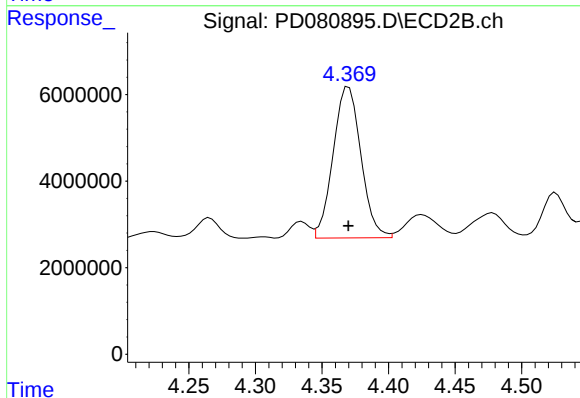


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 50769747
Conc: 414.21 ng/ml

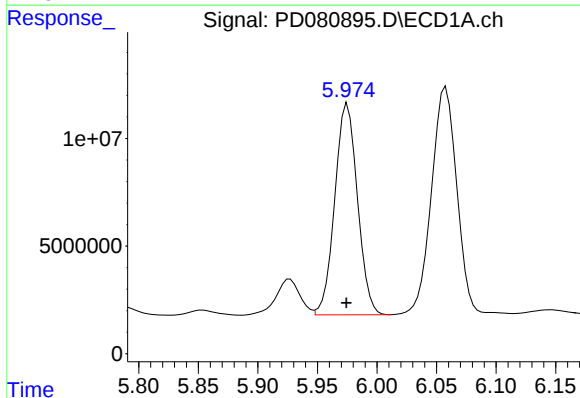


#25 Chlordane-3

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 130058273
Conc: 411.85 ng/ml

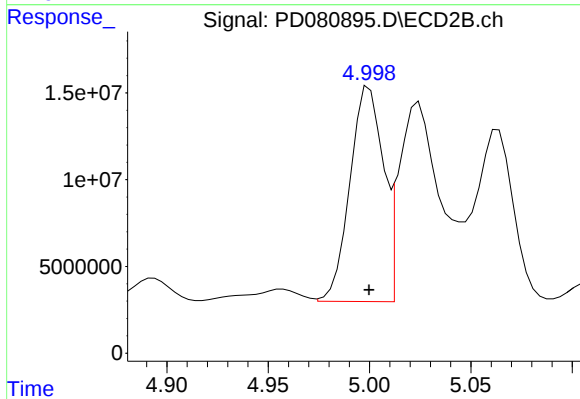

#25 Chlordane-3


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 140846240
Conc: 419.67 ng/ml

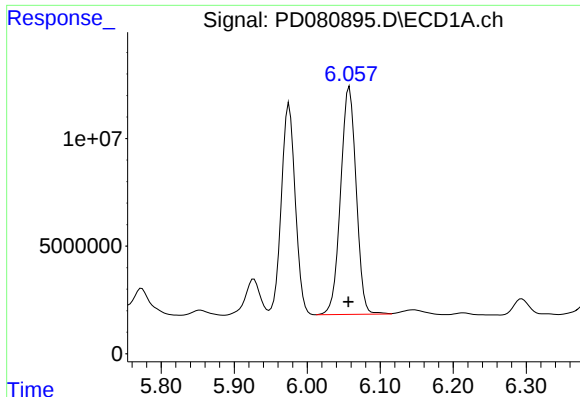

#26 Chlordane-4


R.T.: 6.058 min
Delta R.T.: 0.001 min
Response: 156439887
Conc: 410.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

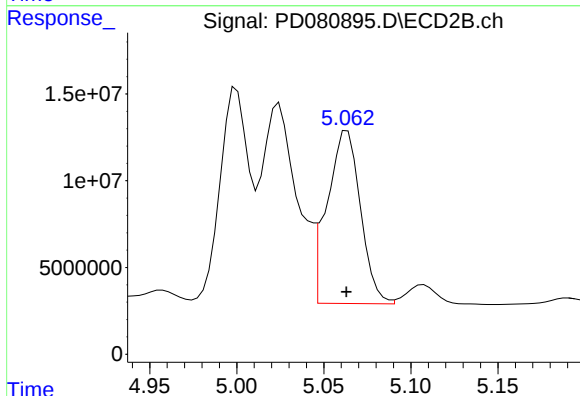


#26 Chlordane-4

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 132658600
Conc: 417.57 ng/ml

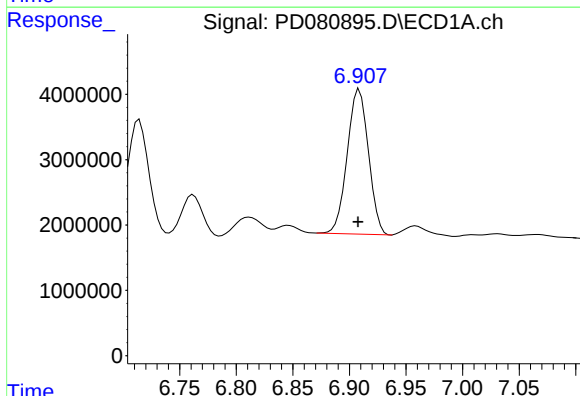


#27 Chlordane-5

R.T.: 6.909 min
Delta R.T.: 0.001 min
Response: 28954402
Conc: 414.76 ng/ml

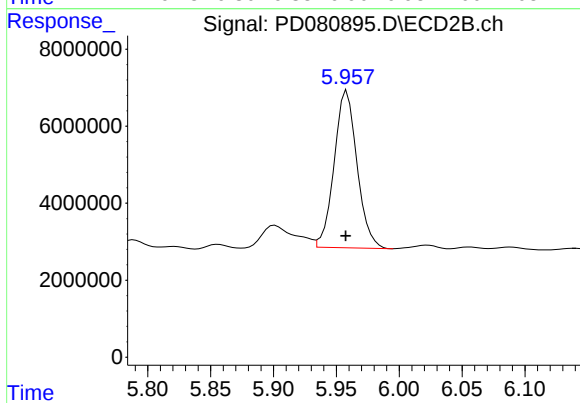

#27 Chlordane-5


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 51672416
Conc: 426.19 ng/ml

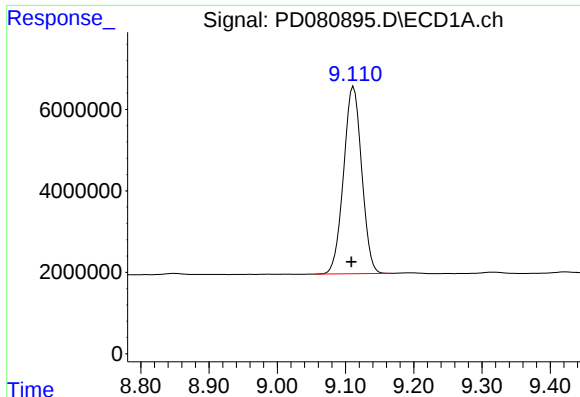

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.003 min
Response: 84723549
Conc: 42.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

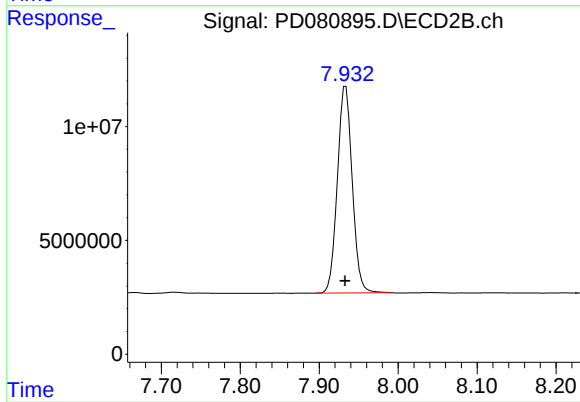

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 118817892
Conc: 44.61 ng/ml