

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
 Data File : PD080906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2024 17:06
 Operator : AR\AJ
 Sample : P1242-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TR-04-012424

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/26/2024
 Supervised By : Ankita Jodhani 01/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 21:53:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	15926641	28876120	11.219	12.071
28)	SA Decachlor...	9.112	7.933	21628683	26881478	10.747	10.092
Target Compounds							
12)	B 4,4'-DDE	6.224	5.251	665326	1153897	0.327	0.377m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012524\
Data File : PD080906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2024 17:06
Operator : AR\AJ
Sample : P1242-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TR-04-012424


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/26/2024
Supervised By : Ankita Jodhani 01/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 21:53:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

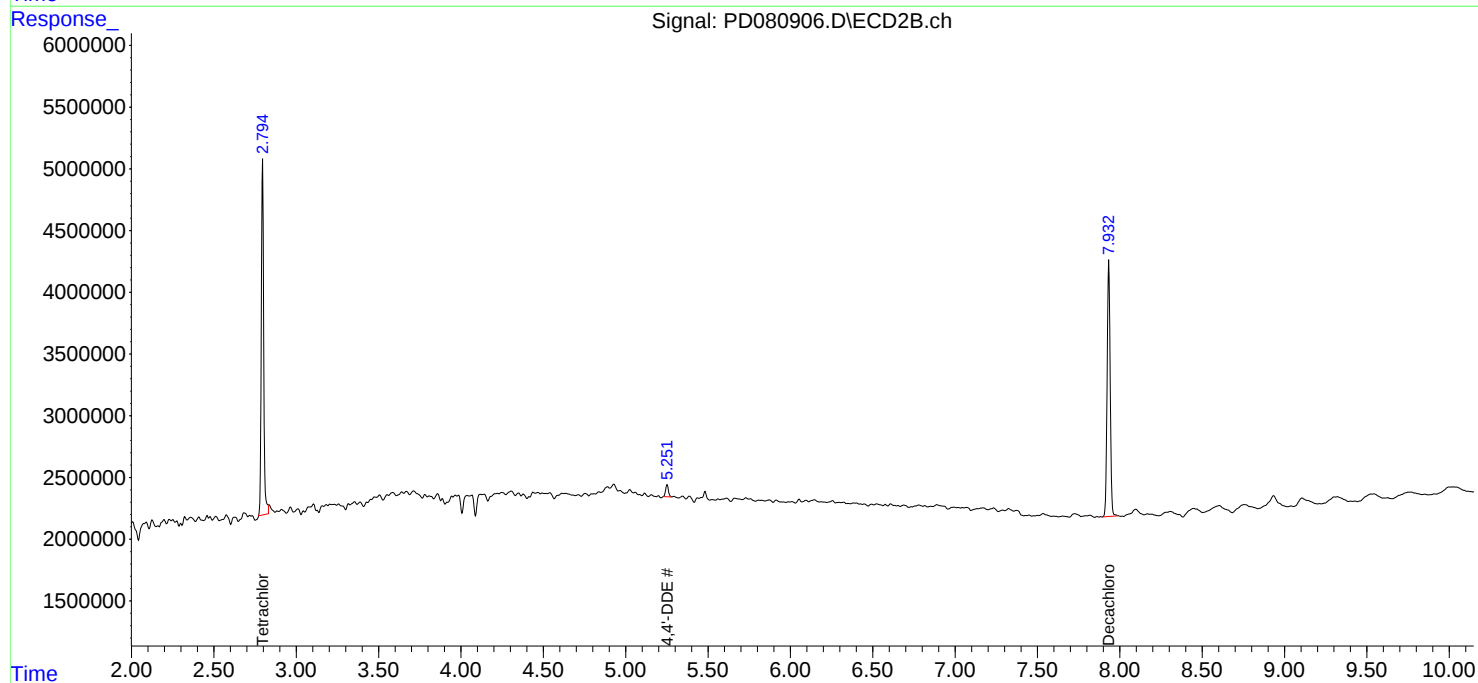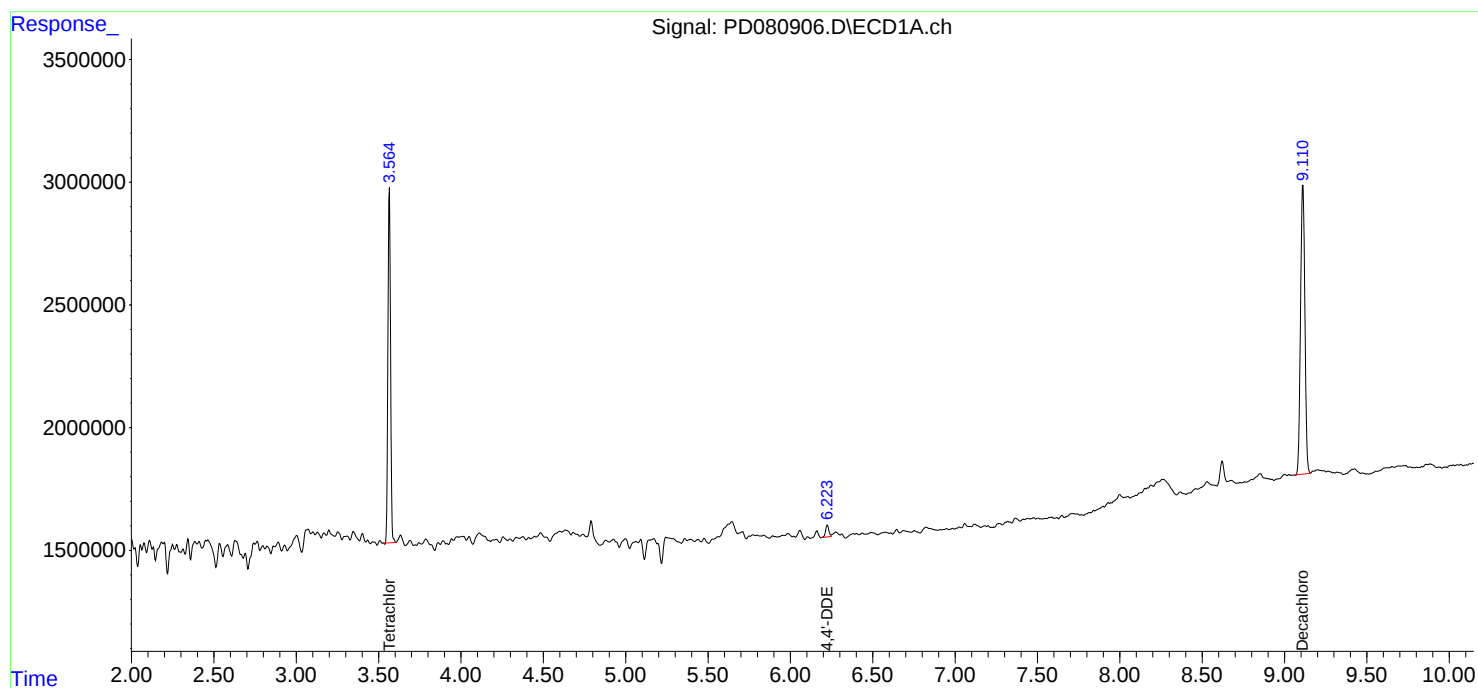

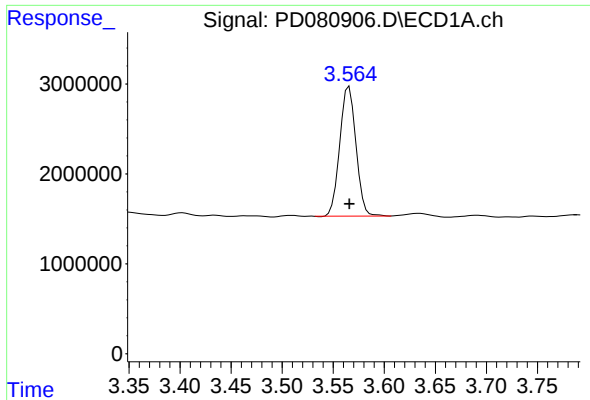


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 15926641
Conc: 11.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
TR-04-012424


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/26/2024
Supervised By :Ankita Jodhani 01/26/2024

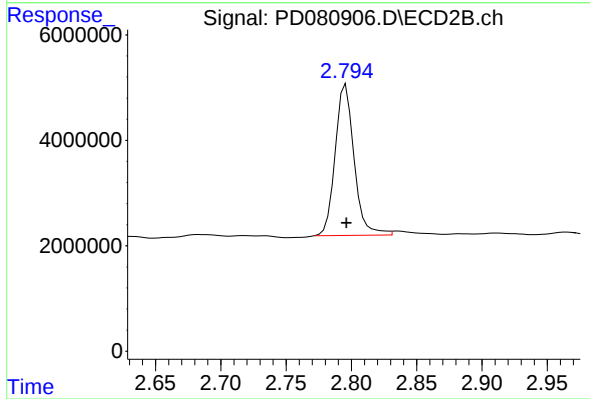


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 28876120
Conc: 12.07 ng/ml

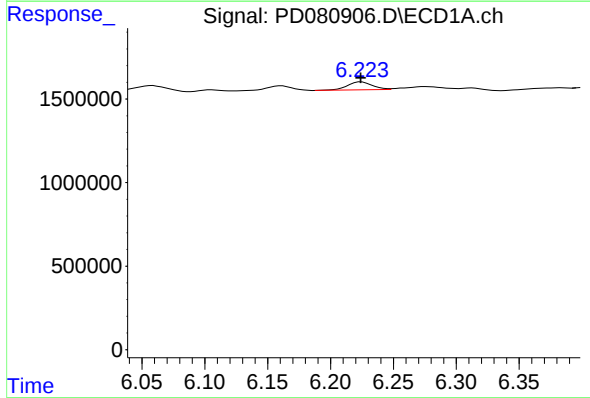


#12 4,4'-DDE

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 665326
Conc: 0.33 ng/ml

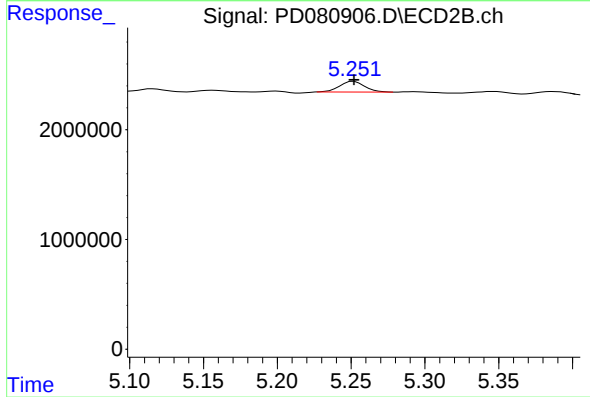

#12 4,4'-DDE

R.T.: 5.251 min
Delta R.T.: -0.001 min
Response: 1153897
Conc: 0.38 ng/ml m

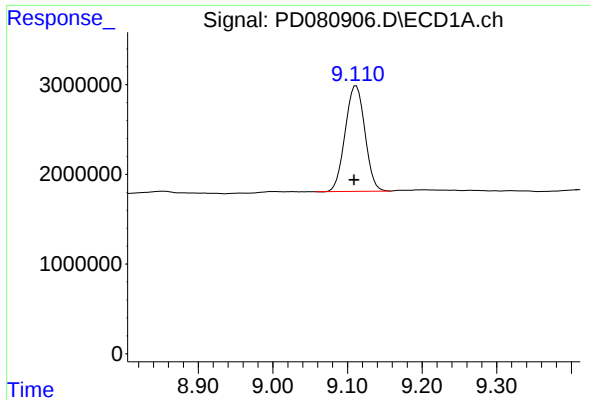

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.003 min
Response: 21628683
Conc: 10.75 ng/ml

Instrument :

ECD_D

ClientSampleId :


TR-04-012424

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 01/26/2024

Supervised By :Ankita Jodhani 01/26/2024

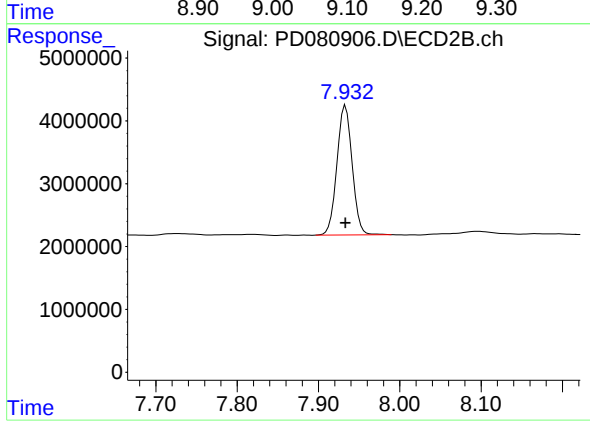

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 26881478
Conc: 10.09 ng/ml