

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012621\
 Data File : PD061051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2021 11:15
 Operator : DD\AJ
 Sample : M1203-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X2Y86

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 01:28:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 26 00:33:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.019	16718137	188.1E6	16.471	26.289 #
27)	SA Decachlor...	8.280	9.106	37614043	236.2E6	29.852	34.789
Target Compounds							
2)	A alpha-BHC	3.938	4.411	85244889	652.2E6	57.182	58.942
3)	MA gamma-BHC...	4.223	4.697	64348040	500.0E6	43.980	49.293
4)	MA Heptachlor	4.528	5.208	55742636	418.9E6	36.885	39.731
5)	MB Aldrin	4.779	5.515	34352869	251.3E6	24.104	25.597
6)	B beta-BHC	4.473	4.865	24930916	181.0E6	39.991	42.331
7)	B delta-BHC	4.680	5.084	42977279	327.9E6	30.541	32.167
8)	B Heptachlo...	5.224	5.902	41301587	253.4E6	30.349	29.238
9)	A Endosulfan I	5.565	6.260	68376243	468.0E6	52.141	54.322
10)	B trans-Chl...	5.452	6.136	50220612	333.3E6	35.506	35.449
11)	B cis-Chlor...	5.511	6.210	66566327	449.7E6	48.511	50.623
12)	B 4,4'-DDE	5.675	6.365	89984211	614.0E6	63.911	69.134
13)	MA Dieldrin	5.812	6.518	102.0E6	445.5E6	69.462	47.919 #
14)	MA Endrin	6.069	6.736	140.9E6	447.5E6	113.352	60.580 #
16)	A 4,4'-DDD	6.192	6.855	54968072	373.5E6	46.831	52.493
17)	MA 4,4'-DDT	6.435	7.155	112.0E6	719.6E6	91.480	99.093
19)	B Endosulfa...	6.725	7.291	33442656	252.8E6	32.048	35.859

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012621\
Data File : PD061051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2021 11:15
Operator : DD\AJ
Sample : M1203-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 01:28:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012521CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jan 26 00:33:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

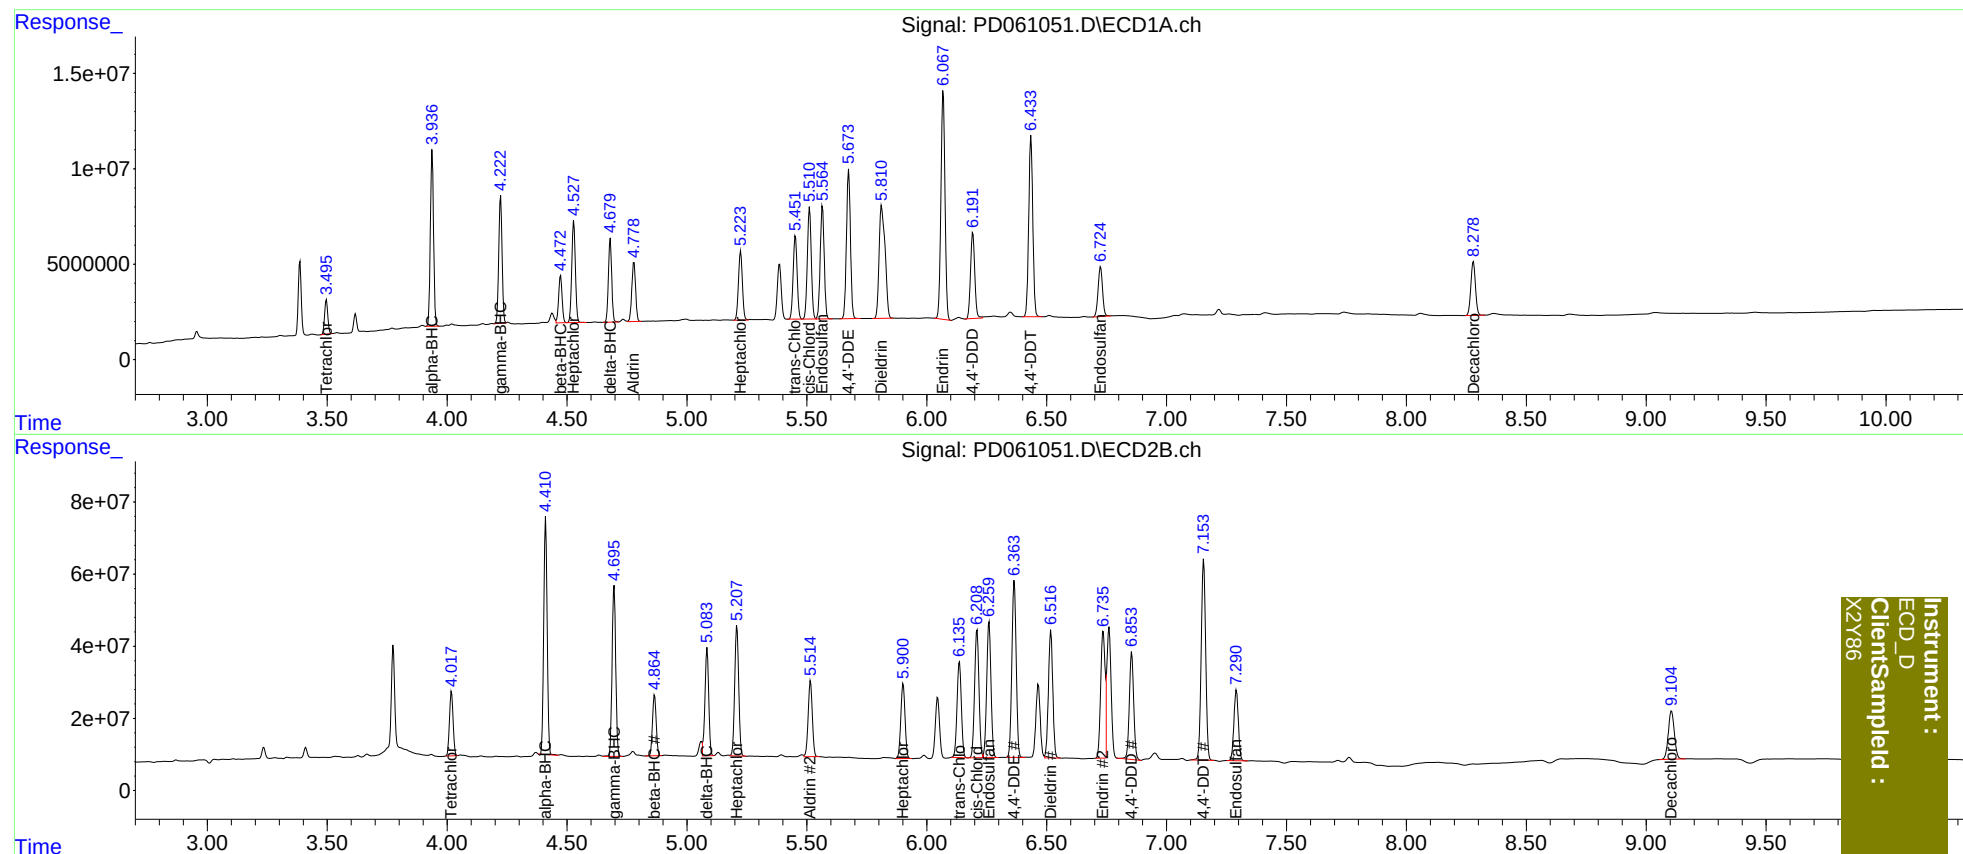

Instrument :
ECD_D
ClientSampled :
X2Y86