

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
 Data File : PD067813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 13:40
 Operator : AR\AJ
 Sample : N1230-13MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q55MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/27/2022
 Supervised By : Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 05:35:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	3.960	35243538	151.7E6	15.556	18.718
27)	SA Decachlor...	8.148	9.010	25368266	140.7E6	26.487	27.845
Target Compounds							
2)	A alpha-BHC	3.866	4.352	129.6E6	385.8E6	39.099	36.812
3)	MA gamma-BHC...	4.147	4.637	125.1E6	392.0E6	39.536	39.730
4)	MA Heptachlor	4.439	5.136	130.2E6	342.2E6	42.002	38.266
5)	MB Aldrin	4.683	5.438	130.3E6	323.5E6	41.682m	38.581m
6)	B beta-BHC	4.396	4.816	52913359	169.2E6	39.373	36.581
7)	B delta-BHC	4.597	5.029	59617666	182.3E6	20.157	19.448m
8)	B Heptachlo...	5.124	5.828	118.2E6	289.6E6	42.504	34.515
9)	A Endosulfan I	5.459	6.185	107.6E6	272.9E6	40.640	37.986
10)	B trans-Chl...	5.347	6.061	117.7E6	296.0E6	41.692	39.572m
11)	B cis-Chlor...	5.405	6.132	115.3E6	289.5E6	42.076	39.288m
12)	B 4,4'-DDE	5.569	6.293	226.0E6	569.3E6	89.995	84.319m
13)	MA Dieldrin	5.702	6.443	241.5E6	592.8E6	85.693	78.836
14)	MA Endrin	5.957	6.660	208.5E6	513.7E6	93.605m	92.083m
15)	B Endosulfa...	6.230	6.876	180.7E6	508.7E6	83.525m	80.525
16)	A 4,4'-DDD	6.082	6.789	175.0E6	471.4E6	87.823m	80.198
17)	MA 4,4'-DDT	6.322	7.086	176.4E6	494.0E6	85.681	85.033
18)	B Endrin al...	6.400	7.000	143.3E6	415.7E6	91.987	87.959m
19)	B Endosulfa...	6.611	7.225	136.1E6	427.7E6	74.921	73.305
20)	A Methoxychlor	6.869	7.549	388.5E6	1150.8E6	440.531	417.381
21)	B Endrin ke...	7.102	7.696	162.0E6	553.9E6	85.157m	83.655m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
Data File : PD067813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 13:40
Operator : AR\AJ
Sample : N1230-13MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 05:35:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

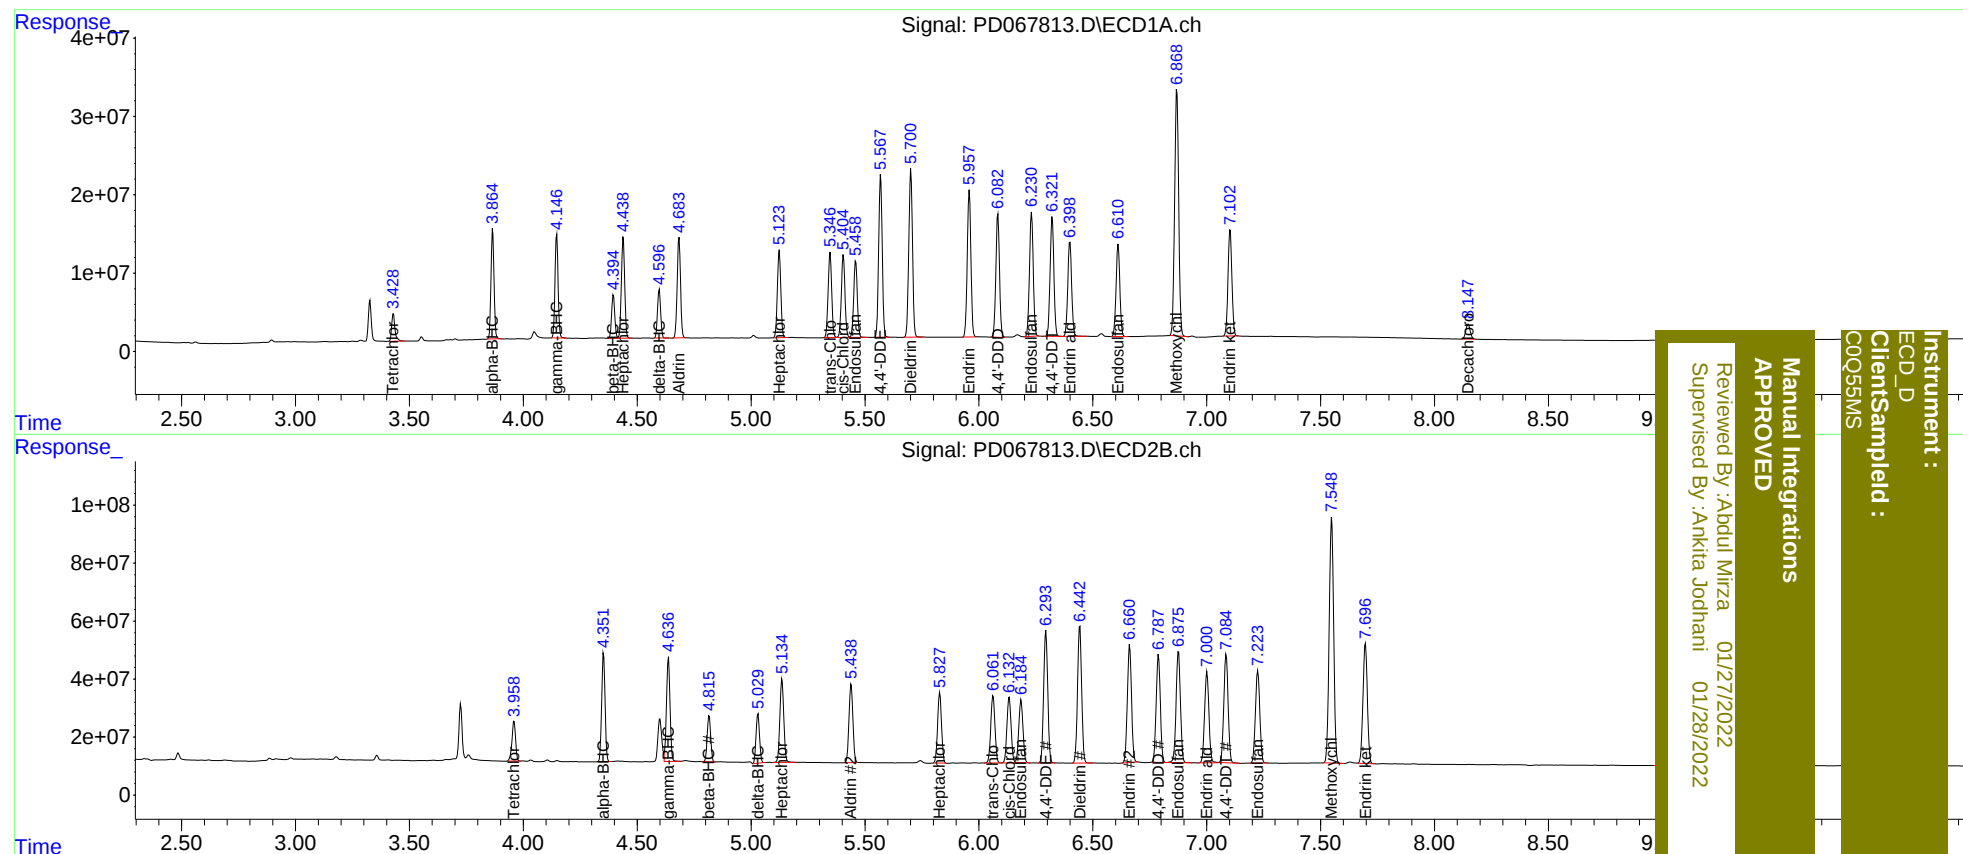

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/27/2022
Supervised By: Ankita Jodhani 01/28/2022

Instrument :
ECD_D
Client Sampled :
C0055MS