

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
 Data File : PD067814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 13:54
 Operator : AR\AJ
 Sample : N1230-14MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q55MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/27/2022
 Supervised By : Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 05:44:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	3.958	35515264	154.6E6	15.676	19.077m
2)	SA Decachlor...	8.149	9.010	25662827	141.9E6	26.795	28.080
Target Compounds							
2)	A alpha-BHC	3.866	4.353	129.8E6	387.0E6	39.156	36.932
3)	MA gamma-BHC...	4.148	4.638	124.8E6	395.3E6	39.465	40.060
4)	MA Heptachlor	4.440	5.137	130.3E6	345.8E6	42.039	38.669
5)	MB Aldrin	4.684	5.440	129.5E6	323.9E6	41.424	38.622
6)	B beta-BHC	4.397	4.815	52963263	171.8E6	39.410	37.149m
7)	B delta-BHC	4.598	5.030	58963745	179.9E6	19.936	19.186
8)	B Heptachlo...	5.124	5.827	118.0E6	283.2E6	42.458	33.759m
9)	A Endosulfan I	5.460	6.185	107.5E6	275.2E6	40.604	38.303
10)	B trans-Chl...	5.348	6.063	117.9E6	294.1E6	41.751	39.325
11)	B cis-Chlor...	5.406	6.134	115.3E6	283.6E6	42.052	38.483
12)	B 4,4'-DDE	5.570	6.294	224.4E6	563.6E6	89.329	83.475
13)	MA Dieldrin	5.702	6.443	240.7E6	595.8E6	85.381	79.232
14)	MA Endrin	5.959	6.662	206.7E6	522.6E6	92.765	93.680
15)	B Endosulfa...	6.232	6.877	179.9E6	511.6E6	83.178	80.994
16)	A 4,4'-DDD	6.083	6.789	173.2E6	473.3E6	86.931m	80.522
17)	MA 4,4'-DDT	6.323	7.086	176.1E6	495.3E6	85.520	85.247
18)	B Endrin al...	6.401	7.000	142.6E6	417.8E6	91.574	88.410m
19)	B Endosulfa...	6.612	7.224	136.5E6	428.4E6	75.103	73.426
20)	A Methoxychlor	6.869	7.549	389.3E6	1152.0E6	441.408	417.828
21)	B Endrin ke...	7.102	7.695	161.6E6	554.9E6	84.944m	83.795m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
Data File : PD067814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 13:54
Operator : AR\AJ
Sample : N1230-14MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 05:44:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

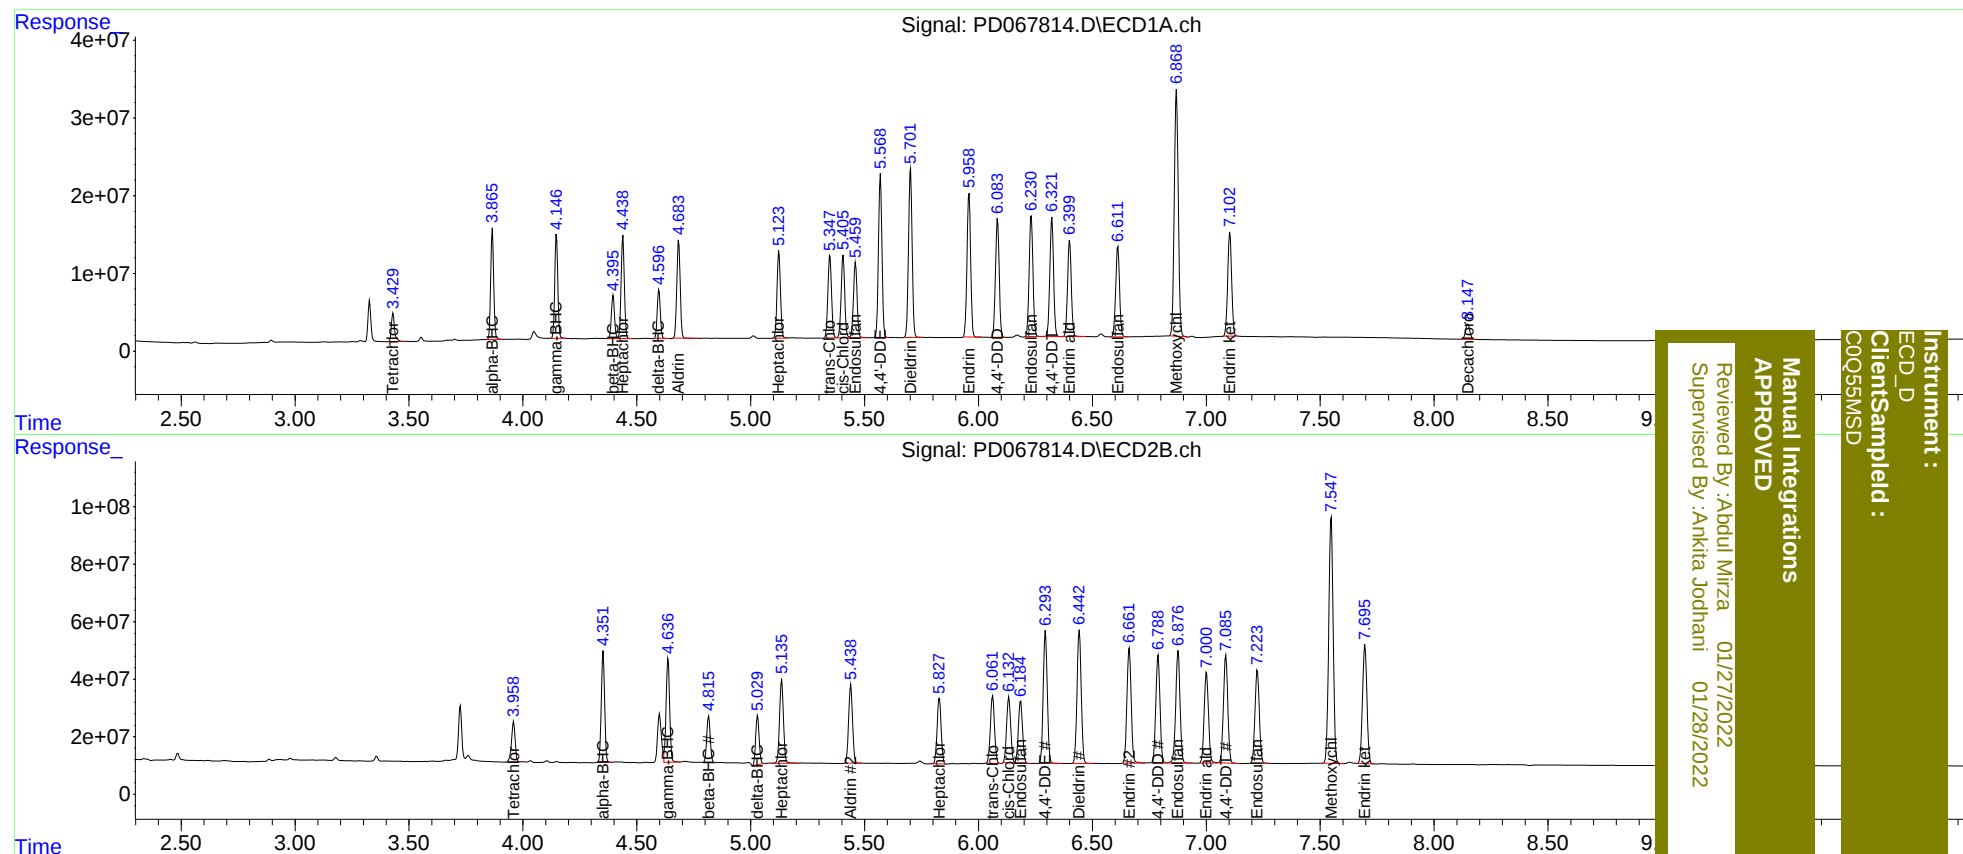

Reviewed By: Abdul Mirza 01/27/2022
Supervised By: Ankita Jodhani 01/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C005MSD