

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
 Data File : PD067817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2022 14:36
 Operator : AR\AJ
 Sample : N1230-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q06

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/27/2022
 Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 05:51:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.430	3.955	31107395	103.5E6	13.730	12.773m
2) SA Decachlor...	8.148	9.009	21359235	121.0E6	22.301	23.952
Target Compounds						
13) MA Dieldrin	5.701	6.441	11341872	30926264	4.024	4.113m
17) MA 4,4'-DDT	6.327	7.076	13770595	7279947	6.687	1.253 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\
Data File : PD067817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2022 14:36
Operator : AR\AJ
Sample : N1230-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 05:51:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

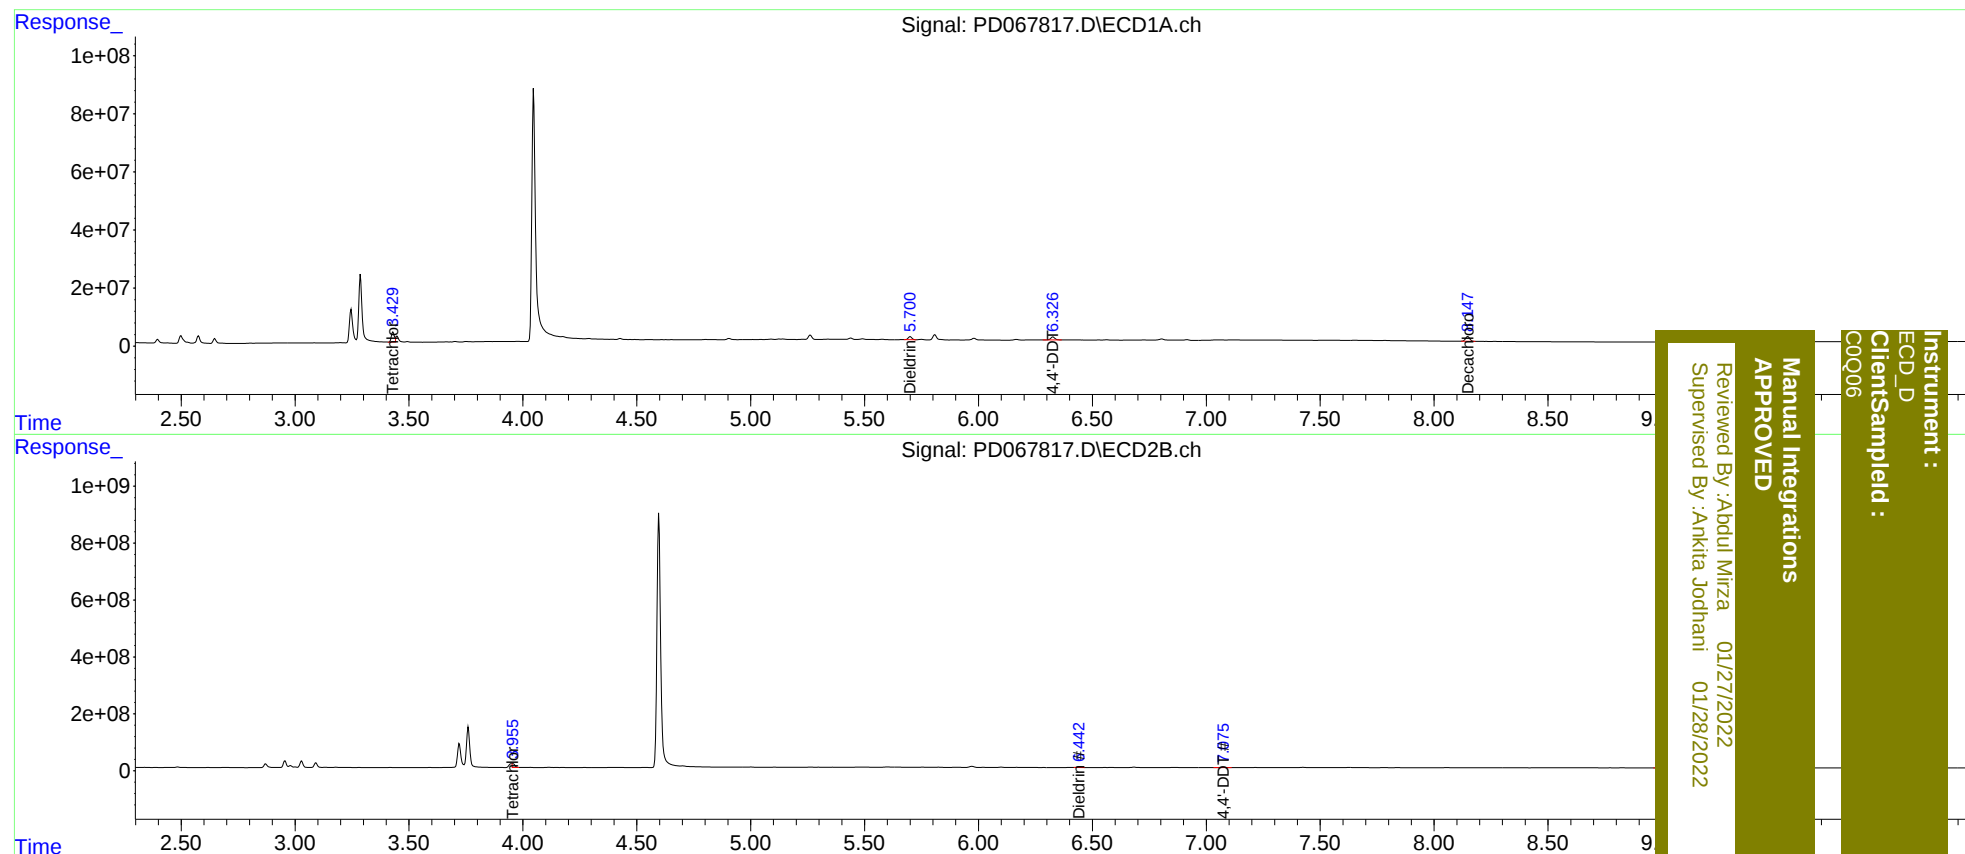

Instrument :
ECD_D
ClientSampled :
C0006

Manual Integrations
APPROVED


Reviewed By : Abdul Mirza 01/27/2022
Supervised By : Ankita Jodhani 01/28/2022

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\PD067817.D
Operator : AR\AJ
Acquired : 26 Jan 2022 14:36 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1230-17
Misc Info :
Vial Number: 22

Instrument :
ECD_D
ClientSampleId :
C0Q06

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/27/2022
Supervised By : Ankita Jodhani 01/28/2022

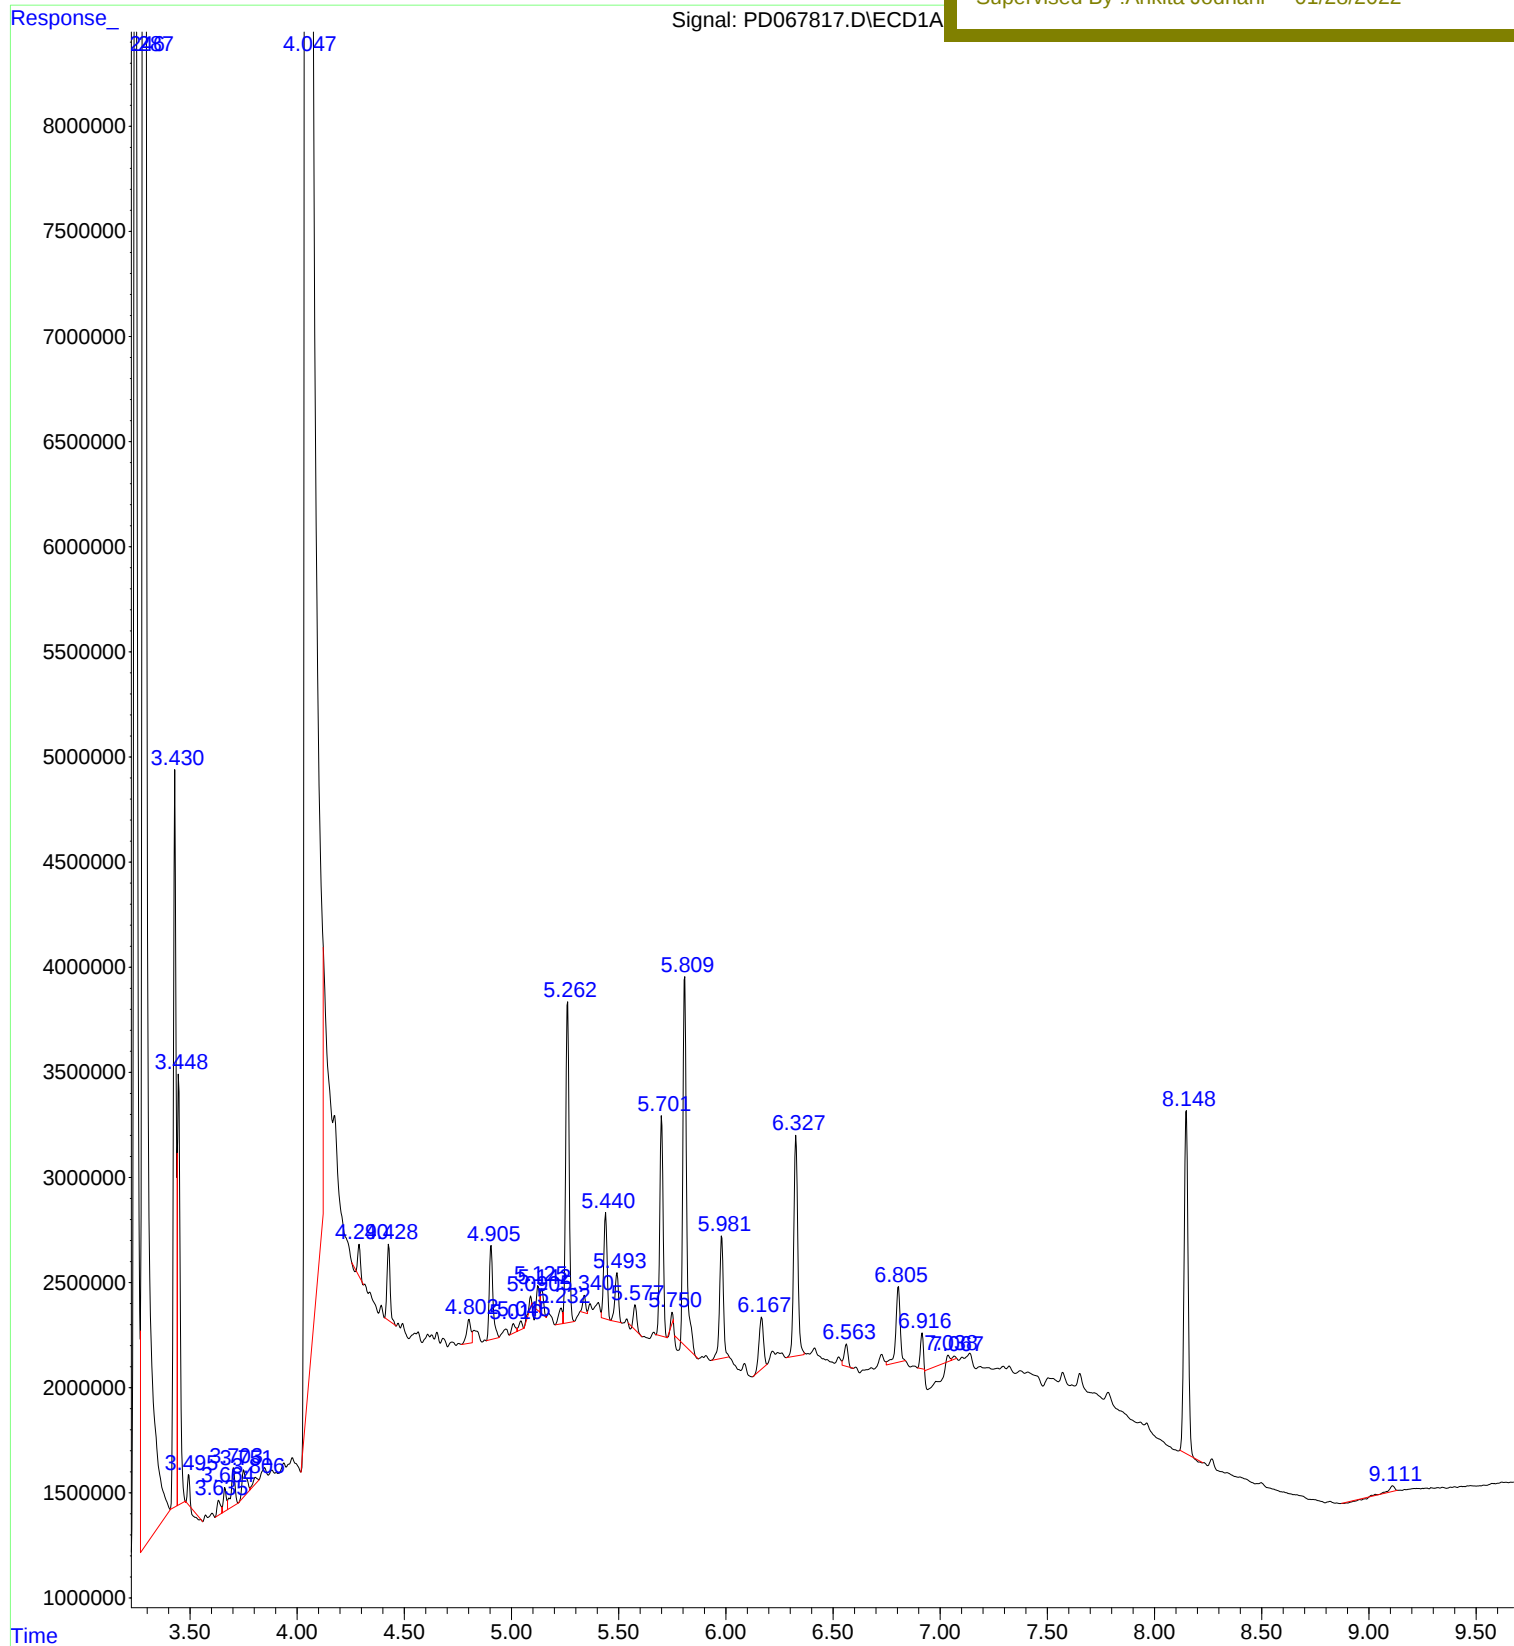

File : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012622\PD067817.D
Operator : AR\AJ
Acquired : 26 Jan 2022 14:36 using AcqMethod ECD_D.M
Instrument : ECD_D
Sample Name: N1230-17
Misc Info :
Vial Number: 22

Instrument :
ECD_D
ClientSampleId :
C0Q06

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/27/2022
Supervised By : Ankita Jodhani 01/28/2022

