

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012623\
 Data File : PD073775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jan 2023 16:05
 Operator : AR\AJ
 Sample : PB150473BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK473

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/26/2023
 Supervised By : Ankita Jodhani 01/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 20:52:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 25 02:23:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.791	49306260	25855639	20.821m	20.369
27)	SA Decachlor...	9.110	7.950	115.3E6	50803176	41.803m	42.212m


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012623\
Data File : PD073775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jan 2023 16:05
Operator : AR\AJ
Sample : PB150473BL
Misc :
ALS Vial : 10 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 20:52:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 25 02:23:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

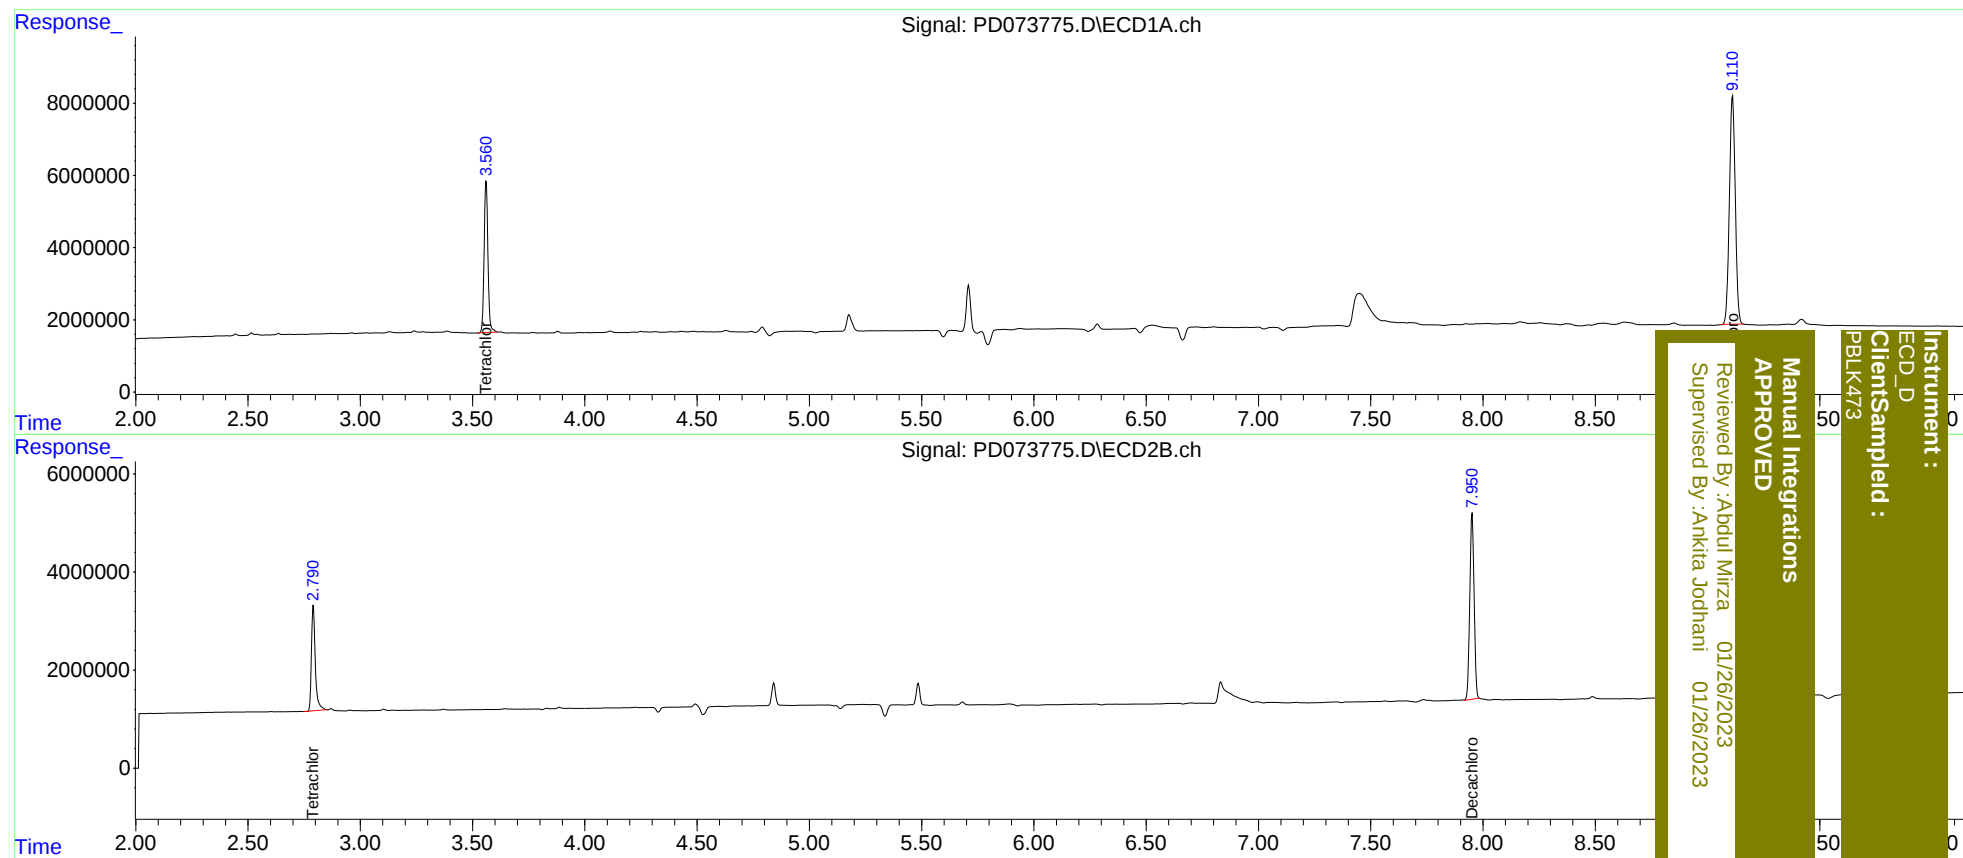

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/26/2023
Supervised By: Ankita Jodhani 01/26/2023

Instrument :
ECD_D
ClientSampled :
PBLK473

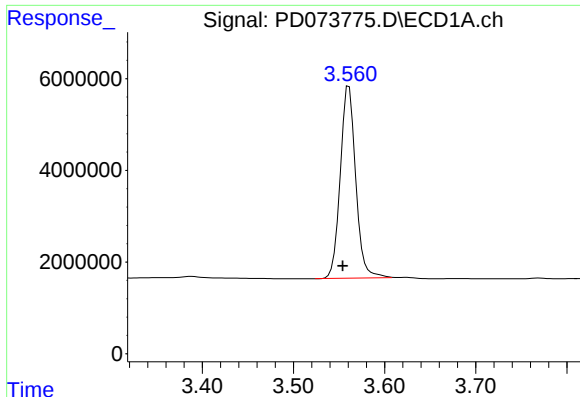


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.006 min
Response: 49306260
Conc: 20.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK473


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/26/2023
Supervised By :Ankita Jodhani 01/26/2023

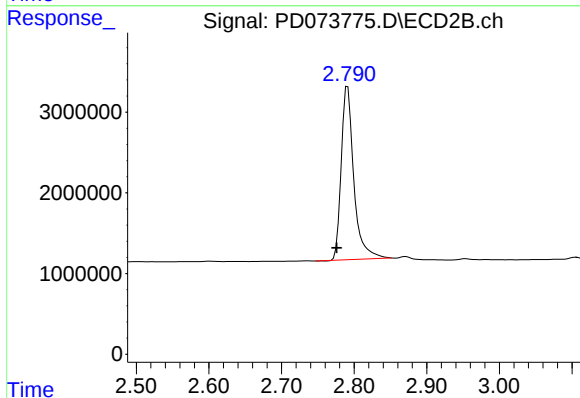


#1 Tetrachloro-m-xylene

R.T.: 2.791 min
Delta R.T.: 0.015 min
Response: 25855639
Conc: 20.37 ng/ml

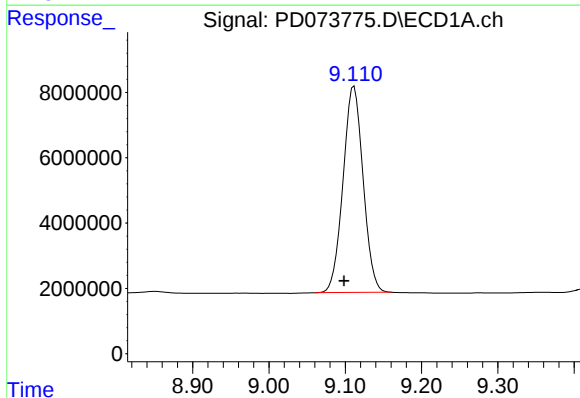

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.012 min
Response: 115333574
Conc: 41.80 ng/ml m

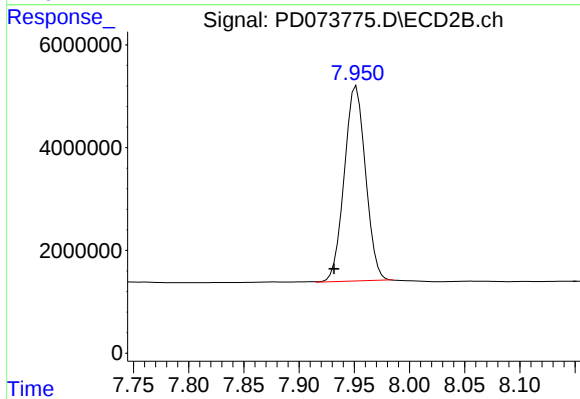

#27 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.019 min
Response: 50803176
Conc: 42.21 ng/ml m