

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
 Data File : PD080918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 10:20
 Operator : AR\AJ
 Sample : P1240-01DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 72-11985DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/29/2024
 Supervised By :Ankita Jodhani 01/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 19:40:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	3657868	6264834	2.577m	2.619
28)	SA Decachlor...	9.112	7.932	3753175	7439707	1.865m	2.793m#
Target Compounds							
8)	B Heptachlo...	5.717	4.750	6753630	7003638	3.016m	2.091 #
10)	B gamma-Chl...	5.977	5.000	47079978	49771863	21.506	15.216 #
11)	B alpha-Chl...	6.060	5.063	72342556	70051071	33.224	21.425 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
Data File : PD080918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 10:20
Operator : AR\AJ
Sample : P1240-01DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
72-11985DL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/29/2024
Supervised By : Ankita Jodhani 01/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 19:40:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

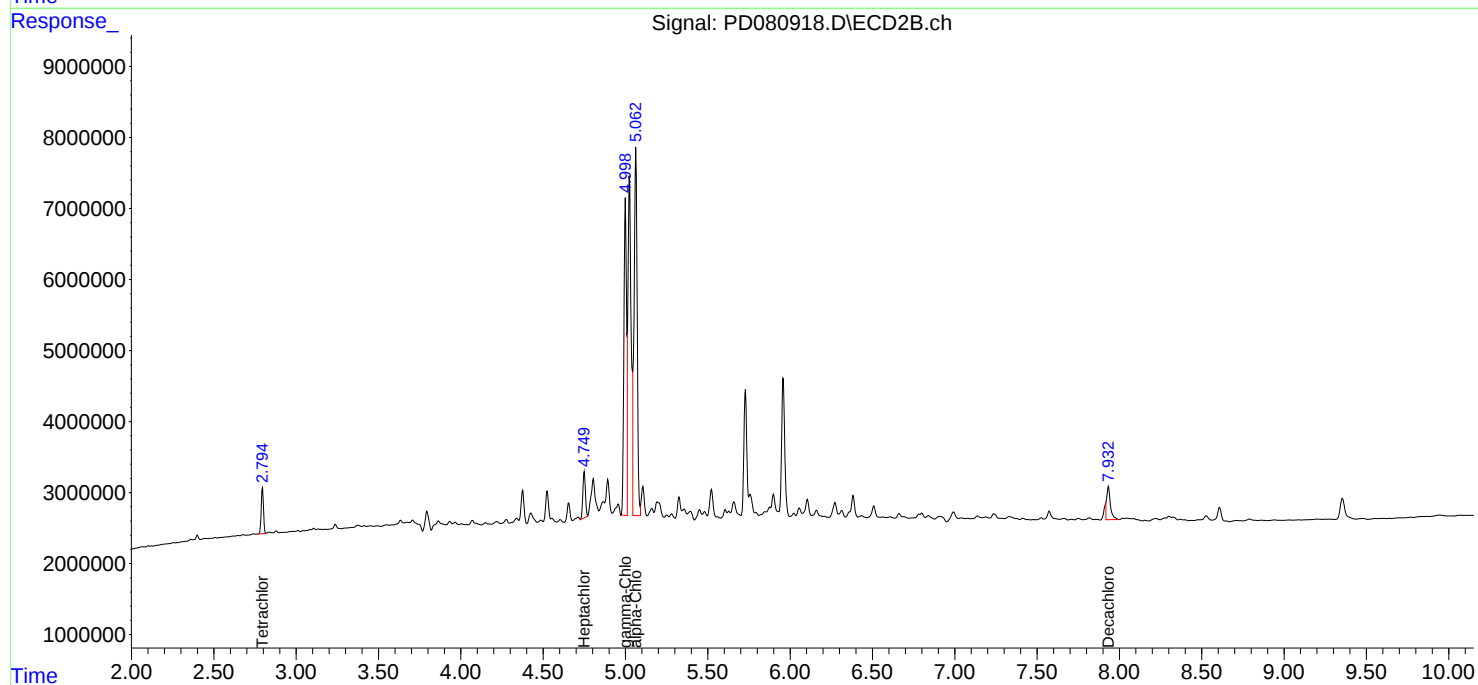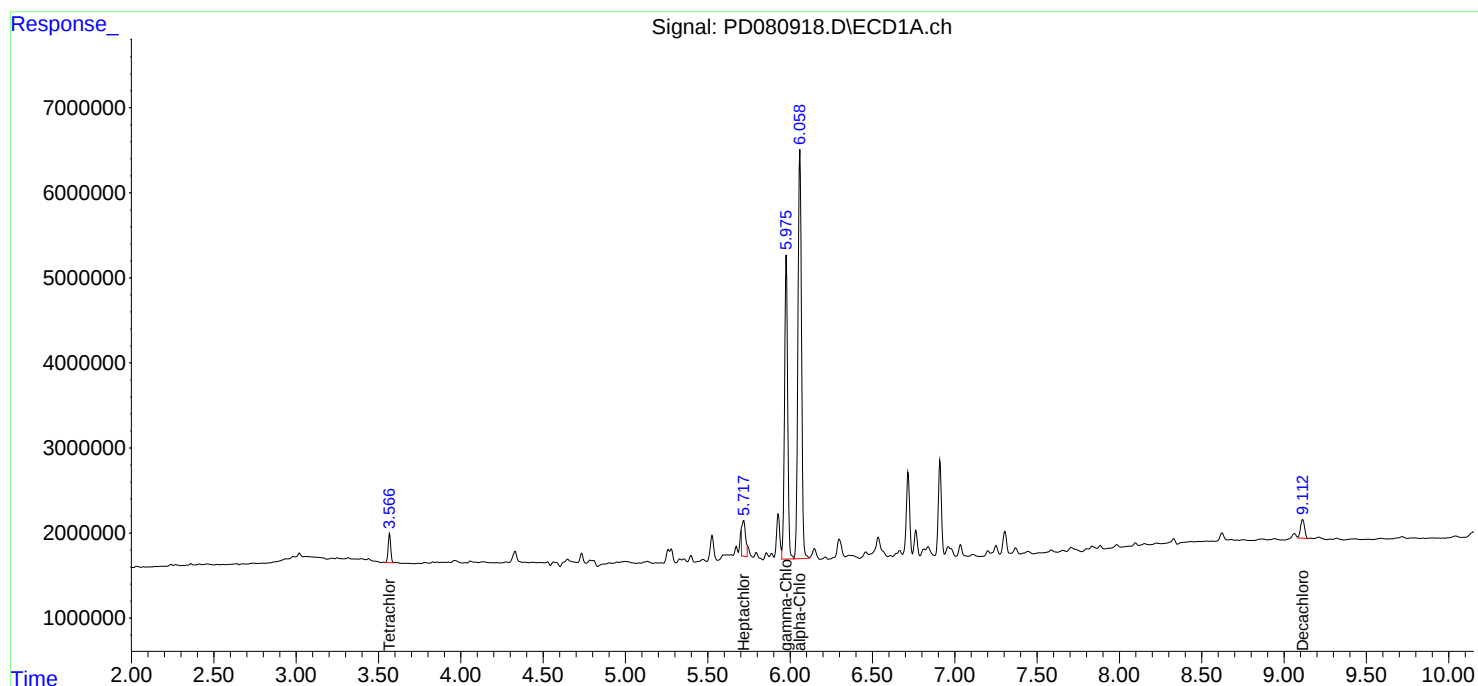

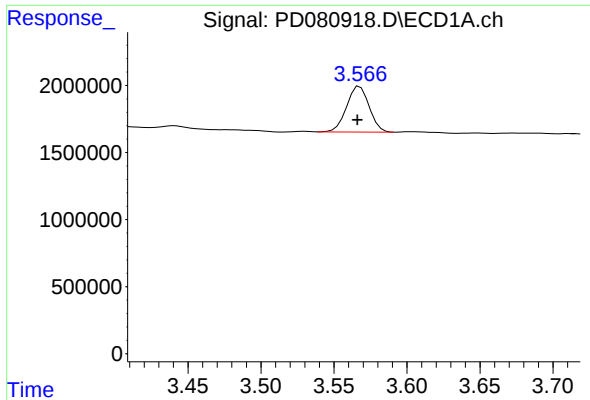


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 3657868
Conc: 2.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
72-11985DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2024
Supervised By :Ankita Jodhani 01/29/2024

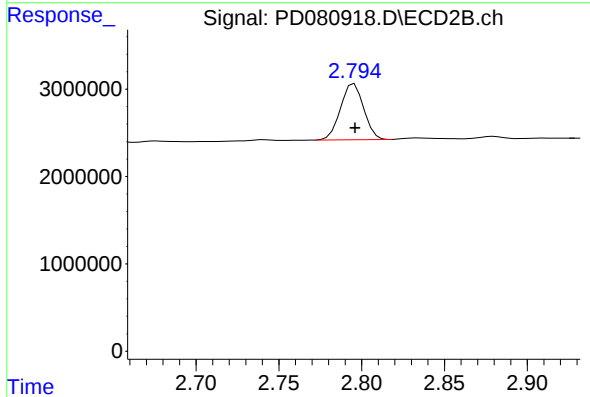


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 6264834
Conc: 2.62 ng/ml

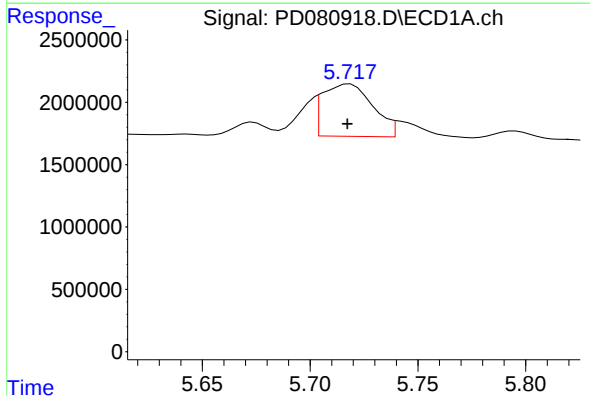


#8 Heptachlor epoxide

R.T.: 5.717 min
Delta R.T.: 0.000 min
Response: 6753630
Conc: 3.02 ng/ml m

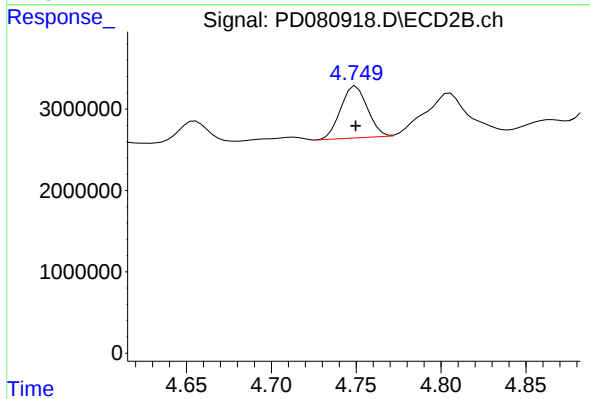

#8 Heptachlor epoxide

R.T.: 4.750 min
Delta R.T.: 0.000 min
Response: 7003638
Conc: 2.09 ng/ml

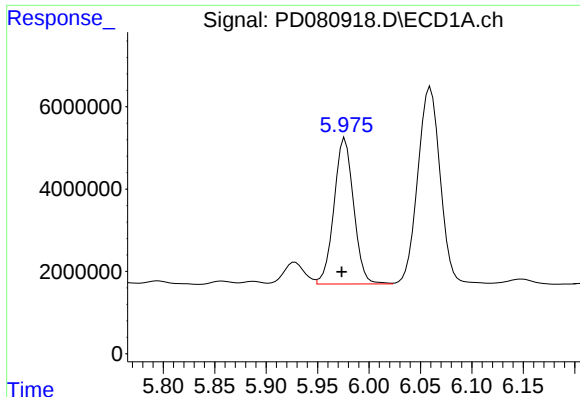


#10 gamma-Chlordane

R.T.: 5.977 min
Delta R.T.: 0.003 min
Response: 47079978
Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
72-11985DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2024
Supervised By :Ankita Jodhani 01/29/2024

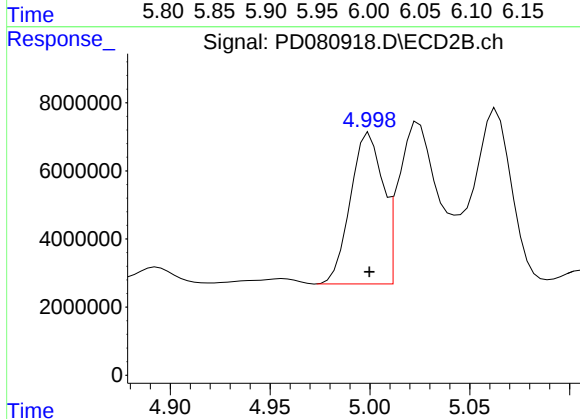


#10 gamma-Chlordane

R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 49771863
Conc: 15.22 ng/ml

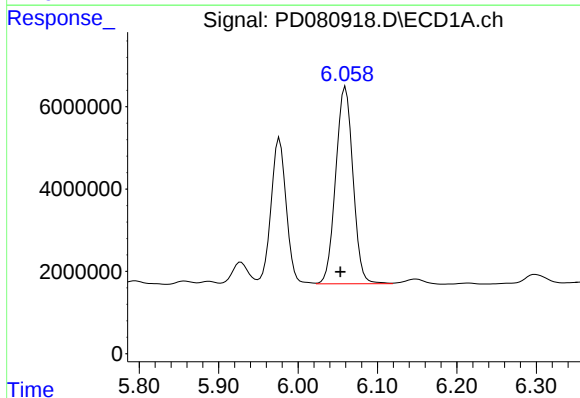


#11 alpha-Chlordane

R.T.: 6.060 min
Delta R.T.: 0.007 min
Response: 72342556
Conc: 33.22 ng/ml

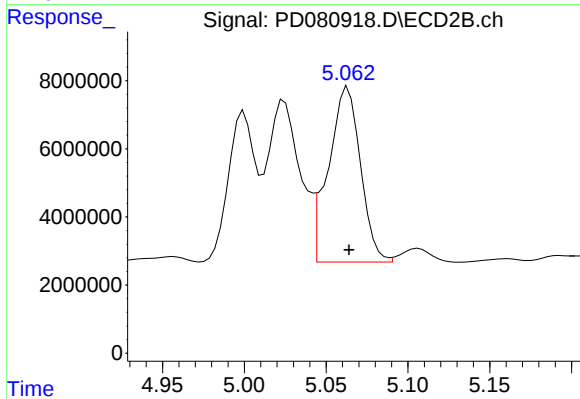

#11 alpha-Chlordane

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 70051071
Conc: 21.43 ng/ml

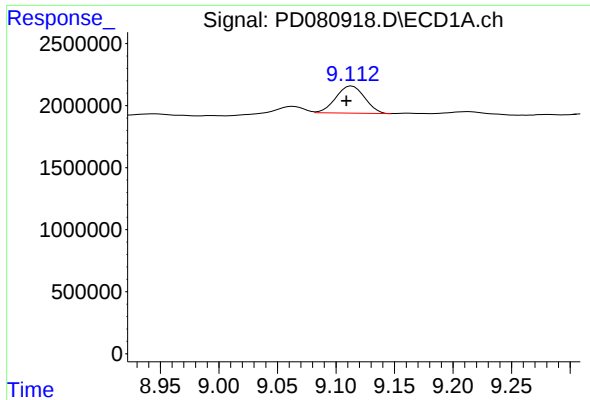


#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.003 min
Response: 3753175
Conc: 1.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
72-11985DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2024
Supervised By :Ankita Jodhani 01/29/2024

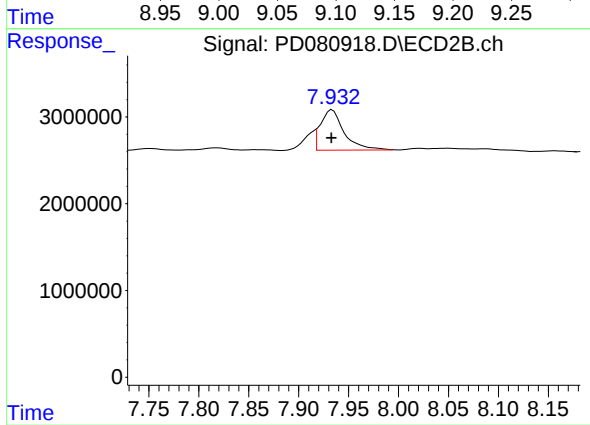

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 7439707
Conc: 2.79 ng/ml m