

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
Data File : PD080931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 15:48
Operator : AR\AJ
Sample : P1234-01DL 100X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
293DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 15:58:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) B	gamma-Chl...	5.975	5.000	77622214	97503276	35.458 29.808
11) B	alpha-Chl...	6.056	5.064	93051321	107.4E6	42.735 32.852



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
Data File : PD080931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 15:48
Operator : AR\AJ
Sample : P1234-01DL 100X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
293DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 15:58:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

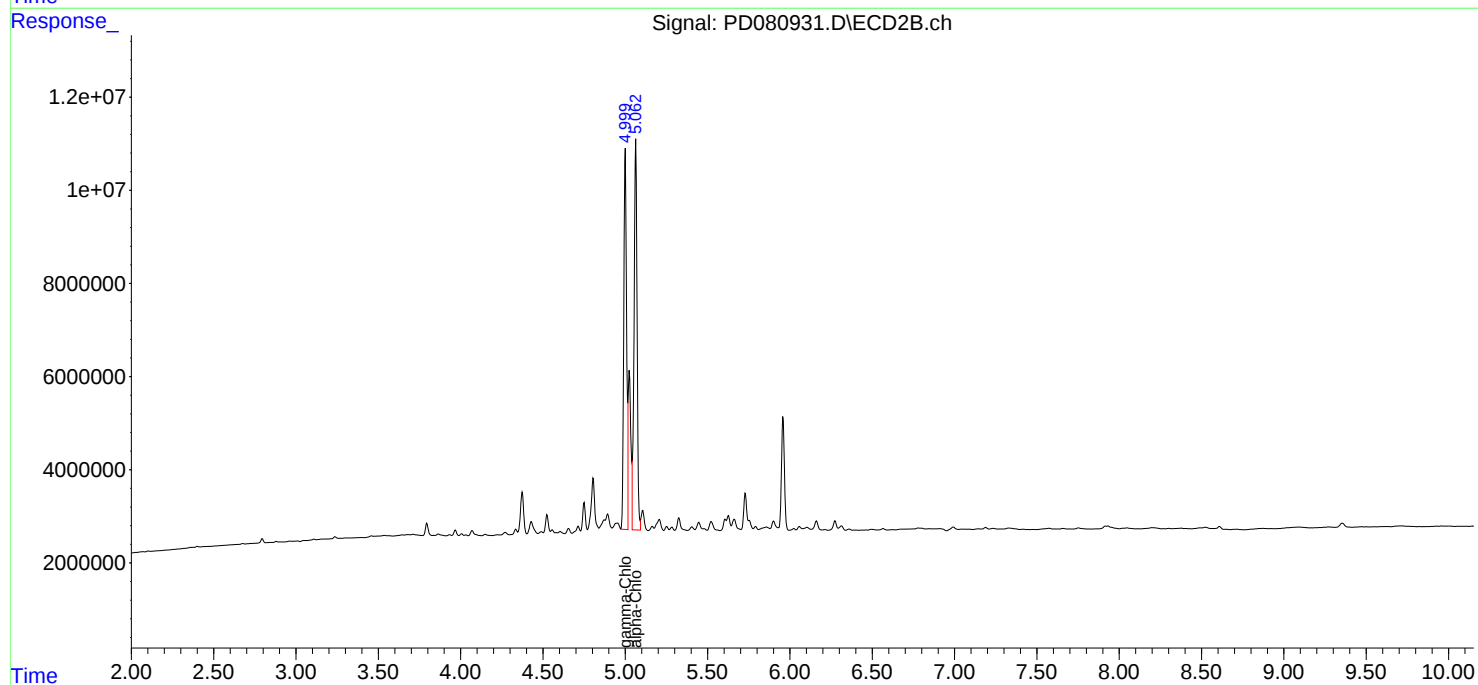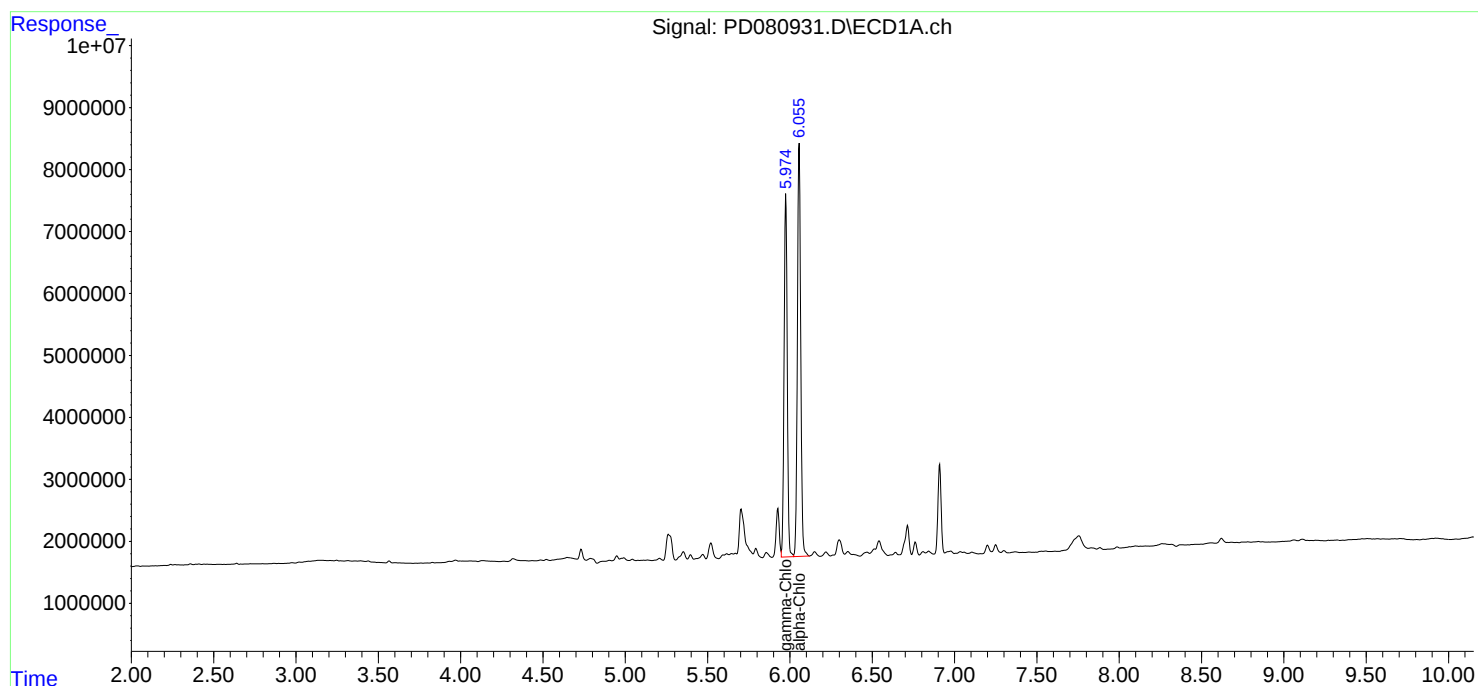


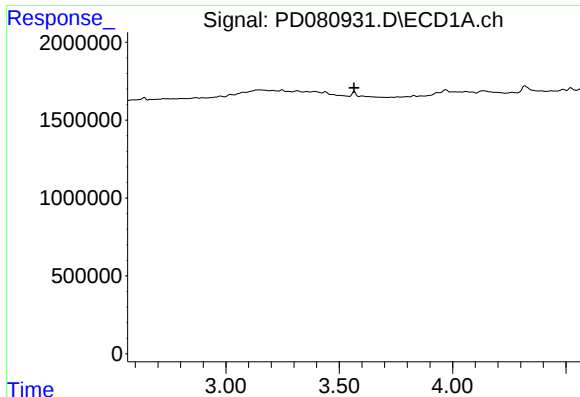

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
293DL

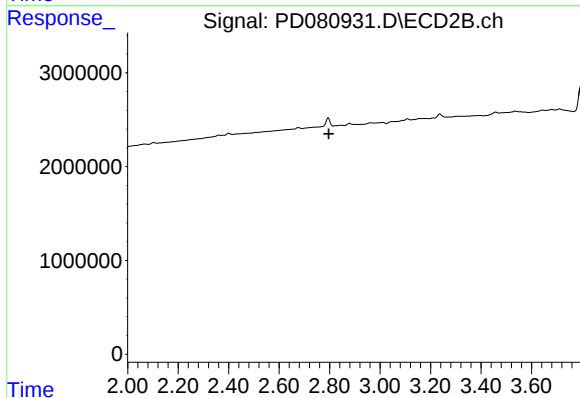


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.796 min
Response: 0
Conc: N.D.

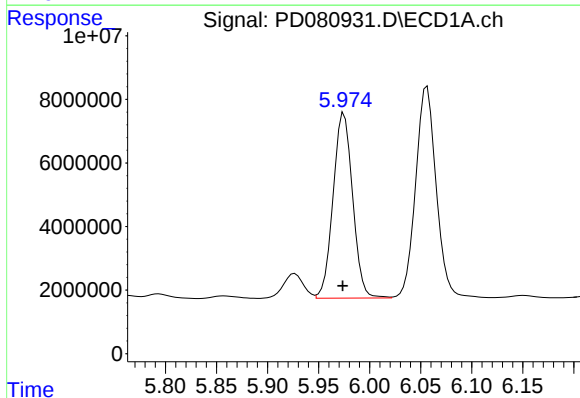


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: 0.001 min
Response: 77622214
Conc: 35.46 ng/ml

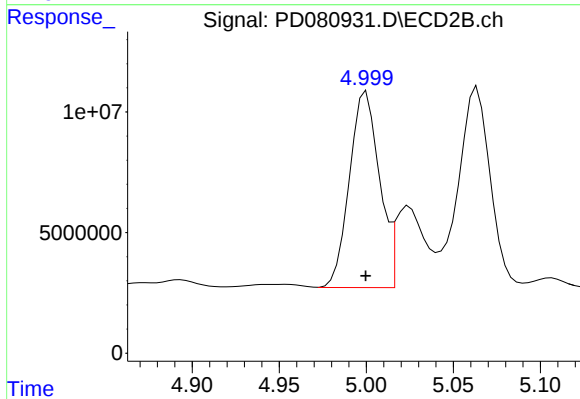

#10 gamma-Chlordane


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 97503276
Conc: 29.81 ng/ml

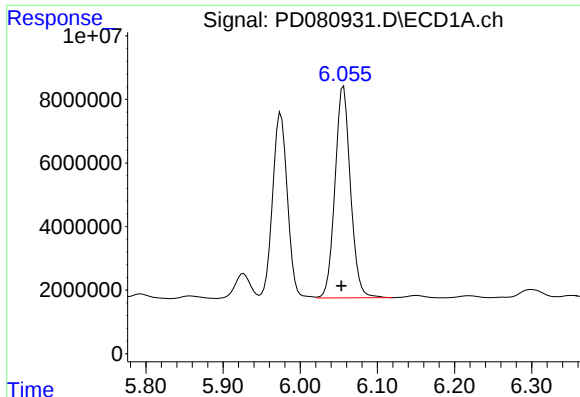

#11 alpha-Chlordane


R.T.: 6.056 min
Delta R.T.: 0.003 min
Response: 93051321
Conc: 42.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
293DL

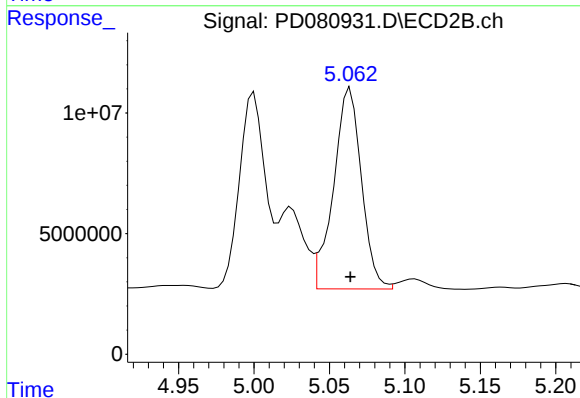


#11 alpha-Chlordane

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 107409461
Conc: 32.85 ng/ml

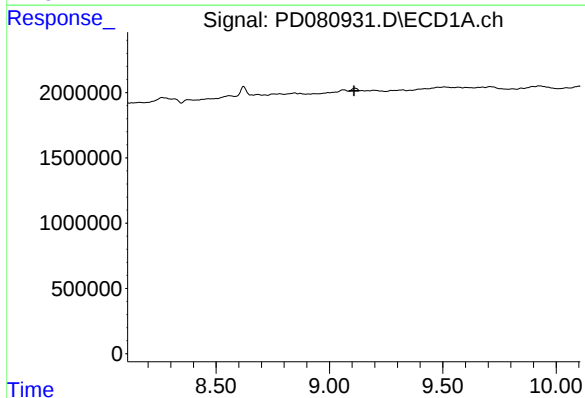

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.109 min
Response: 0
Conc: N.D.

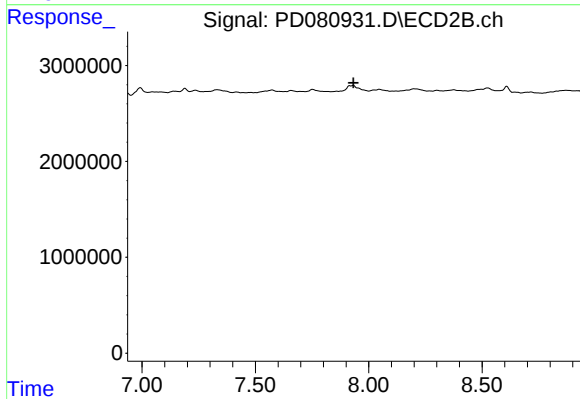

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.