

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
 Data File : PD080932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 16:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/29/2024
 Supervised By :Ankita Jodhani 01/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 19:56:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 11:14:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.572	2.793	29818466	53393136	21.005	22.320
2) SA Decachlor...	9.108	7.915f	134.7E6	193.5E6	66.951	72.634m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012624\
Data File : PD080932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 16:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/29/2024
Supervised By : Ankita Jodhani 01/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 19:56:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 11:14:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

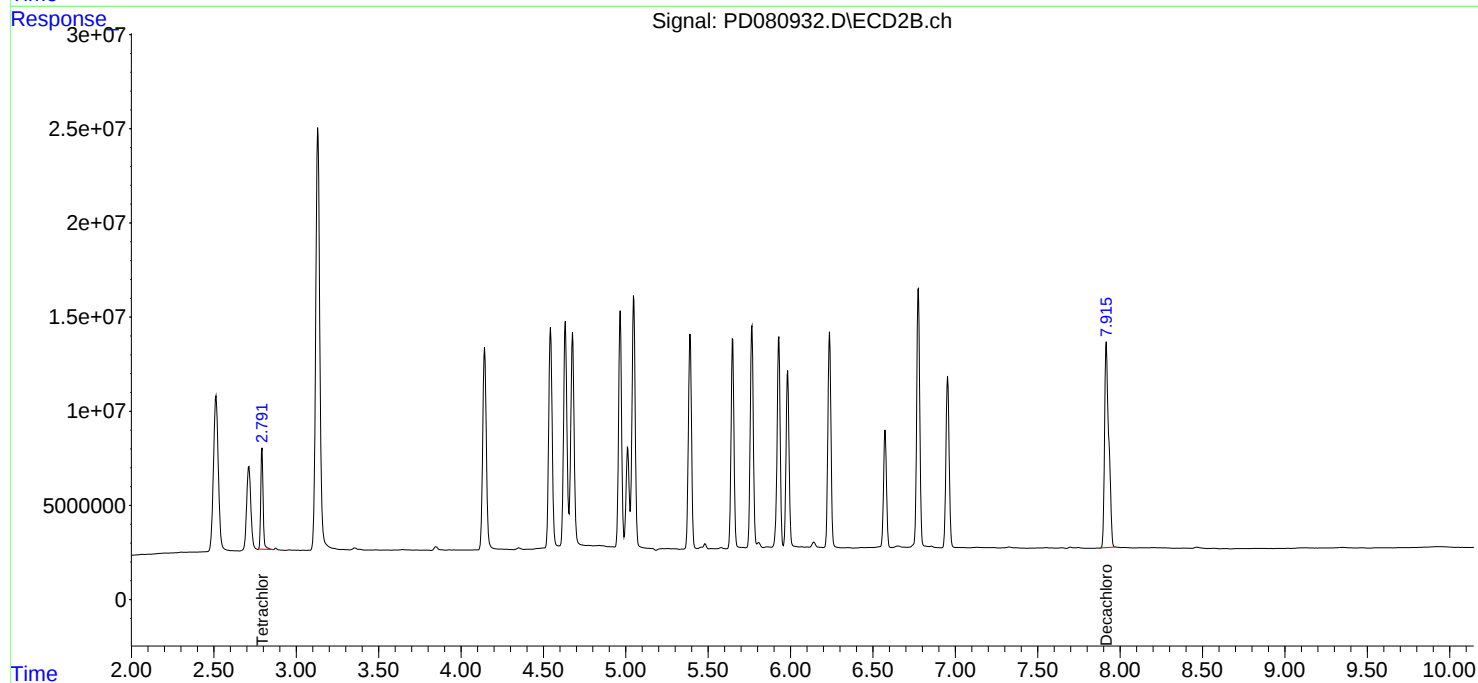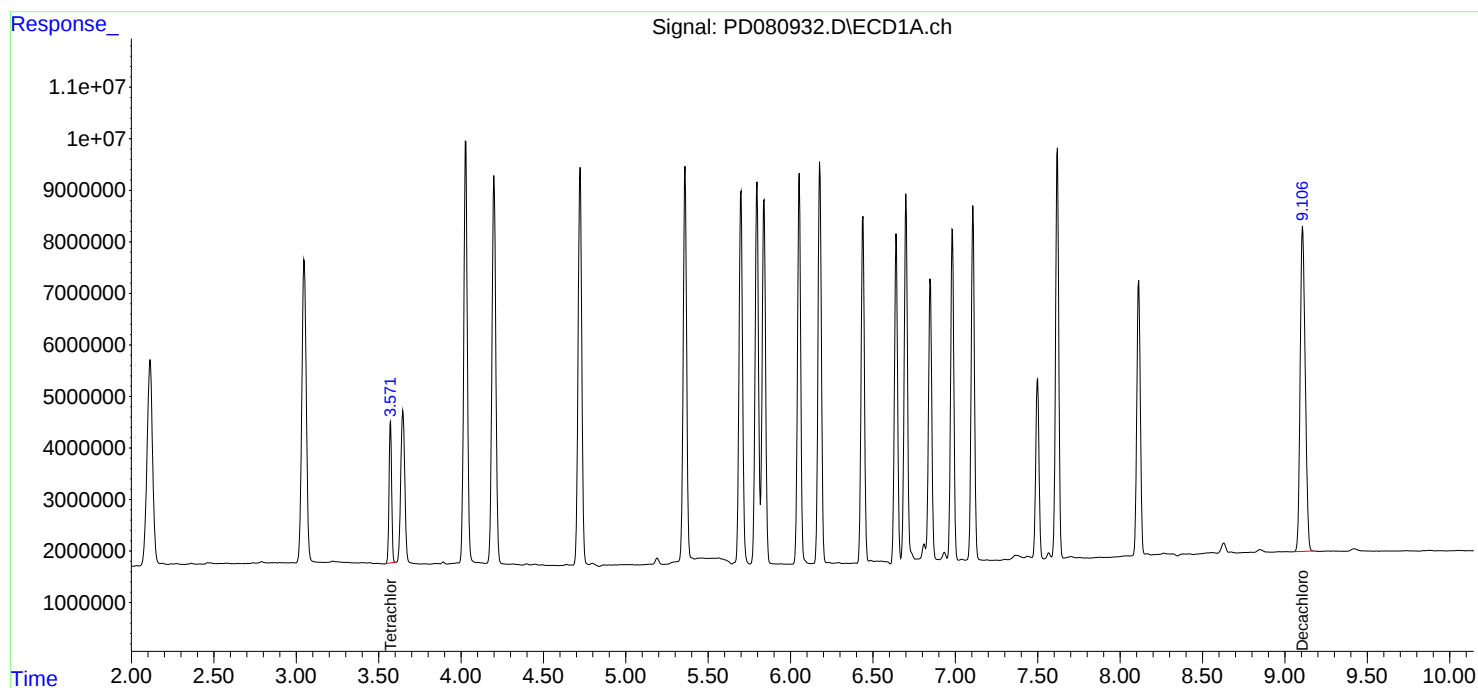

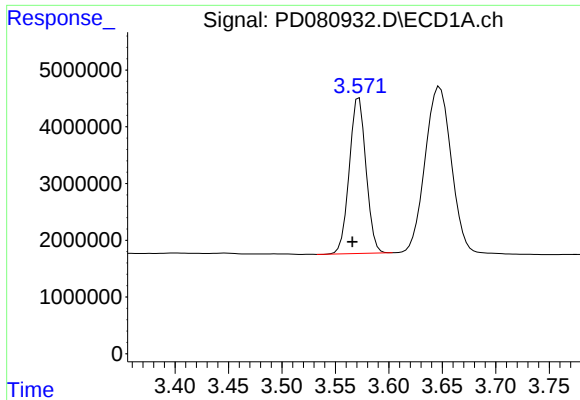


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: 0.006 min
Response: 29818466
Conc: 21.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/29/2024
Supervised By :Ankita Jodhani 01/29/2024

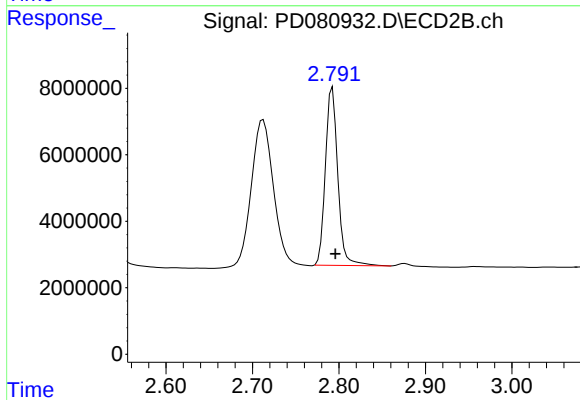


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.004 min
Response: 53393136
Conc: 22.32 ng/ml

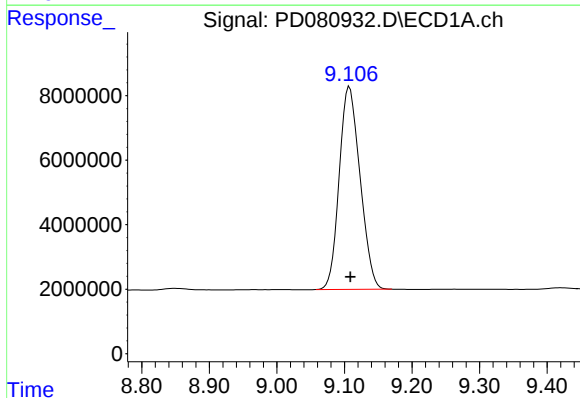

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.001 min
Response: 134735844
Conc: 66.95 ng/ml

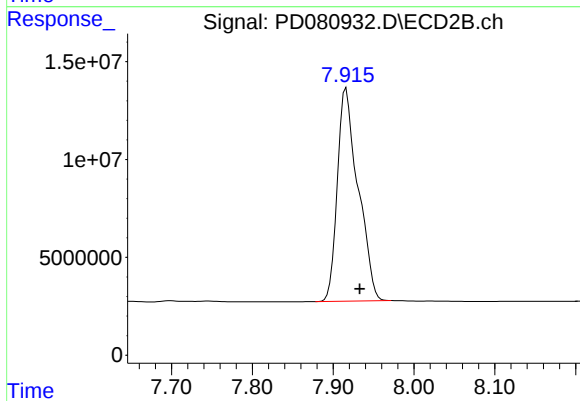

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.018 min
Response: 193468998
Conc: 72.63 ng/ml m