

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012725\
 Data File : PD087526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2025 13:31
 Operator : AR\AJ
 Sample : Q1148-02DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XA171DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/28/2025
 Supervised By : Ankita Jodhani 01/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:46:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.883	23126536	143.6E6	11.348	11.613
27)	SA Decachlor...	9.092	8.086	34458630	158.0E6	10.307	10.910
Target Compounds							
2)	A alpha-BHC	4.010	3.397	2878.6E6	8840.9E6	692.912	446.474 #
3)	MA gamma-BHC...	4.341	3.734	2219.8E6	7269.9E6	551.841	396.899 #
4)	MA Heptachlor	4.942	4.089	1486.5E6	4931.6E6	363.667	264.227 #
5)	MB Aldrin	5.284	4.375	1036.2E6	4033.1E6	258.731	223.141
6)	B beta-BHC	4.526	4.030	814.5E6	3220.1E6	453.513	377.479
7)	B delta-BHC	4.775	4.267	1273.6E6	4290.5E6	308.194	229.882 #
8)	B Heptachlo...	5.704	4.880	1275.2E6	4483.7E6	341.297	264.906
9)	A Endosulfan I	6.086	5.255	959.3E6	3422.0E6	275.336m	215.594
10)	B trans-Chl...	5.958	5.134	554.7E6	2336.7E6	150.561	129.979
11)	B cis-Chlor...	6.039	5.198	1298.5E6	4775.0E6	349.292m	275.888
12)	B 4,4'-DDE	6.208	5.384	2026.6E6	7344.7E6	575.393m	448.429
13)	MA Dieldrin	6.361	5.521	1977.4E6	6703.8E6	518.684	401.651
14)	MA Endrin	6.586	5.797	899.9E6	3387.2E6	277.259m	226.686
15)	B Endosulfa...	6.799	6.089	374.0E6	1712.6E6	116.171	115.602
16)	A 4,4'-DDD	6.718	5.939	1684.4E6	6127.8E6	612.632	458.332 #
17)	MA 4,4'-DDT	7.033	6.193	1475.0E6	5494.4E6	508.917m	398.697
18)	B Endrin al...	6.928	6.267	941.4E6	3565.0E6	373.603	309.219
19)	B Endosulfa...	7.162	6.491	1094.9E6	4281.2E6	354.642	294.505
20)	A Methoxychlor	7.506	6.764	482.2E6	1831.5E6	304.333	297.347
21)	B Endrin ke...	7.643	7.001	1558.3E6	5441.3E6	452.643	342.609

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012725\
Data File : PD087526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2025 13:31
Operator : AR\AJ
Sample : Q1148-02DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:46:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

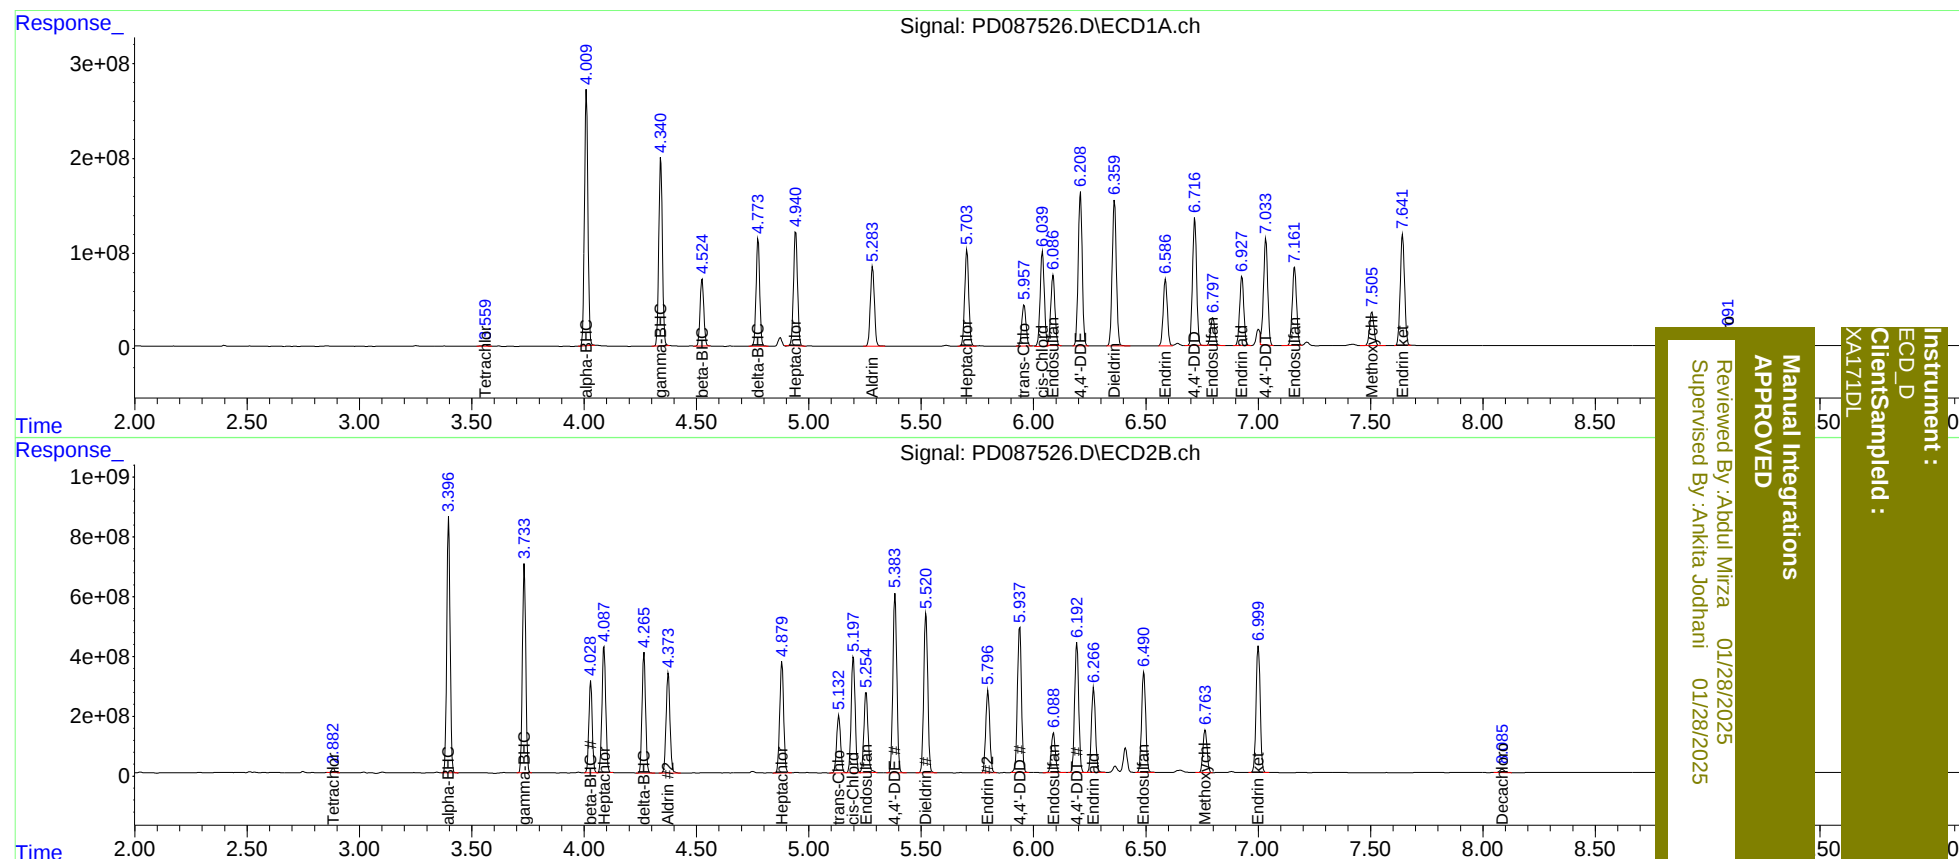

Instrument :
ECD_D
Client Sampled :
XA171DL

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 01/28/2025
Supervised By: Ankita Jodhani 01/28/2025