

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012725\
 Data File : PD087523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2025 11:32
 Operator : AR\AJ
 Sample : Q1161-03MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2947MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/28/2025
 Supervised By : Ankita Jodhani 01/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 00:44:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	28363126	196.6E6	13.917	15.896
2)	SA Decachlor...	9.086	8.084	41638968	168.4E6	12.454	11.624
Target Compounds							
2)	A alpha-BHC	4.004	3.396	199.5E6	901.6E6	48.029m	45.533
3)	MA gamma-BHC...	4.335	3.733	185.5E6	833.0E6	46.126m	45.477
4)	MA Heptachlor	4.935	4.088	182.3E6	811.9E6	44.610m	43.502
5)	MB Aldrin	5.279	4.374	173.9E6	777.2E6	43.417	43.002
6)	B beta-BHC	4.520	4.029	69513410	338.0E6	38.704	39.627
7)	B delta-BHC	4.769	4.266	190.0E6	810.6E6	45.975	43.430
8)	B Heptachlo...	5.698	4.879	151.8E6	682.3E6	40.640	40.310
9)	A Endosulfan I	6.081	5.254	139.1E6	609.2E6	39.916m	38.378
10)	B trans-Chl...	5.953	5.132	140.5E6	719.6E6	38.141	40.025
11)	B cis-Chlor...	6.033	5.197	145.7E6	695.4E6	39.201m	40.180
12)	B 4,4'-DDE	6.202	5.383	273.9E6	1291.6E6	77.768m	78.858
13)	MA Dieldrin	6.355	5.520	312.4E6	1320.3E6	81.937	79.102
14)	MA Endrin	6.582	5.796	259.3E6	1173.8E6	79.882	78.557
15)	B Endosulfa...	6.794	6.088	239.5E6	1129.6E6	74.409	76.246
16)	A 4,4'-DDD	6.713	5.938	215.1E6	1001.4E6	78.222	74.901
17)	MA 4,4'-DDT	7.029	6.192	238.6E6	1043.7E6	82.323	75.735
18)	B Endrin al...	6.922	6.266	169.3E6	766.3E6	67.208	66.467
19)	B Endosulfa...	7.156	6.490	236.9E6	1055.3E6	76.740	72.597
20)	A Methoxychlor	7.501	6.764	601.9E6	2150.7E6	379.884	349.179
21)	B Endrin ke...	7.638	6.999	261.2E6	1049.7E6	75.879	66.093

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012725\
Data File : PD087523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2025 11:32
Operator : AR\AJ
Sample : Q1161-03MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 00:44:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

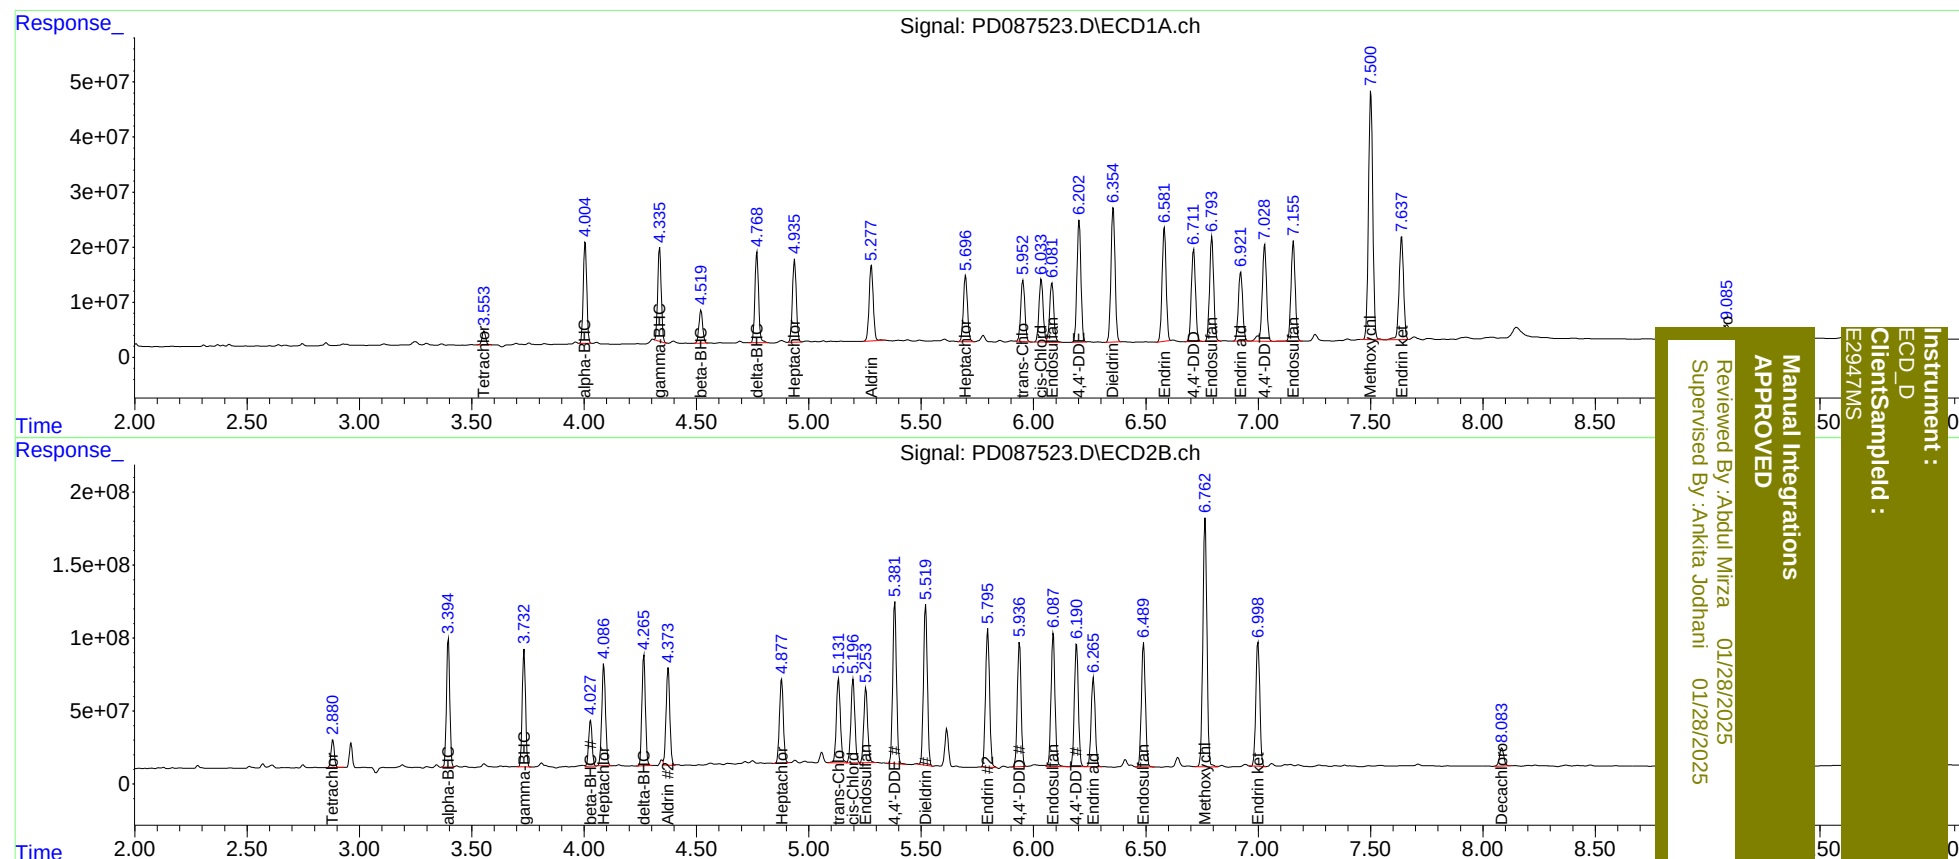

Instrument :
ECD_D
ClientSampled :
E2947MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/28/2025
Supervised By :Ankita Jodhani 01/28/2025