

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012820\
 Data File : PD057076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2020 14:10
 Operator : AJ\MA
 Sample : L1008-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CL-02-012420

Manual Integrations
 APPROVED

mohammad
 1/29/2020 3:05:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 00:25:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.958	361429	708072	0.438m	0.433m
28)	SA Decachlor...	7.968	8.998	294799	702038	0.304m	0.421m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012820\
Data File : PD057076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2020 14:10
Operator : AJ\MA
Sample : L1008-21
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CL-02-012420


Manual Integrations
APPROVED

mohammad
1/29/2020 3:05:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 00:25:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

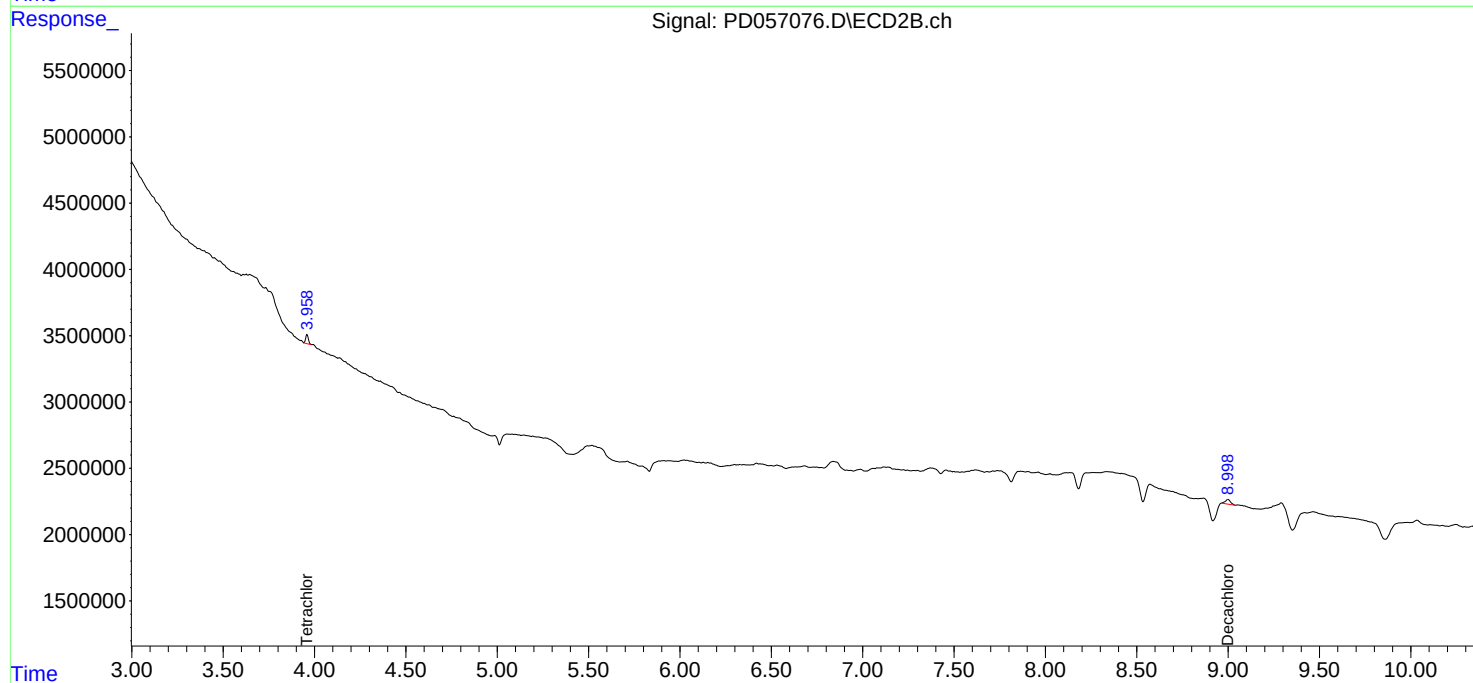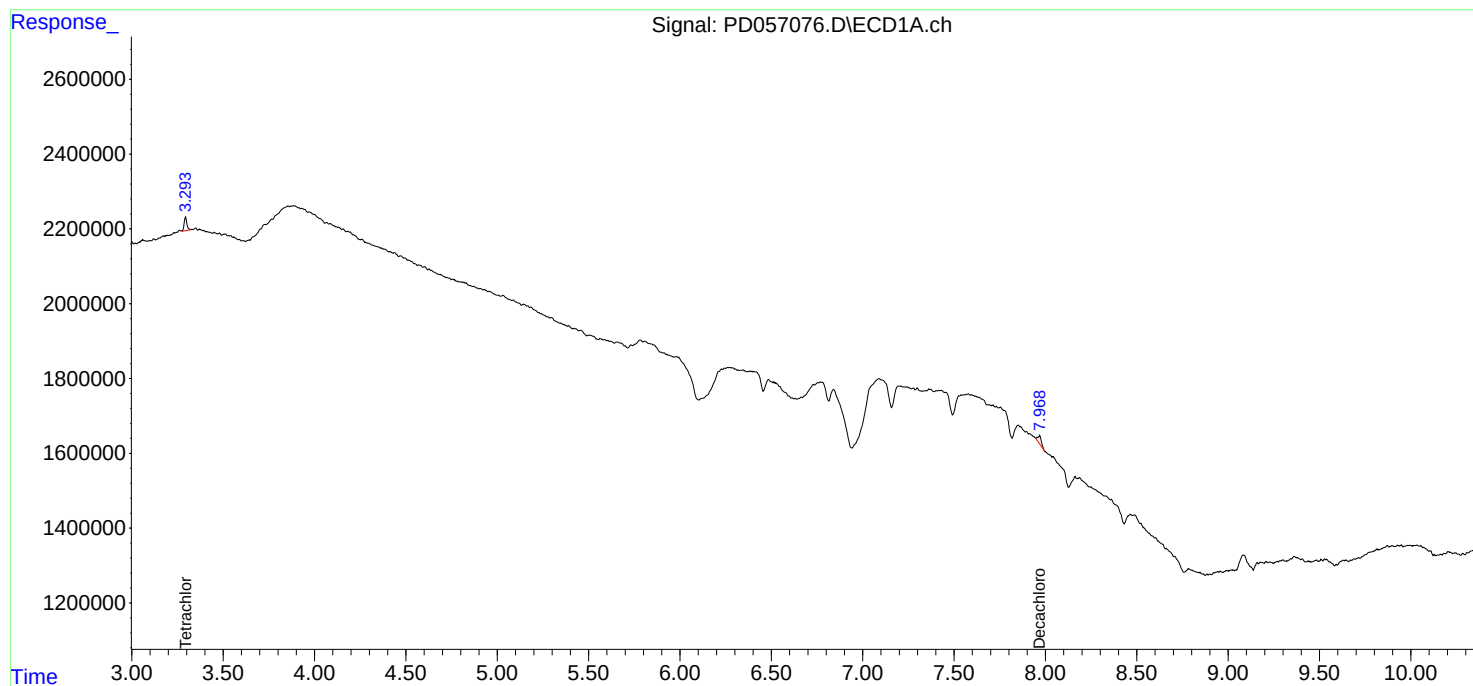

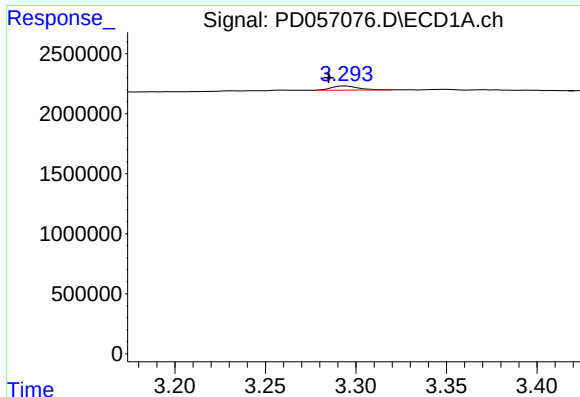


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: 0.008 min
Response: 361429
Conc: 0.44 ng/ml m

Instrument :
ECD_D
ClientSampleId :
CL-02-012420


Manual Integrations
APPROVED

mohammad
1/29/2020 3:05:43 PM

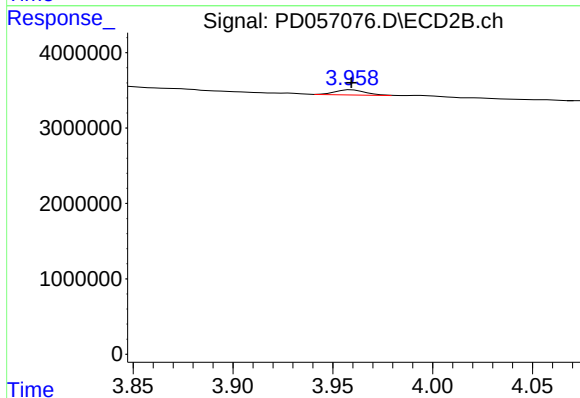


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 708072
Conc: 0.43 ng/ml m

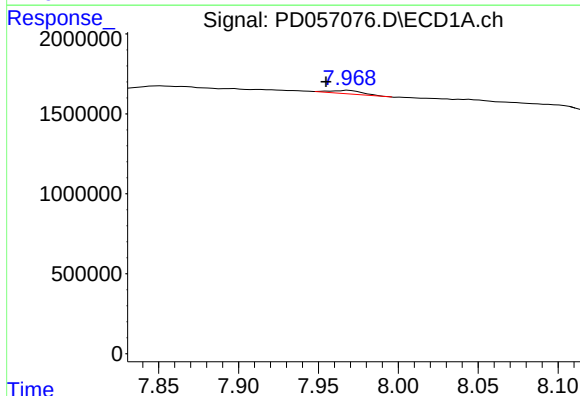

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.013 min
Response: 294799
Conc: 0.30 ng/ml m

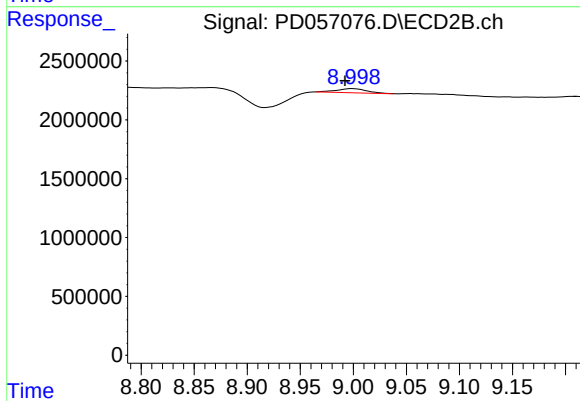

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.006 min
Response: 702038
Conc: 0.42 ng/ml m