

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
 Data File : PD061057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 19:11
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:51:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:48:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.108	0	2123673	N.D.	0.348 #
Target Compounds							
7)	B delta-BHC	0.000	5.059f	0	7943989	N.D.	0.797 #
8)	B Heptachlo...	0.000	5.895	0	6765991	N.D.	0.837 #
9)	A Endosulfan I	0.000	6.248	0	6384344	N.D.	0.797 #
12)	B 4,4'-DDE	0.000	6.334f	0	2627280	N.D.	0.317 #
19)	B Endosulfa...	6.714	0.000	1216947	0	1.372	N.D. #
22)	Mirex	7.410	0.000	2053477	0	2.849	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
Data File : PD061057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 19:11
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:51:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:48:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

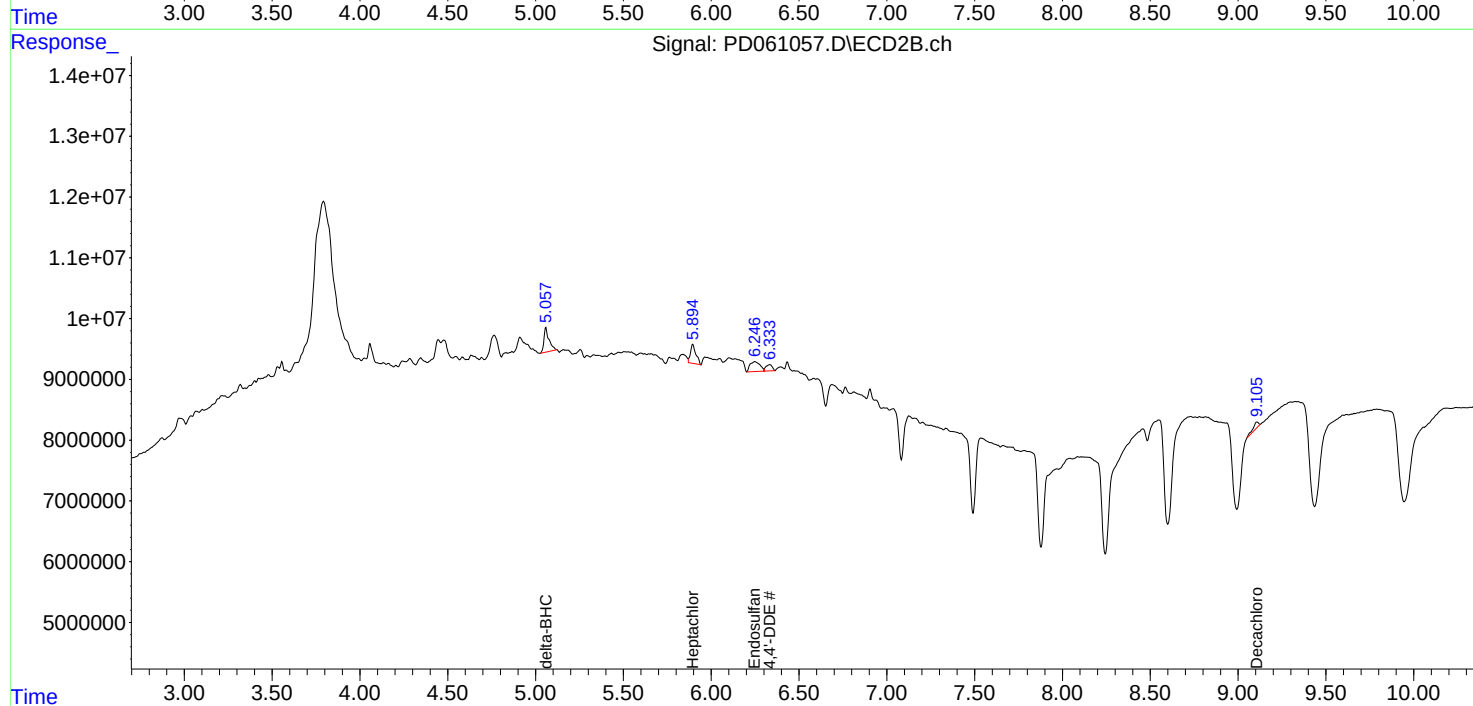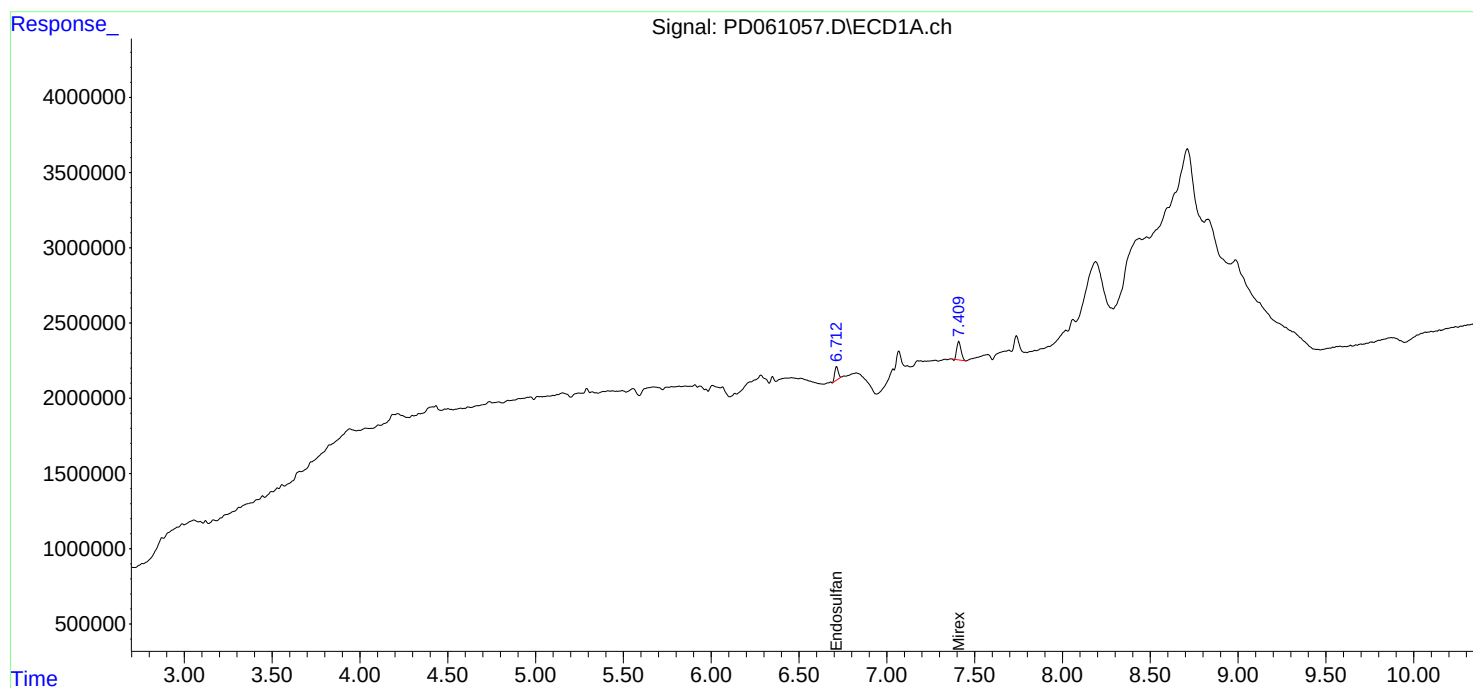


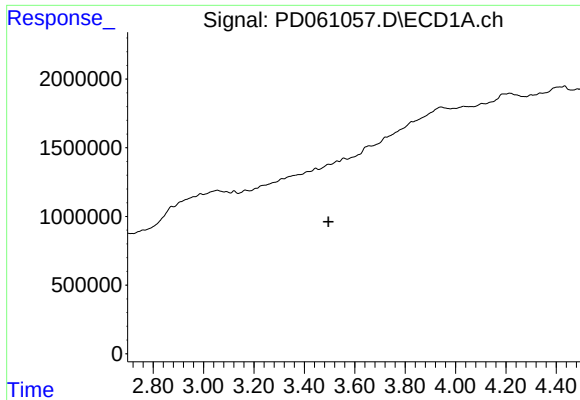

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

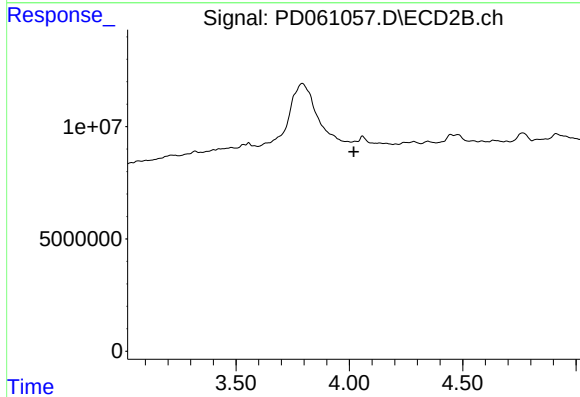


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.020 min
Response: 0
Conc: N.D.

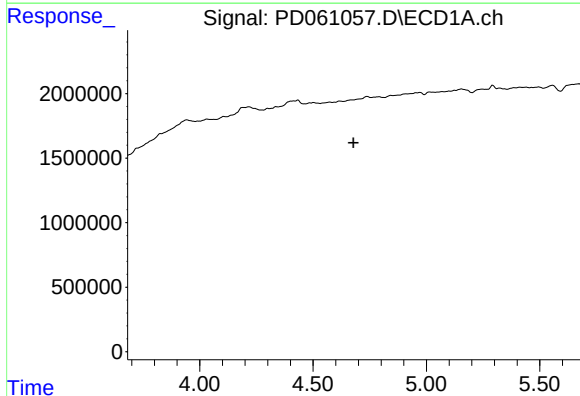


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

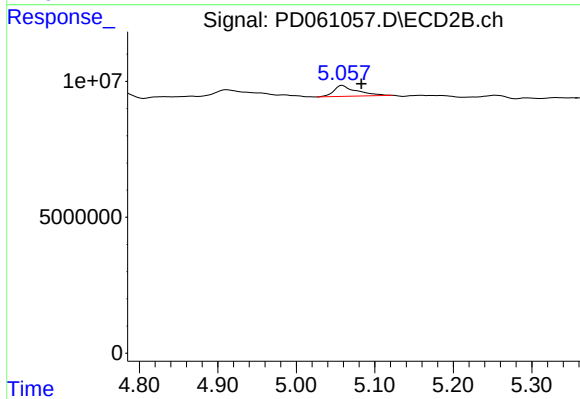

#7 delta-BHC


R.T.: 5.059 min
Delta R.T.: -0.024 min
Response: 7943989
Conc: 0.80 ng/ml

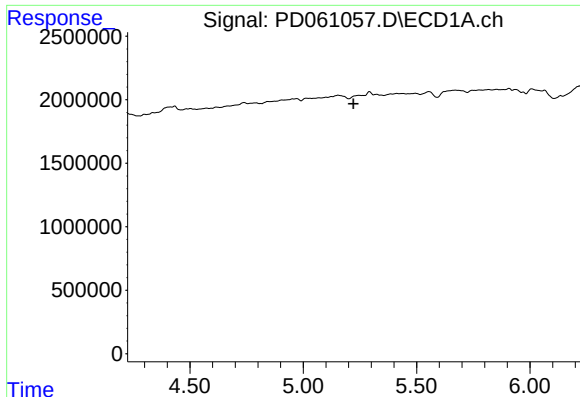

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

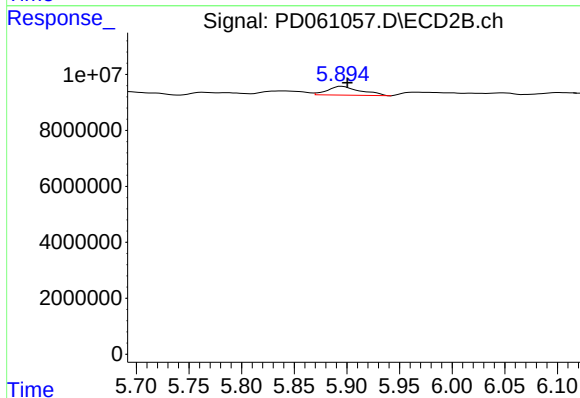


#8 Heptachlor epoxide

R.T.: 5.895 min
Delta R.T.: -0.006 min
Response: 6765991
Conc: 0.84 ng/ml

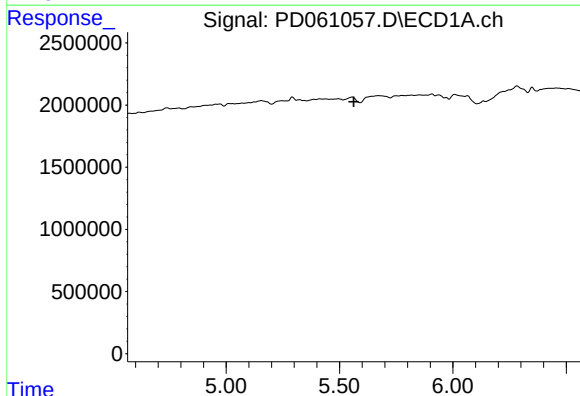


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.563 min
Response: 0
Conc: N.D.

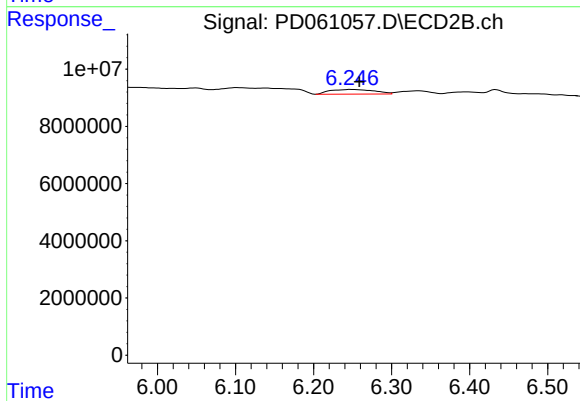

#9 Endosulfan I


R.T.: 6.248 min
Delta R.T.: -0.010 min
Response: 6384344
Conc: 0.80 ng/ml

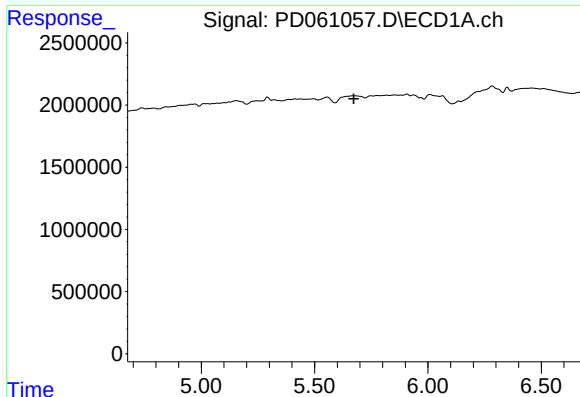

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

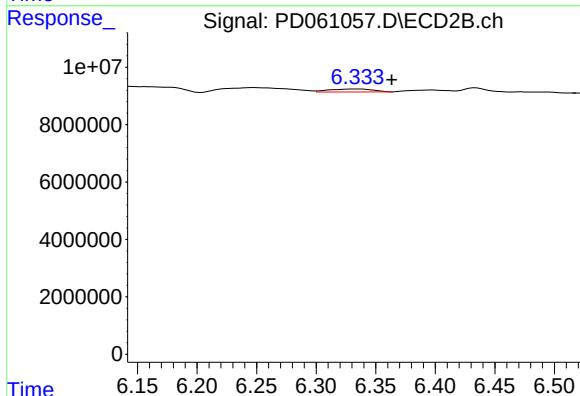


#12 4,4'-DDE

R.T.: 6.334 min
Delta R.T.: -0.029 min
Response: 2627280
Conc: 0.32 ng/ml

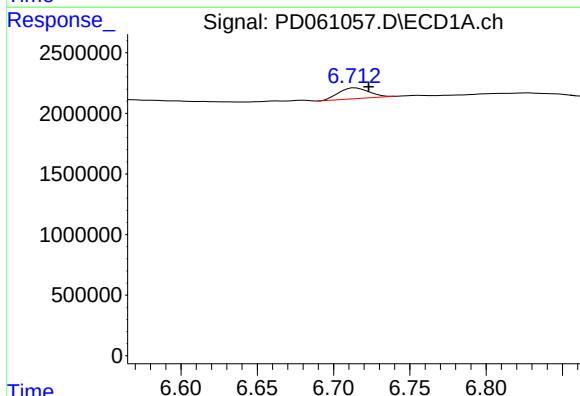


#19 Endosulfan Sulfate

R.T.: 6.714 min
Delta R.T.: -0.009 min
Response: 1216947
Conc: 1.37 ng/ml

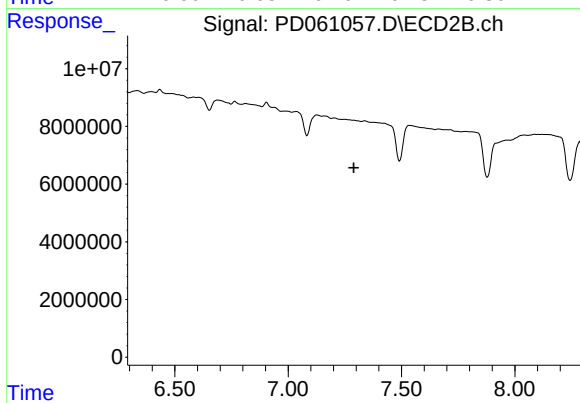

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.290 min
Response: 0
Conc: N.D.

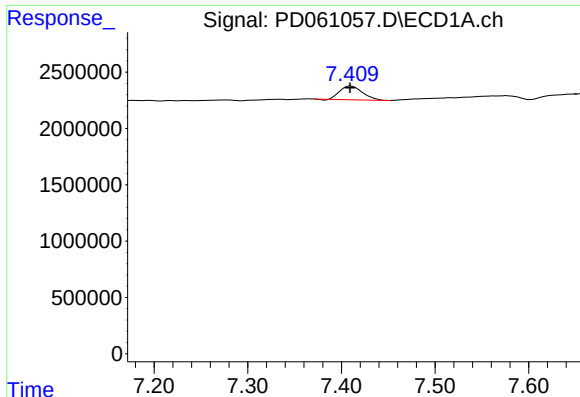

#22 Mirex


R.T.: 7.410 min
Delta R.T.: 0.001 min
Response: 2053477
Conc: 2.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

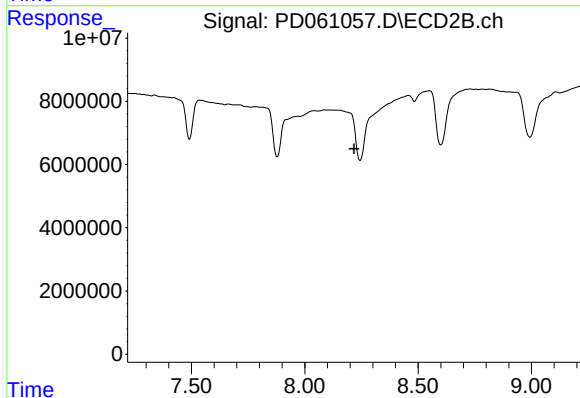


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.218 min
Response: 0
Conc: N.D.

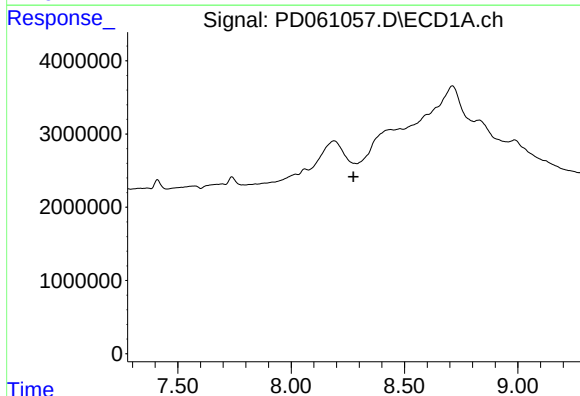

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.276 min
Response: 0
Conc: N.D.

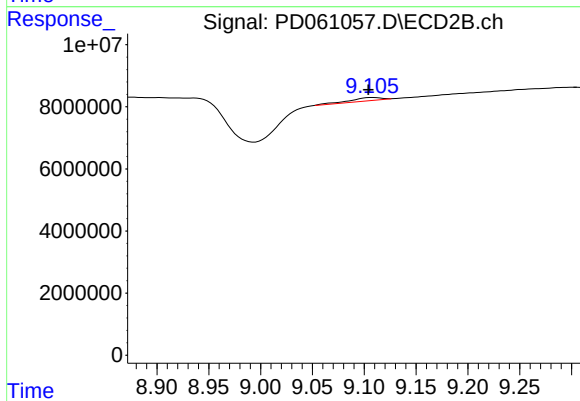

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.004 min
Response: 2123673
Conc: 0.35 ng/ml