

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
 Data File : PD061058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 19:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:52:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:48:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	18070780	139.1E6	20.464	20.578
28)	SA Decachlor...	8.277	9.105	17087776	124.6E6	19.842	20.425
Target Compounds							
7)	B delta-BHC	0.000	5.059f	0	6879513	N.D.	0.690 #
9)	A Endosulfan I	0.000	6.230f	0	1719558	N.D.	0.215 #
11)	B alpha-Chl...	0.000	6.230f	0	1719558	N.D.	0.203 #
12)	B 4,4'-DDE	0.000	6.375	0	1469617	N.D.	0.177 #
26)	Chlordane-4	0.000	6.230f	0	1719558	N.D.	1.396 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
Data File : PD061058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 19:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:52:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:48:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

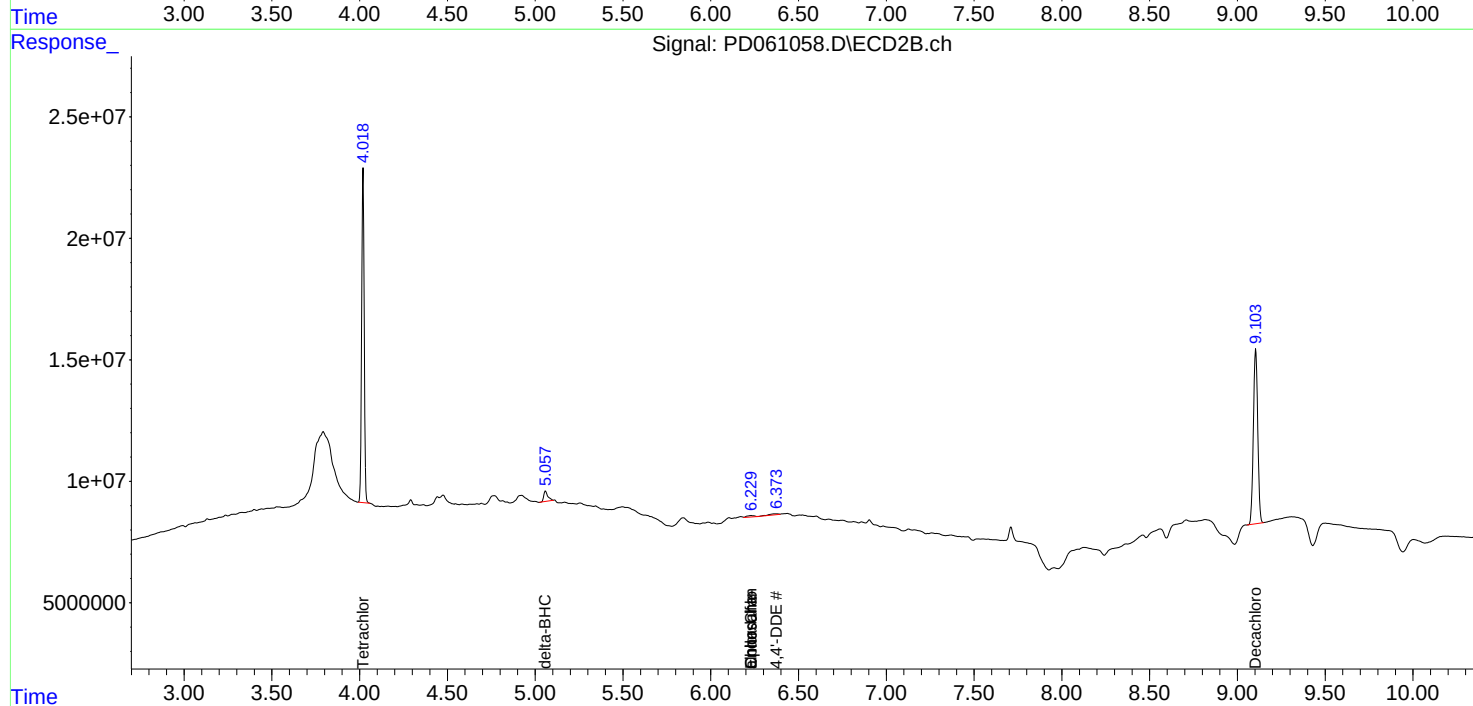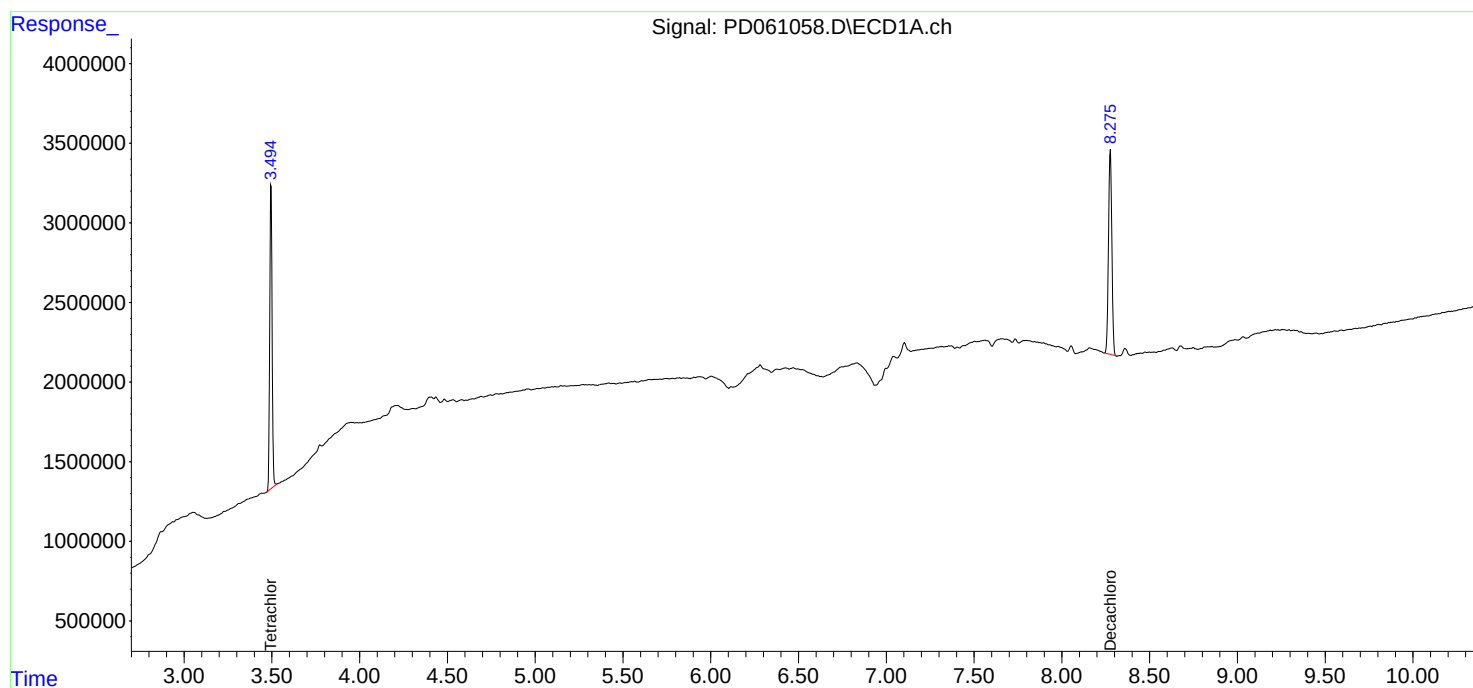


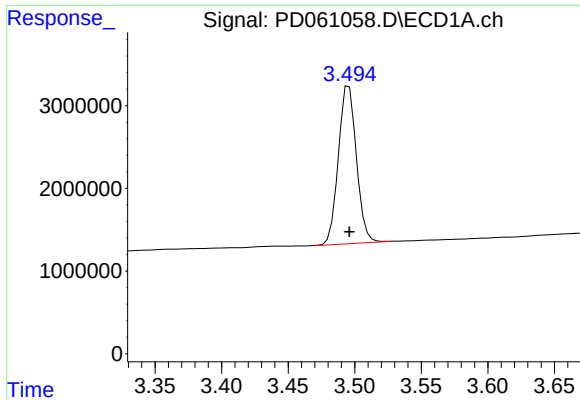

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 18070780
Conc: 20.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

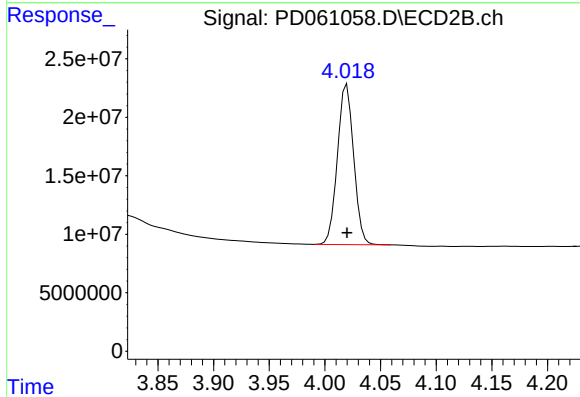


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 139080108
Conc: 20.58 ng/ml

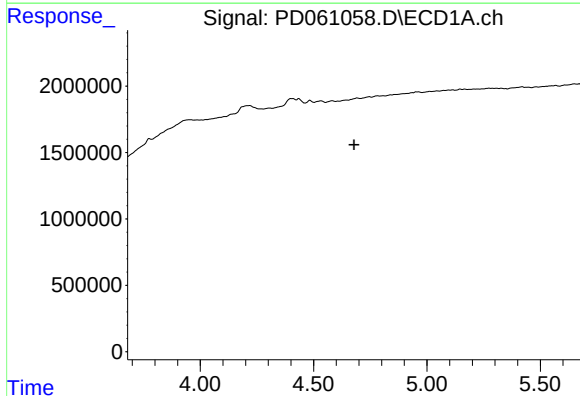


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

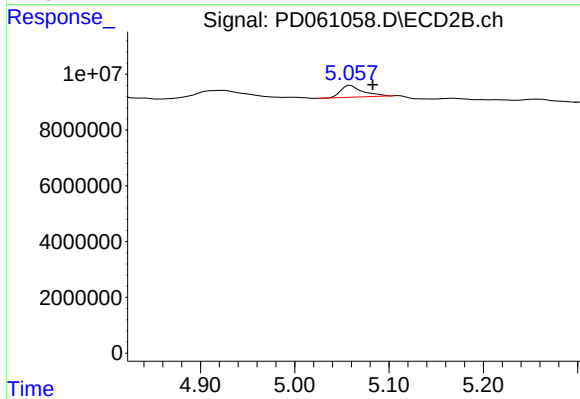

#7 delta-BHC


R.T.: 5.059 min
Delta R.T.: -0.024 min
Response: 6879513
Conc: 0.69 ng/ml

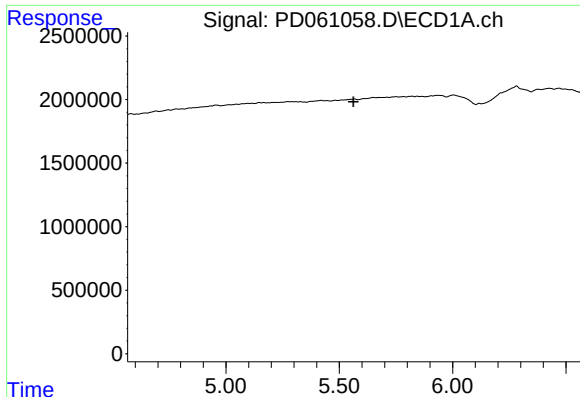

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.563 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

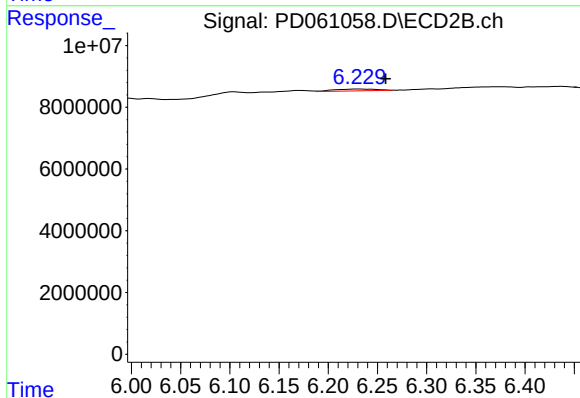


#9 Endosulfan I

R.T.: 6.230 min
Delta R.T.: -0.028 min
Response: 1719558
Conc: 0.21 ng/ml

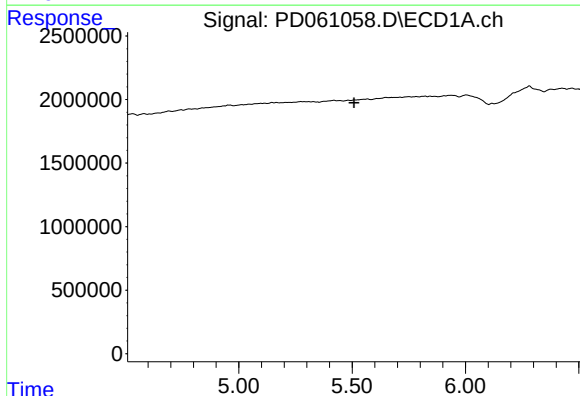


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

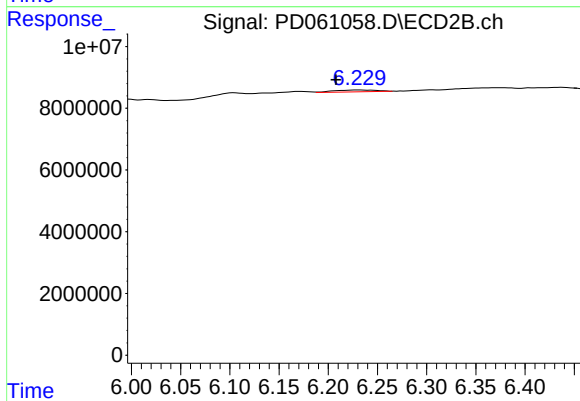

#11 alpha-Chlordane


R.T.: 6.230 min
Delta R.T.: 0.023 min
Response: 1719558
Conc: 0.20 ng/ml

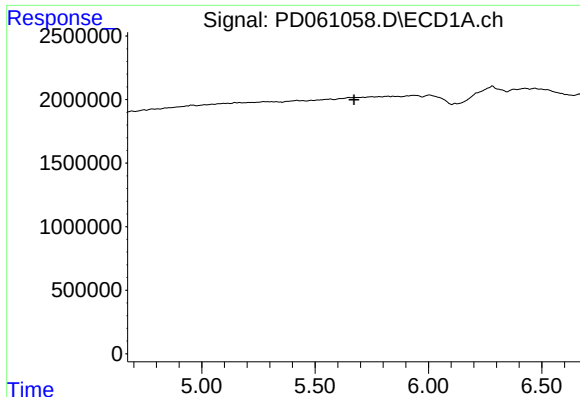

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

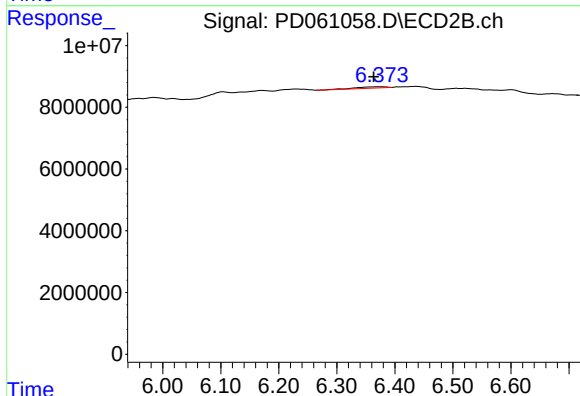


#12 4,4'-DDE

R.T.: 6.375 min
Delta R.T.: 0.011 min
Response: 1469617
Conc: 0.18 ng/ml

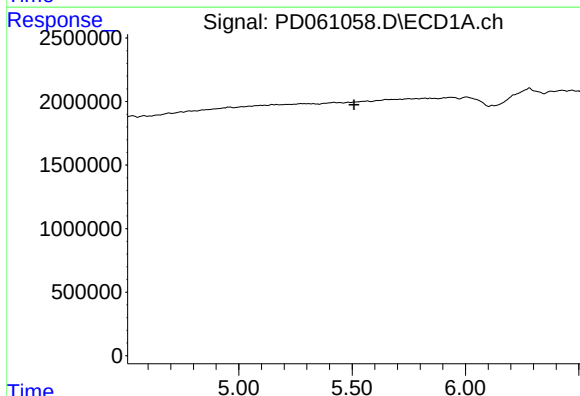


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

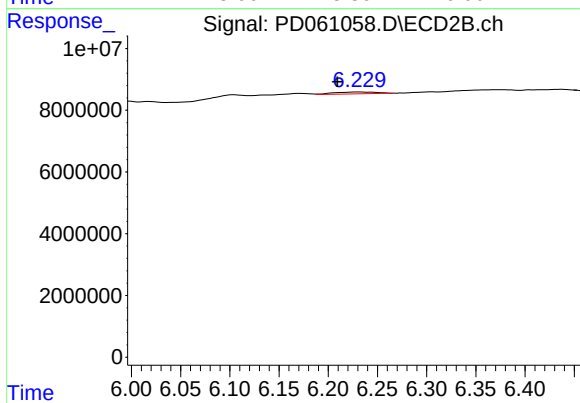

#26 Chlordane-4


R.T.: 6.230 min
Delta R.T.: 0.021 min
Response: 1719558
Conc: 1.40 ng/ml

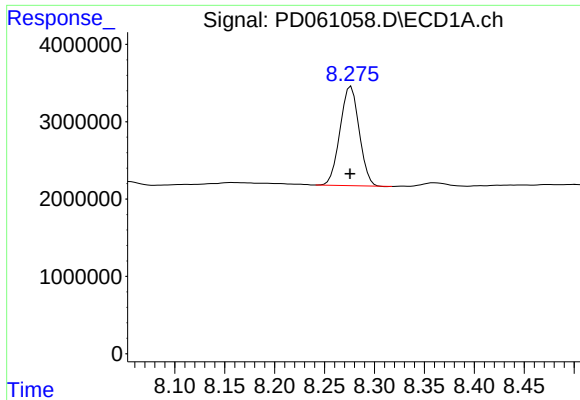

#28 Decachlorobiphenyl

R.T.: 8.277 min
Delta R.T.: 0.000 min
Response: 17087776
Conc: 19.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

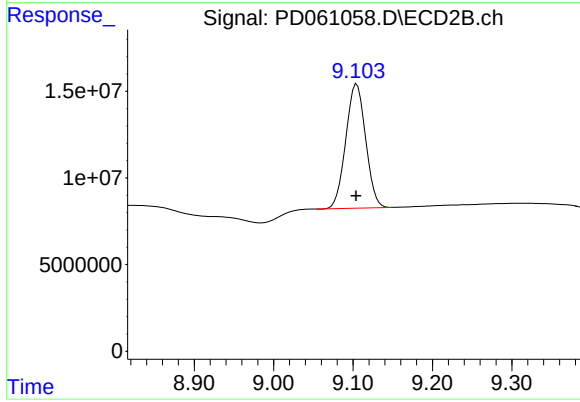

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 124556680
Conc: 20.42 ng/ml