

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
 Data File : PD061066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 21:18
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 01:22:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:21:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.020	48311650	326.8E6	50.000	50.000
28)	SA Decachlor...	8.276	9.104	40796422	291.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.373	5.019	16071739	135.1E6	500.000	500.000
24)	Chlordane-2	4.877	5.487	17353797	128.6E6	500.000	500.000
25)	Chlordane-3	5.450	6.134	47538406	529.0E6	500.000	500.000
26)	Chlordane-4	5.508	6.209	40289306	616.0E6	500.000	500.000
27)	Chlordane-5	6.349	7.015	18360981	109.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012821\
Data File : PD061066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 21:18
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 01:22:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:21:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

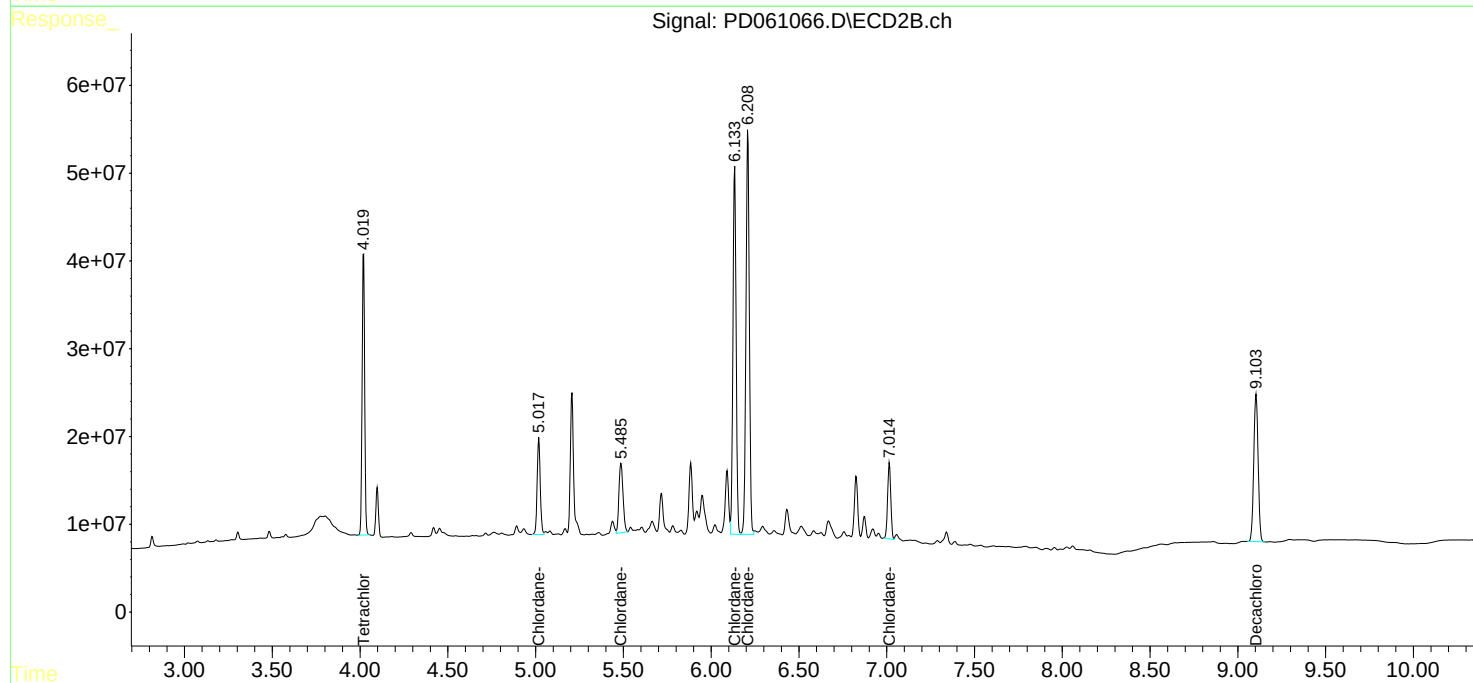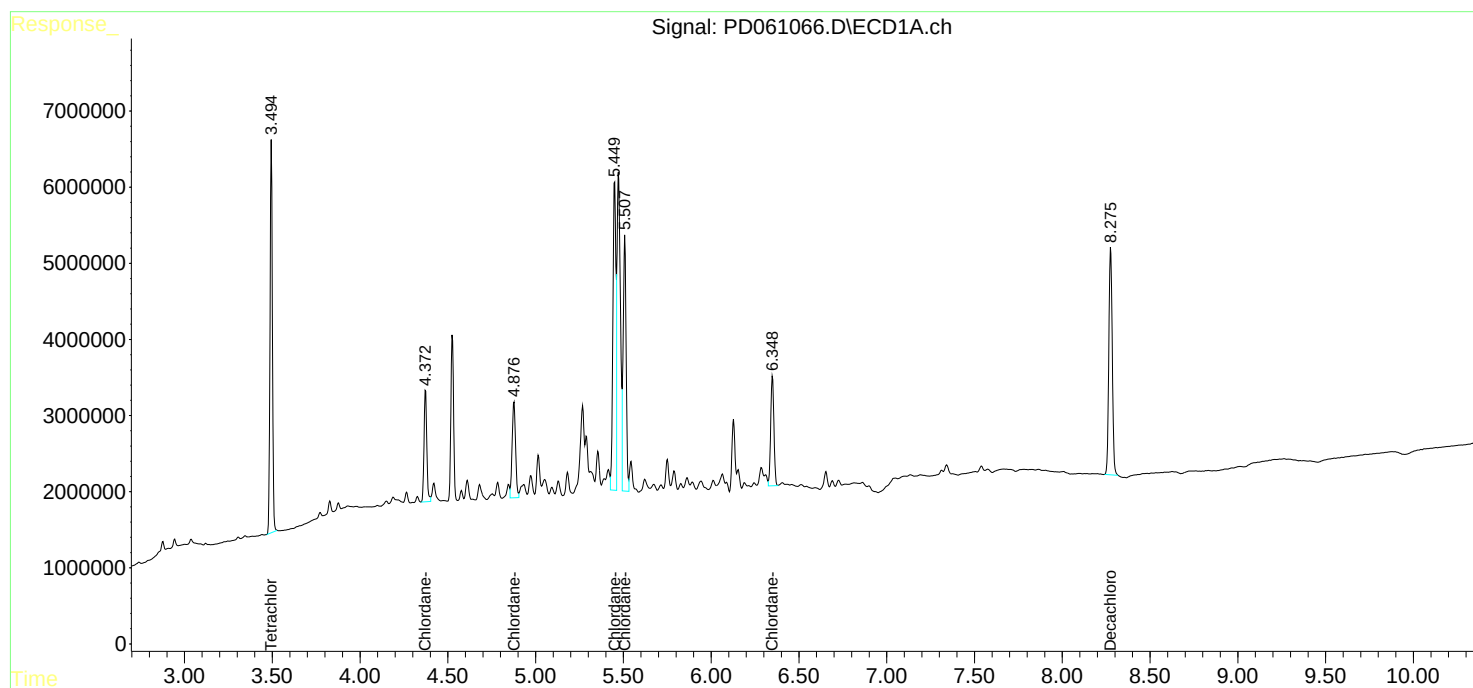


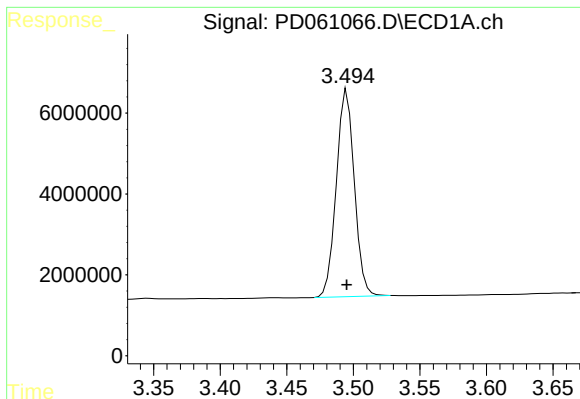

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 48311650
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

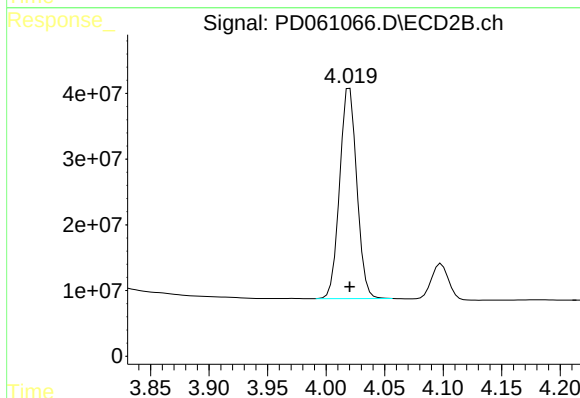


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 326782982
Conc: 50.00 ng/ml

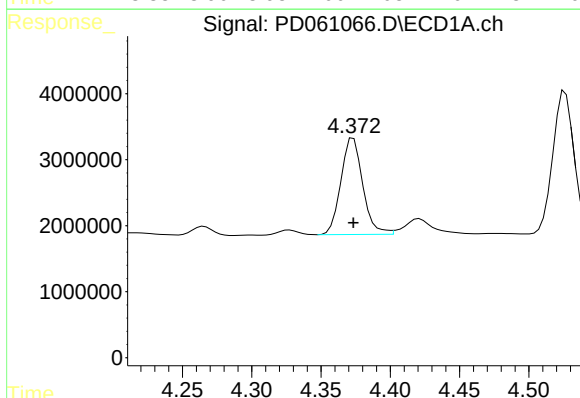


#23 Chlordane-1

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 16071739
Conc: 500.00 ng/ml

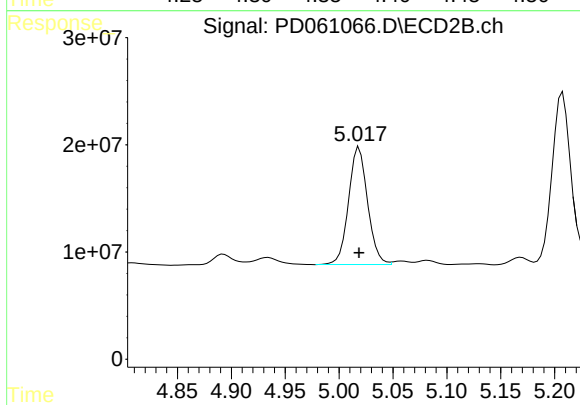

#23 Chlordane-1


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 135084938
Conc: 500.00 ng/ml

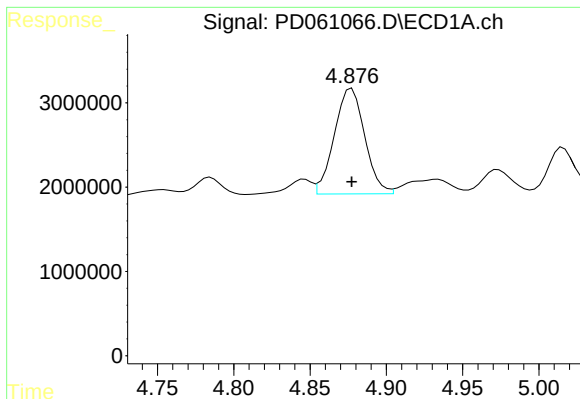

#24 Chlordane-2


R.T.: 4.877 min
Delta R.T.: 0.000 min
Response: 17353797
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

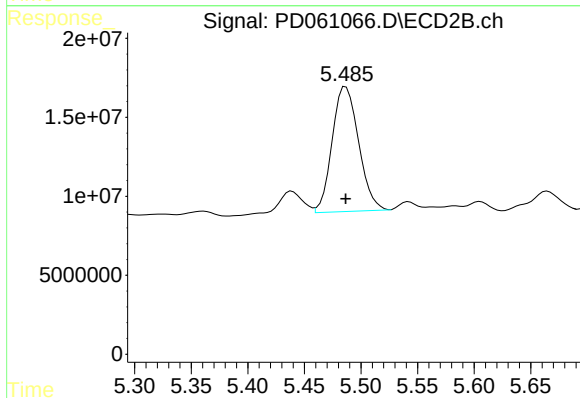


#24 Chlordane-2

R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 128569716
Conc: 500.00 ng/ml

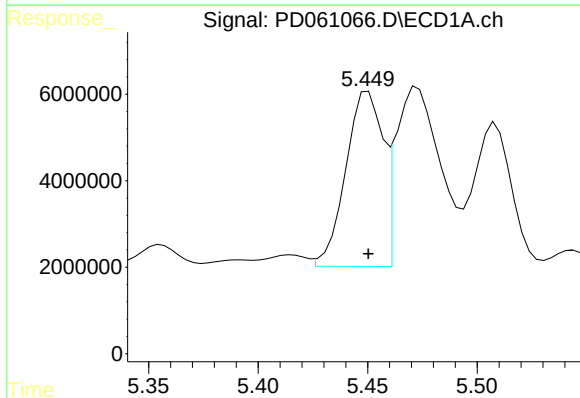


#25 Chlordane-3

R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 47538406
Conc: 500.00 ng/ml

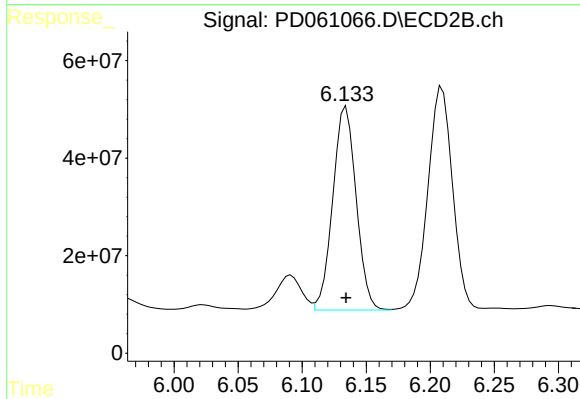

#25 Chlordane-3


R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 528999042
Conc: 500.00 ng/ml

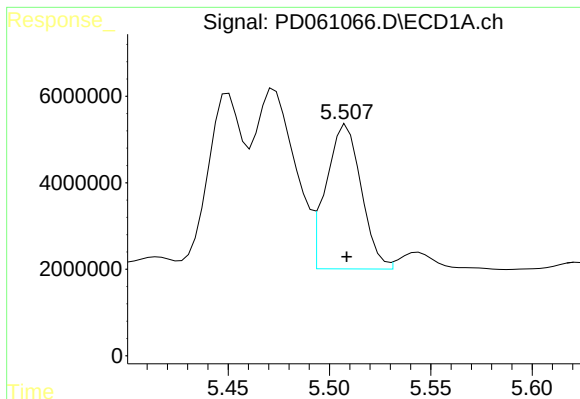

#26 Chlordane-4


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 40289306
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

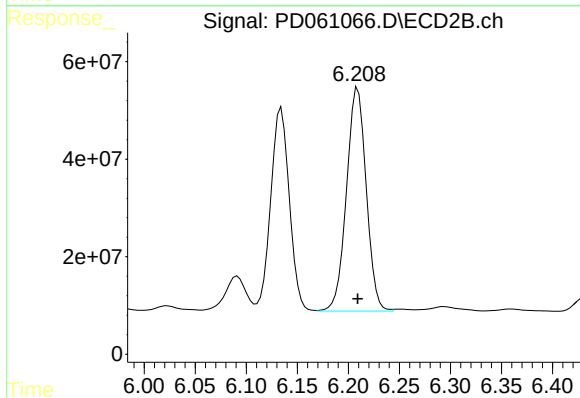


#26 Chlordane-4

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 615974621
Conc: 500.00 ng/ml

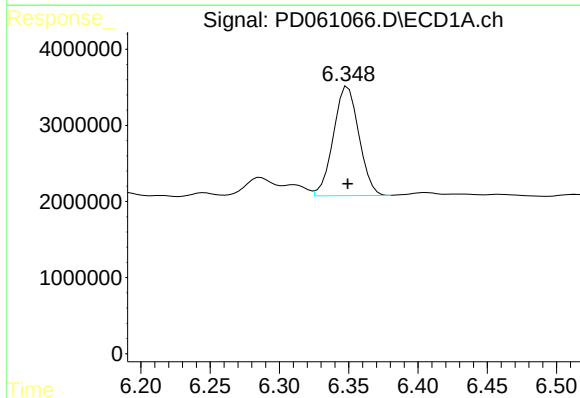


#27 Chlordane-5

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 18360981
Conc: 500.00 ng/ml

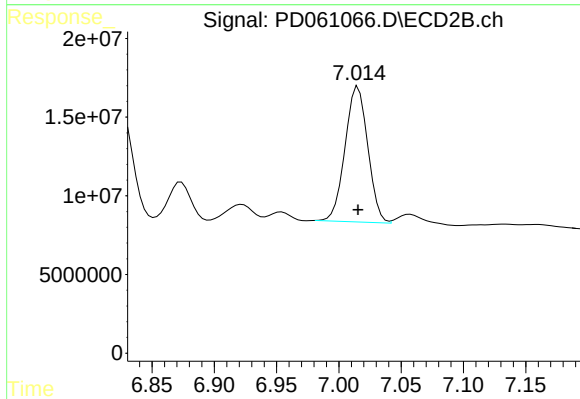

#27 Chlordane-5


R.T.: 7.015 min
Delta R.T.: 0.000 min
Response: 109945290
Conc: 500.00 ng/ml

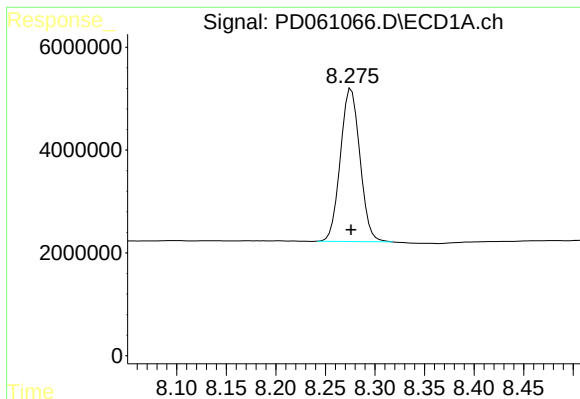

#28 Decachlorobiphenyl

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 40796422
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

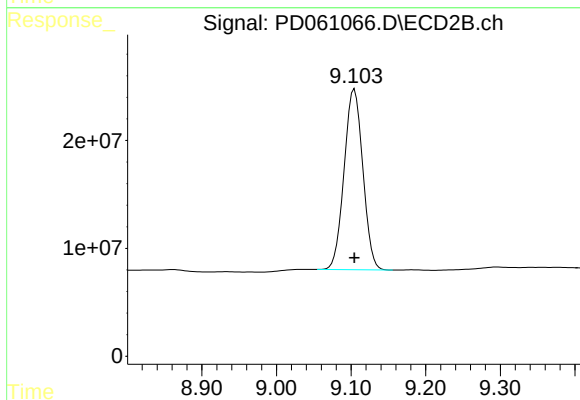

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 291795145
Conc: 50.00 ng/ml