

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
 Data File : PD087550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2025 11:27
 Operator : AR\AJ
 Sample : Q1148-07DL2 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XA176DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 07:49:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.882	2716437	20486715	1.333m	1.656
2) SA Decachlor...	9.091	8.087	4124698	18433311	1.234	1.273
Target Compounds						
2) A alpha-BHC	4.006	3.396	249.4E6	1095.5E6	60.043	55.323
3) MA gamma-BHC...	4.338	3.733	194.9E6	848.9E6	48.454	46.348
4) MA Heptachlor	4.938	4.088	25633739	133.5E6	6.271	7.154
5) MB Aldrin	5.281	4.375	240.7E6	1039.4E6	60.106	57.506
6) B beta-BHC	4.522	4.030	127.5E6	594.5E6	70.998	69.687
7) B delta-BHC	4.771	4.267	102.3E6	481.7E6	24.763	25.807
8) B Heptachlo...	5.700	4.879	56955135	286.0E6	15.244	16.898
9) A Endosulfan I	6.083	5.254	139.7E6	650.3E6	40.095m	40.969
10) B trans-Chl...	5.956	5.133	149.9E6	727.2E6	40.700	40.451
11) B cis-Chlor...	6.035	5.198	142.5E6	675.2E6	38.319m	39.013
12) B 4,4'-DDE	6.205	5.383	165.6E6	832.4E6	47.014m	50.825
13) MA Dieldrin	6.358	5.521	139.5E6	668.3E6	36.598	40.040
14) MA Endrin	6.584	5.797	326.4E6	1452.4E6	100.556m	97.203
15) B Endosulfa...	6.796	6.089	147.1E6	723.7E6	45.695	48.851
16) A 4,4'-DDD	6.715	5.938	64753971	375.4E6	23.551	28.078
17) MA 4,4'-DDT	7.032	6.193	44936536	250.1E6	15.505	18.151
18) B Endrin al...	6.925	6.267	185.9E6	873.1E6	73.782	75.727
19) B Endosulfa...	7.159	6.492	111.0E6	572.8E6	35.940	39.400
20) A Methoxychlor	7.505	6.765	27727601	145.8E6	17.501	23.676 #
21) B Endrin ke...	7.641	7.002	295.0E6	1373.0E6	85.696	86.449

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
Data File : PD087550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2025 11:27
Operator : AR\AJ
Sample : Q1148-07DL2 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 07:49:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

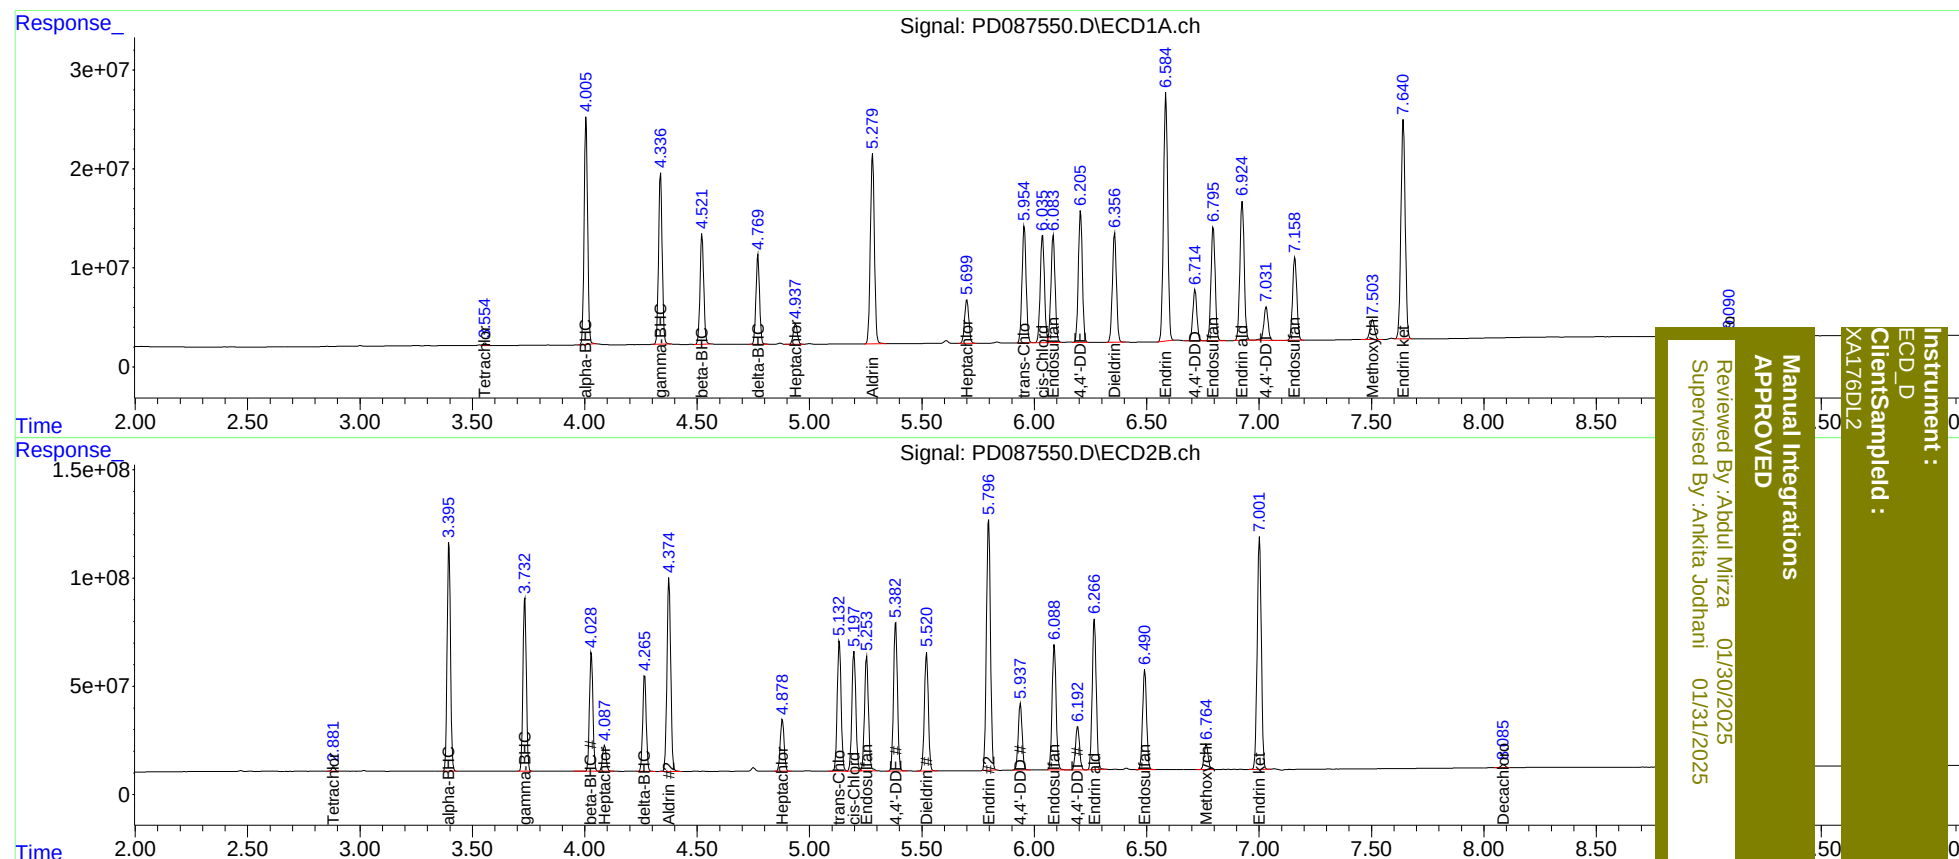

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/30/2025
Supervised By: Ankita Jodhani 01/31/2025

Instrument :
ECD_D
Client Sampled :
XA176DL2