

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
 Data File : PD087549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2025 11:12
 Operator : AR\AJ
 Sample : Q1148-07DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XA176DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 07:48:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.559	2.881	24398699	166.3E6	11.972m	13.449m
2) SA Decachlor...	9.096	8.088	32909340	154.7E6	9.843	10.683
Target Compounds						
2) A alpha-BHC	4.011	3.396	2811.4E6	9170.5E6	676.750	463.118 #
3) MA gamma-BHC...	4.343	3.733	2129.5E6	7068.0E6	529.386	385.872 #
4) MA Heptachlor	4.943	4.088	243.0E6	1007.7E6	59.453	53.993
5) MB Aldrin	5.286	4.375	2441.5E6	7782.1E6	609.607	430.565 #
6) B beta-BHC	4.527	4.029	1211.3E6	4719.3E6	674.450	553.231
7) B delta-BHC	4.776	4.267	1117.9E6	3958.6E6	270.532	212.099
8) B Heptachlo...	5.705	4.880	552.7E6	2189.2E6	147.937	129.342
9) A Endosulfan I	6.088	5.255	1346.4E6	4806.7E6	386.459m	302.835
10) B trans-Chl...	5.961	5.133	1553.9E6	5849.6E6	421.798	325.382
11) B cis-Chlor...	6.041	5.199	1457.9E6	5356.0E6	392.159m	309.458
12) B 4,4'-DDE	6.210	5.384	1737.1E6	6471.0E6	493.196m	395.086
13) MA Dieldrin	6.363	5.522	1420.1E6	5074.1E6	372.486	304.005
14) MA Endrin	6.589	5.798	3272.9E6	9877.5E6	1008.393m	661.044 #
15) B Endosulfa...	6.800	6.090	1423.5E6	5336.9E6	442.183m	360.243
16) A 4,4'-DDD	6.721	5.940	657.2E6	2829.8E6	239.020	211.657
17) MA 4,4'-DDT	7.036	6.194	463.5E6	2081.5E6	159.919m	151.041
18) B Endrin al...	6.931	6.269	1719.7E6	6026.2E6	682.498	522.704
19) B Endosulfa...	7.165	6.493	1067.3E6	4273.3E6	345.691	293.957
20) A Methoxychlor	7.510	6.766	246.5E6	1044.0E6	155.566	169.500
21) B Endrin ke...	7.646	7.003	2841.6E6	9249.0E6	825.401	582.357 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
Data File : PD087549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2025 11:12
Operator : AR\AJ
Sample : Q1148-07DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 07:48:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

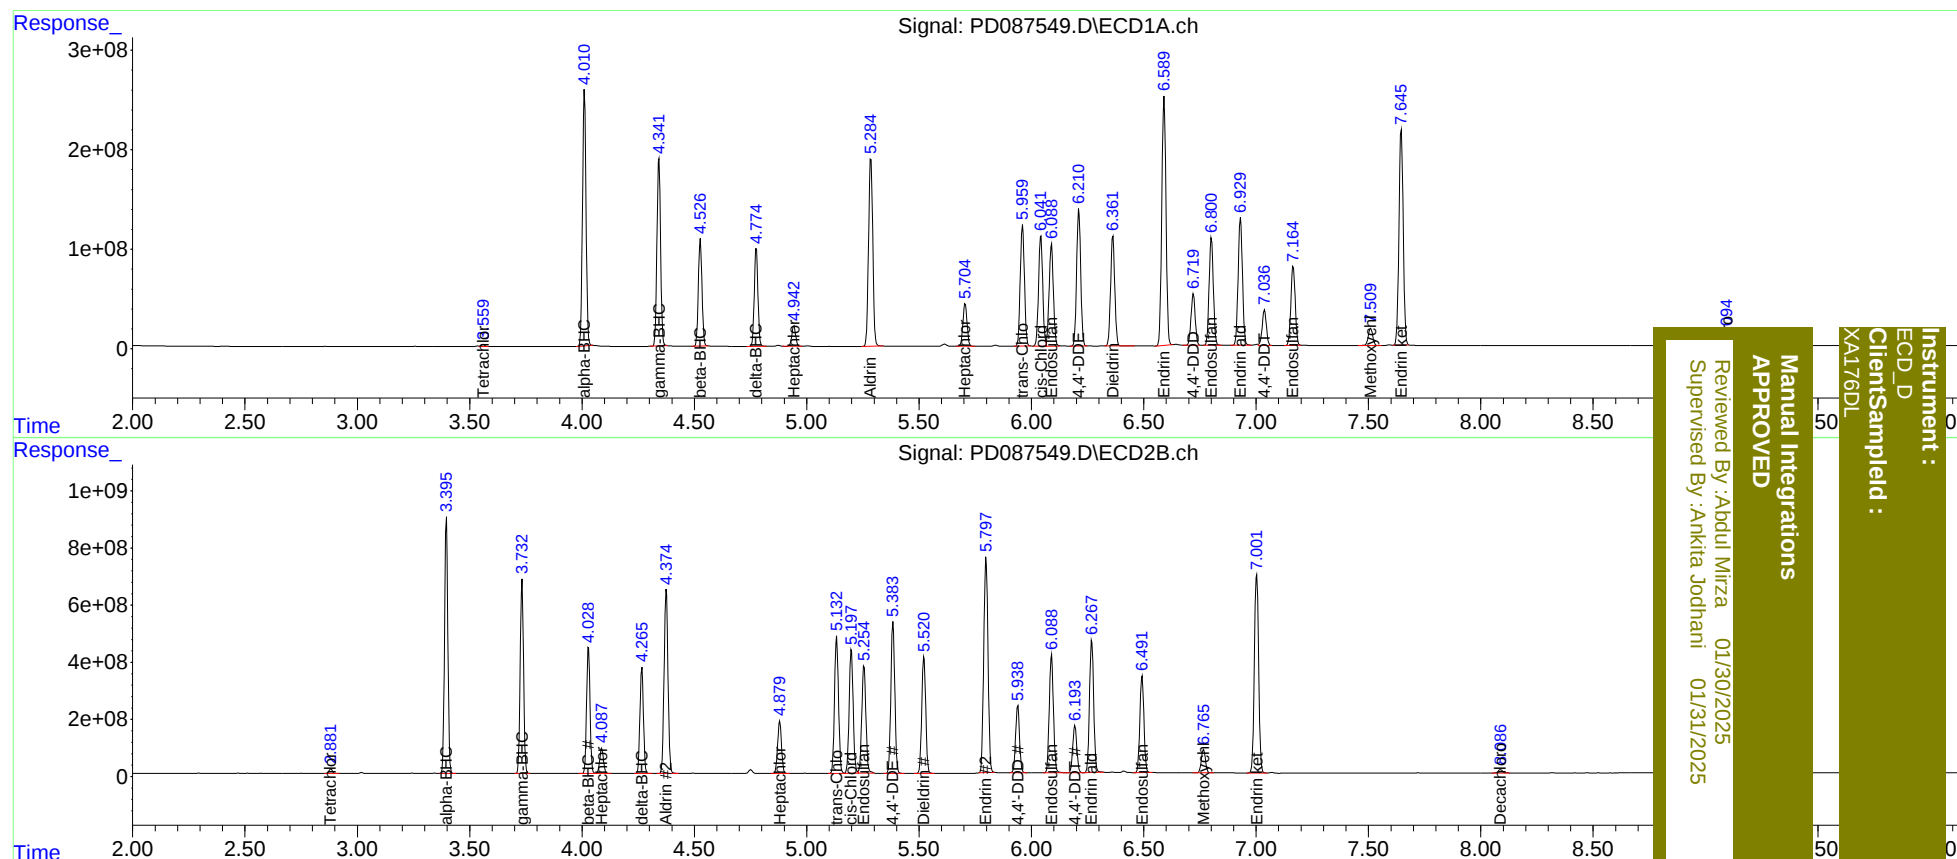

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/30/2025
Supervised By: Ankita Jodhani 01/31/2025

Instrument :
ECD_D
Client Sampled :
XA176DL