

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
 Data File : PD087562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2025 14:54
 Operator : AR\AJ
 Sample : Q1174-15MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2944MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/29/2025
 Supervised By : Ankita Jodhani 01/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 07:53:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.556	2.883	37181652	250.2E6	18.244	20.230
2) SA Decachlor...	9.090	8.087	62474264	285.0E6	18.686	19.673
Target Compounds						
2) A alpha-BHC	4.006	3.397	207.2E6	954.1E6	49.867	48.182
3) MA gamma-BHC...	4.337	3.734	199.4E6	876.2E6	49.568	47.837
4) MA Heptachlor	4.938	4.089	185.1E6	812.6E6	45.283	43.539
5) MB Aldrin	5.280	4.375	180.5E6	793.6E6	45.067	43.910
6) B beta-BHC	4.522	4.030	74986261	359.6E6	41.751	42.151
7) B delta-BHC	4.771	4.267	198.7E6	858.3E6	48.074	45.989
8) B Heptachlo...	5.699	4.880	165.4E6	728.7E6	44.282m	43.055
9) A Endosulfan I	6.082	5.255	153.8E6	686.5E6	44.155m	43.251
10) B trans-Chl...	5.955	5.134	159.4E6	779.0E6	43.261	43.331
11) B cis-Chlor...	6.035	5.199	163.1E6	754.5E6	43.883m	43.595
12) B 4,4'-DDE	6.204	5.384	312.6E6	1418.1E6	88.765m	86.580
13) MA Dieldrin	6.357	5.521	348.0E6	1470.8E6	91.285	88.123
14) MA Endrin	6.584	5.798	288.2E6	1349.9E6	88.805	90.341
15) B Endosulfa...	6.796	6.090	274.8E6	1277.8E6	85.366	86.249
16) A 4,4'-DDD	6.715	5.939	244.4E6	1200.6E6	88.872	89.803
17) MA 4,4'-DDT	7.032	6.194	261.7E6	1220.6E6	90.311	88.573
18) B Endrin al...	6.924	6.268	205.5E6	953.9E6	81.573	82.741
19) B Endosulfa...	7.159	6.492	264.9E6	1253.3E6	85.788	86.215
20) A Methoxychlor	7.503	6.766	641.4E6	2509.4E6	404.831	407.420
21) B Endrin ke...	7.639	7.002	288.7E6	1344.4E6	83.868m	84.647

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012825\
Data File : PD087562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2025 14:54
Operator : AR\AJ
Sample : Q1174-15MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 07:53:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

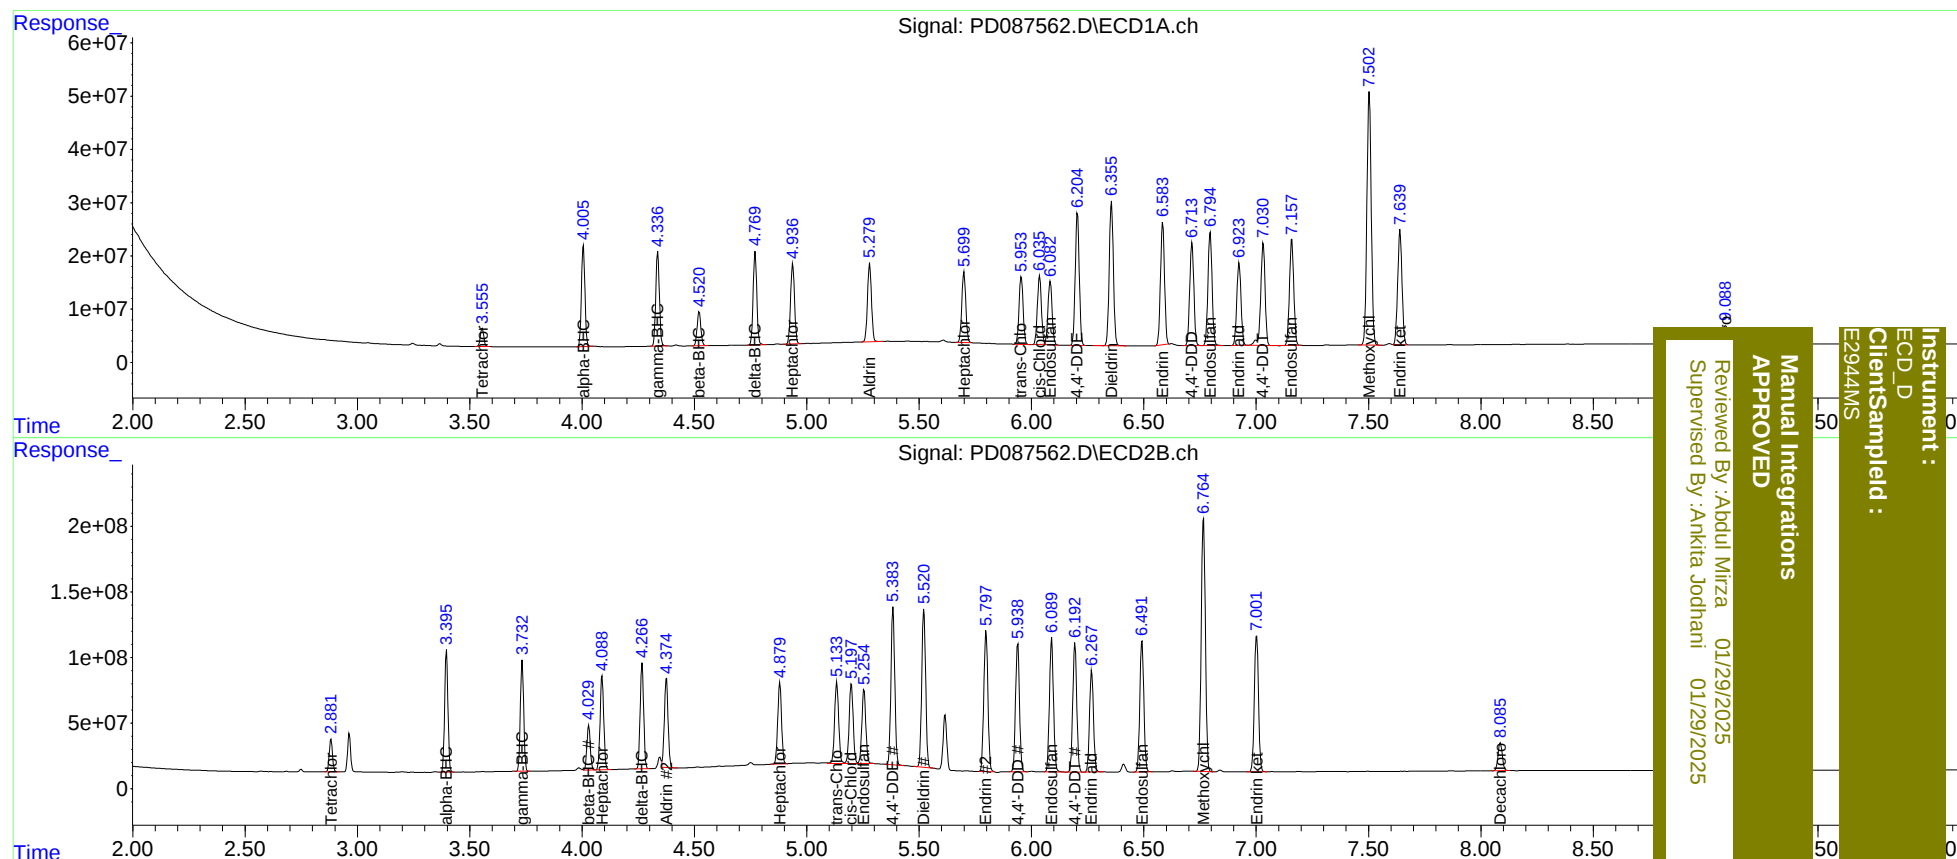

880.0
Reviewed By: Abdul Mirza 01/29/2025
Supervised By: Ankita Jodhani 01/29/2025

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
E2944MS