

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012919\
 Data File : PD051226.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2019 12:36
 Operator : AJ\SJ
 Sample : PIBLK40
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:12:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 03:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.225	4.045	28131235	566.9E6	20.159	19.883
27) SA Decachlor...	7.828	9.160	48527870	694.6E6	39.721	37.344
Target Compounds						
6) B beta-BHC	0.000	4.936f	0 91119970	N.D.		4.937
8) B Heptachlo...	0.000	5.927	0 401.2E6	N.D.		11.910
10) B trans-Chl...	0.000	6.122f	0 5529110	N.D.		0.164


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012919\
Data File : PD051226.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2019 12:36
Operator : AJ\SJ
Sample : PIBLK40
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:12:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 03:30:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

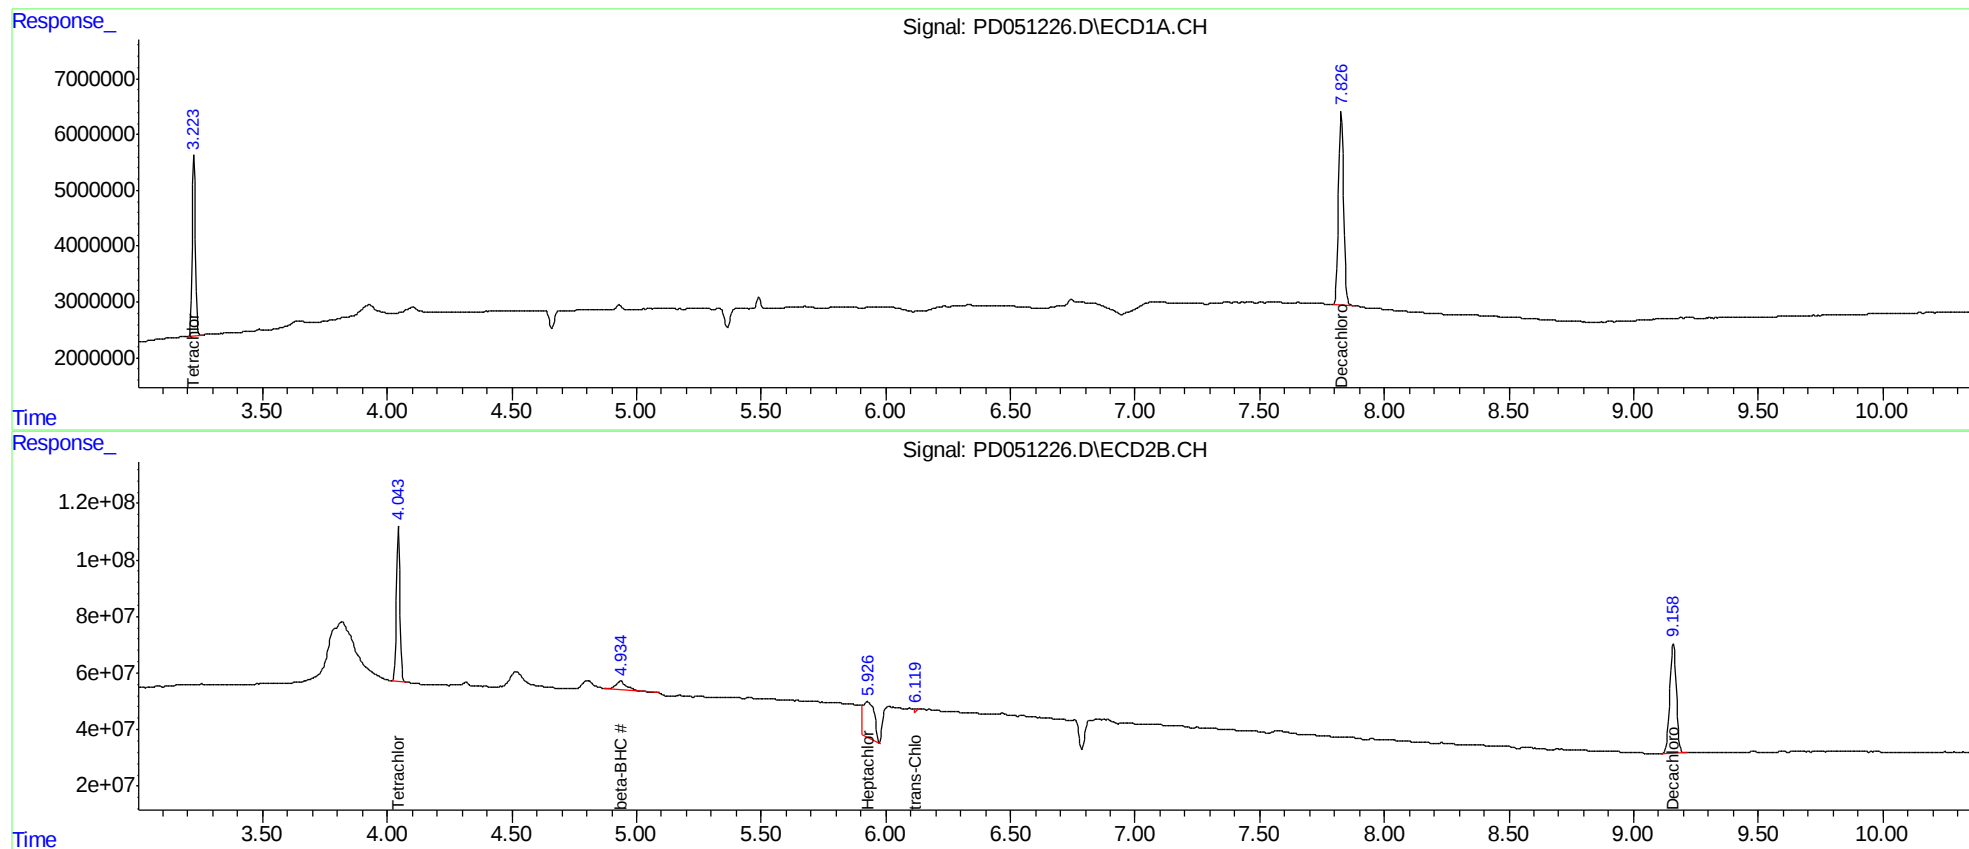


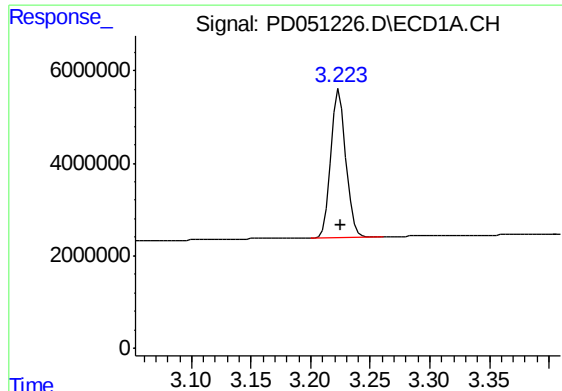

#1 Tetrachloro-m-xylene


R.T.: 3.225 min
Delta R.T.: 0.000 min
Response: 28131235
Conc: 20.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK40

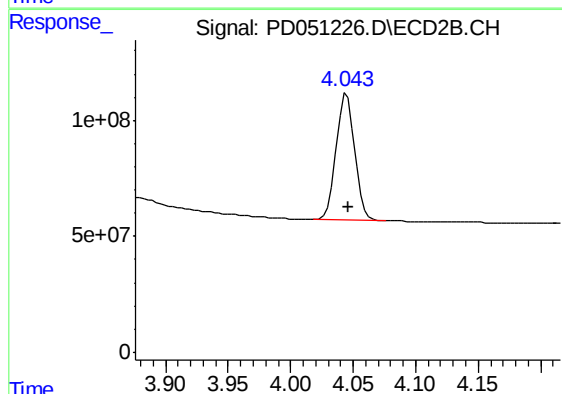


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 566887564
Conc: 19.88 ng/ml

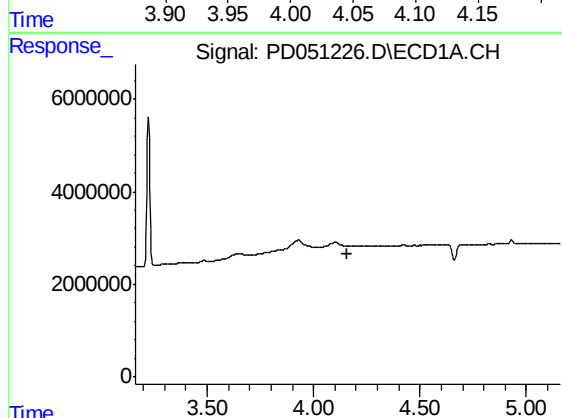


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

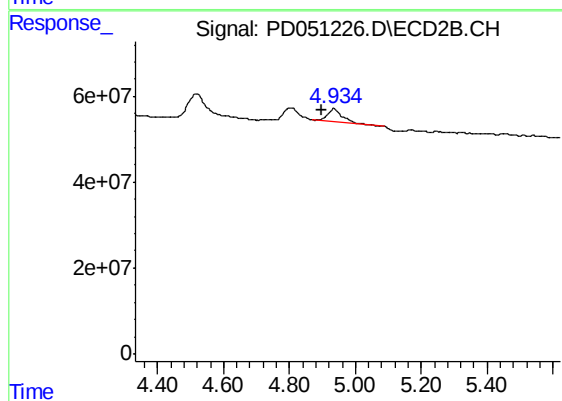

#6 beta-BHC


R.T.: 4.936 min
Delta R.T.: 0.040 min
Response: 91119970
Conc: 4.94 ng/ml

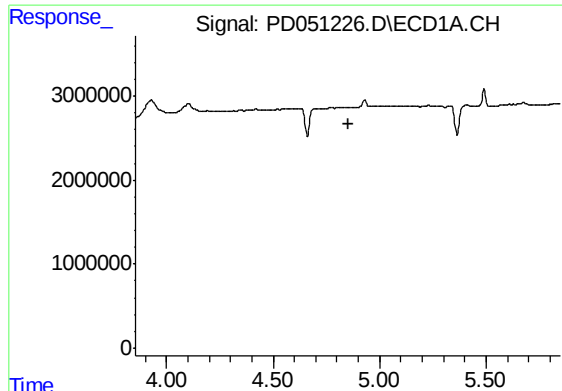

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK40

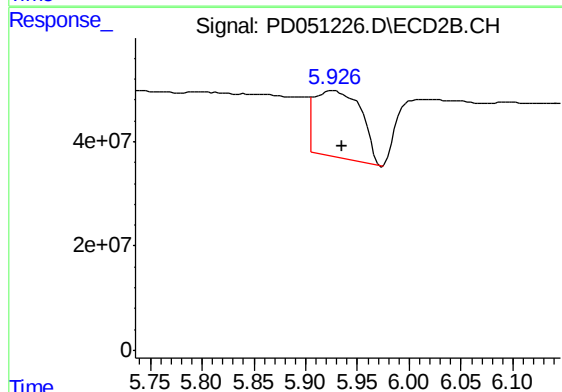


#8 Heptachlor epoxide

R.T.: 5.927 min
Delta R.T.: -0.009 min
Response: 401163654
Conc: 11.91 ng/ml

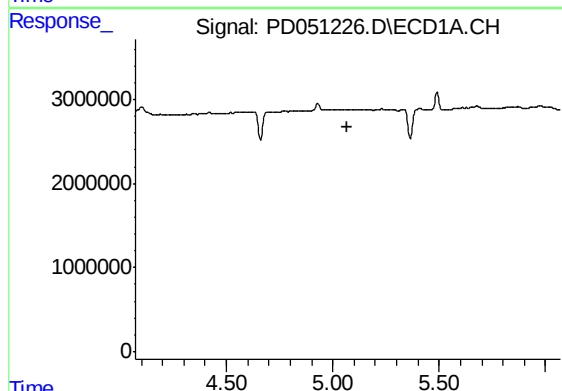


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

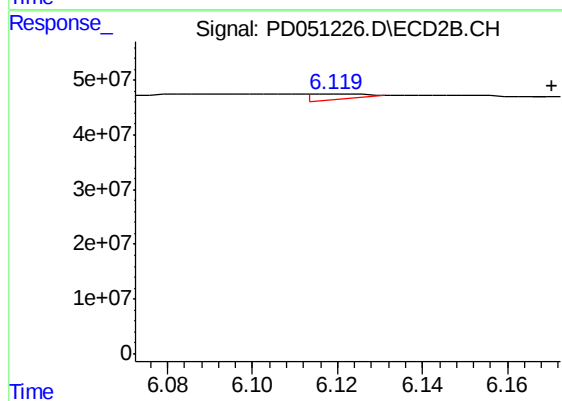

#10 trans-Chlordane


R.T.: 6.122 min
Delta R.T.: -0.049 min
Response: 5529110
Conc: 0.16 ng/ml

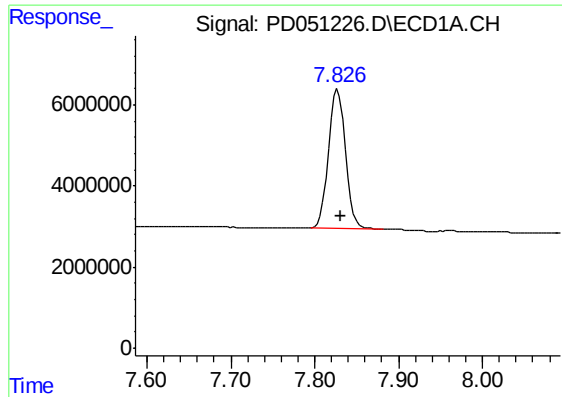

#27 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: -0.004 min
Response: 48527870
Conc: 39.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK40

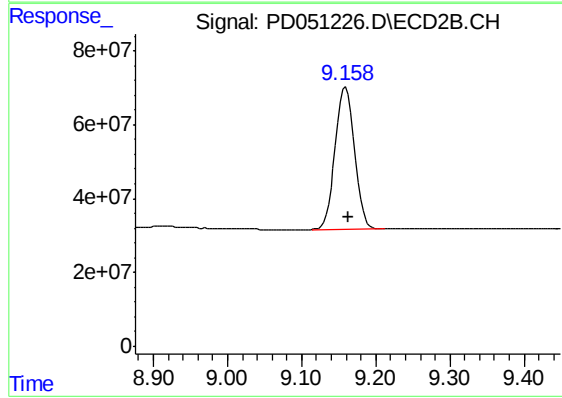

#27 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: -0.004 min
Response: 694554962
Conc: 37.34 ng/ml