

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
 Data File : PD061077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 10:48
 Operator : DD\AJ
 Sample : M1263-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:14:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:48:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.020	18670920	143.0E6	21.143	21.155
28)	SA Decachlor...	8.283	9.107	12530040	92392673	14.550	15.151
Target Compounds							
2)	A alpha-BHC	0.000	4.412	0	36776495	N.D.	3.315 #
3)	MA gamma-BHC...	0.000	4.701	0	7716616	N.D.	0.759 #
4)	MA Heptachlor	0.000	5.188f	0	2757129	N.D.	0.271 #
5)	MB Aldrin	4.770	0.000	2649873	0	2.125	N.D. #
6)	B beta-BHC	4.442f	0.000	10511994	0	18.175	N.D. #
7)	B delta-BHC	0.000	5.059f	0	85589344	N.D.	8.587 #
8)	B Heptachlo...	0.000	5.921f	0	2026660	N.D.	0.251 #
14)	MA Endrin	0.000	6.748	0	2479331	N.D.	0.352 #
15)	B Endosulfa...	0.000	6.946	0	1433037	N.D.	0.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
Data File : PD061077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 10:48
Operator : DD\AJ
Sample : M1263-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:14:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:48:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

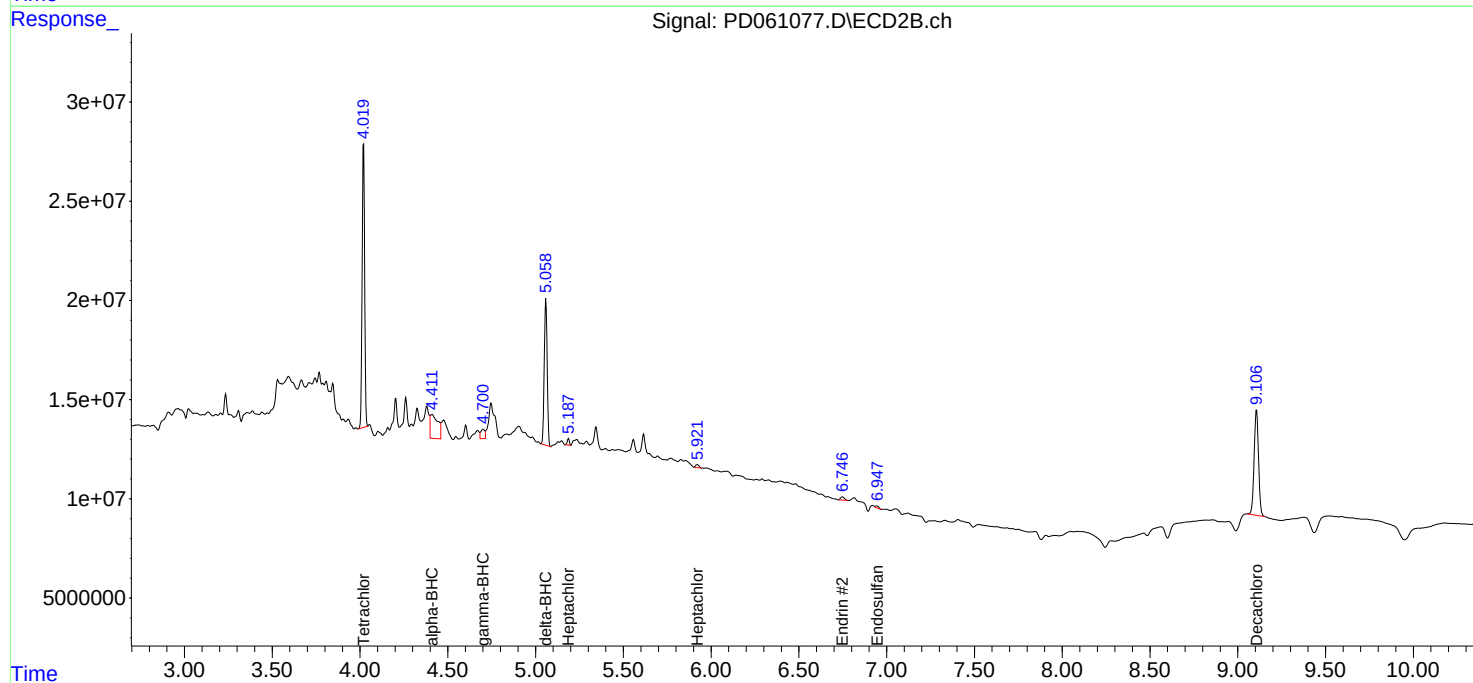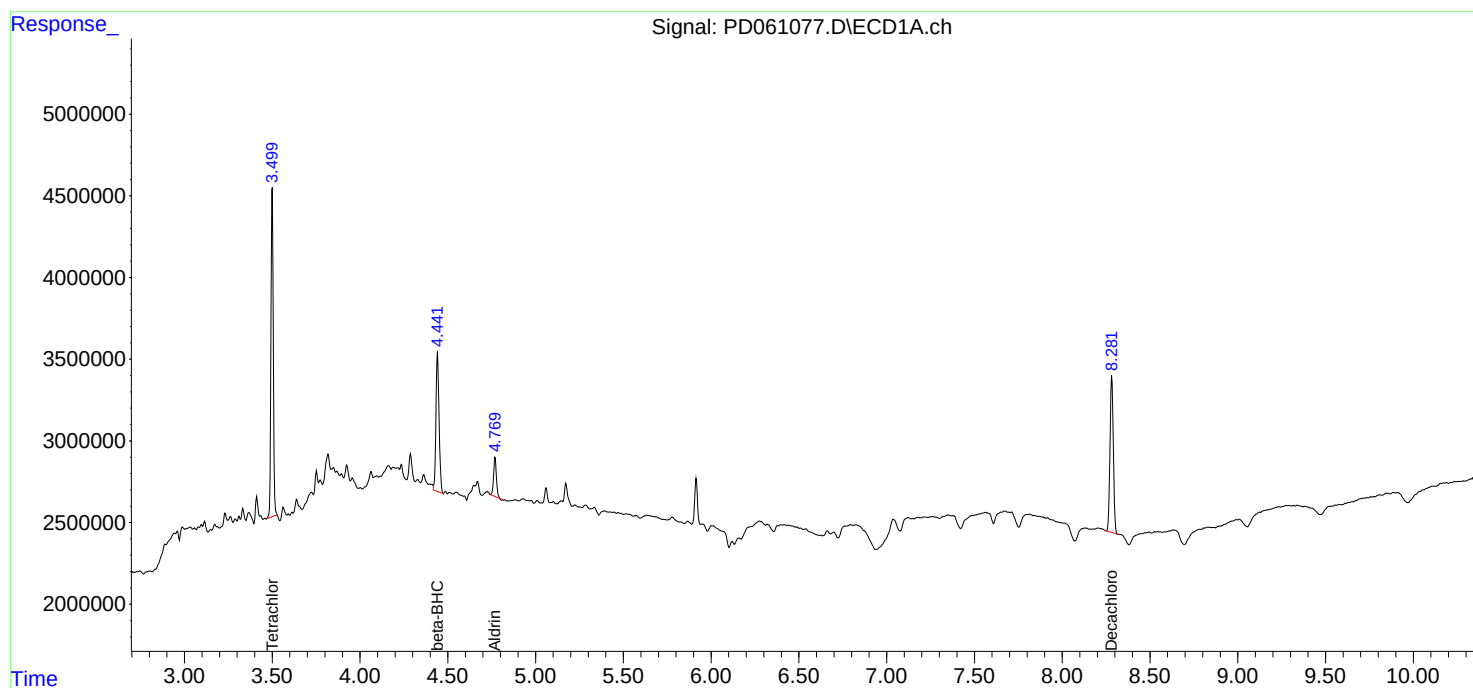


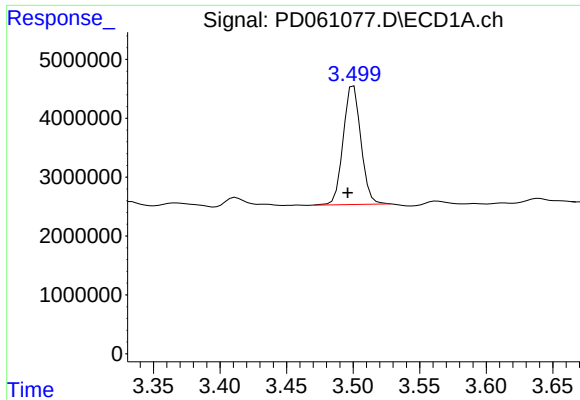

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.004 min
Response: 18670920
Conc: 21.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

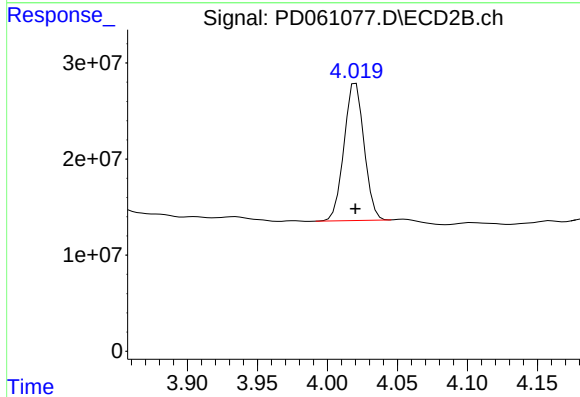


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 142974097
Conc: 21.15 ng/ml

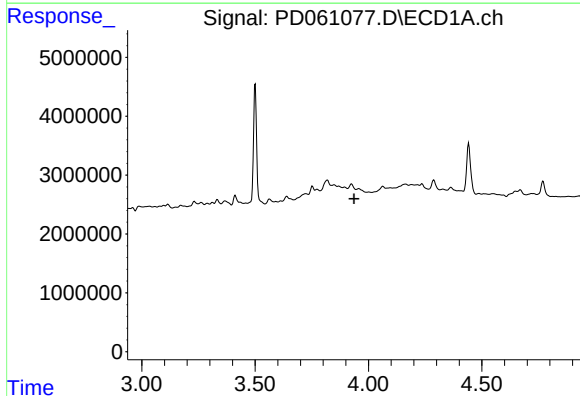


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.937 min
Response: 0
Conc: N.D.

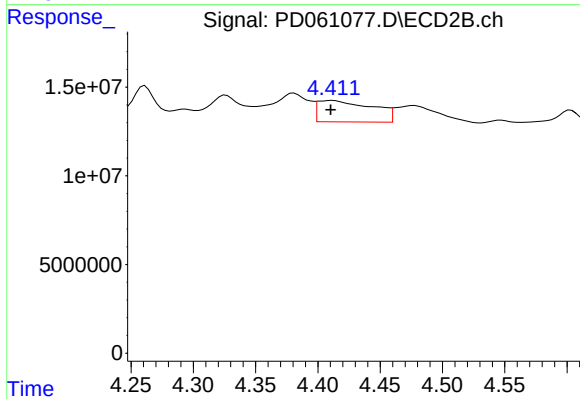

#2 alpha-BHC


R.T.: 4.412 min
Delta R.T.: 0.001 min
Response: 36776495
Conc: 3.32 ng/ml

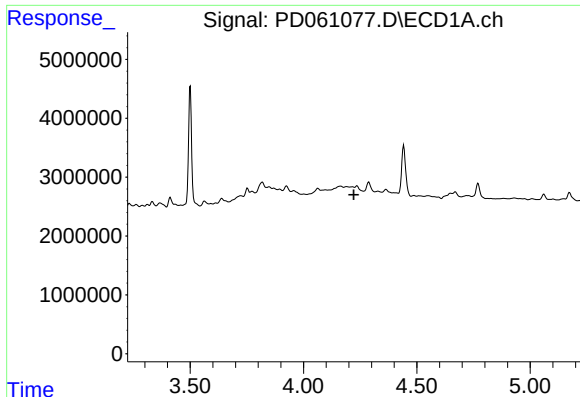

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

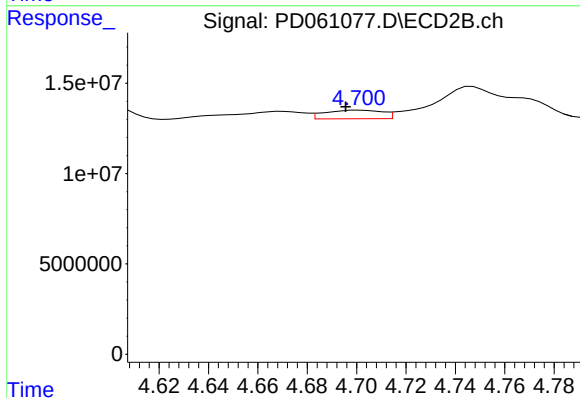


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.006 min
Response: 7716616
Conc: 0.76 ng/ml

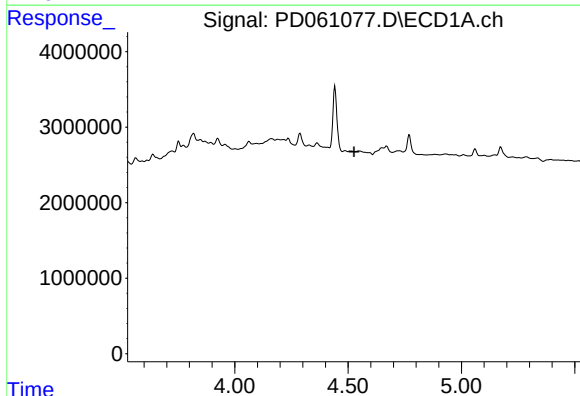


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.526 min
Response: 0
Conc: N.D.

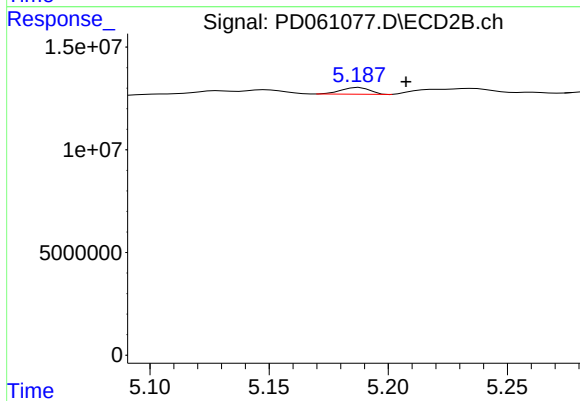

#4 Heptachlor


R.T.: 5.188 min
Delta R.T.: -0.020 min
Response: 2757129
Conc: 0.27 ng/ml

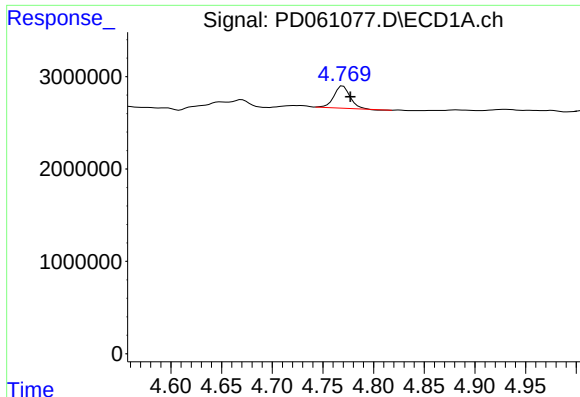

#5 Aldrin


R.T.: 4.770 min
Delta R.T.: -0.007 min
Response: 2649873
Conc: 2.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

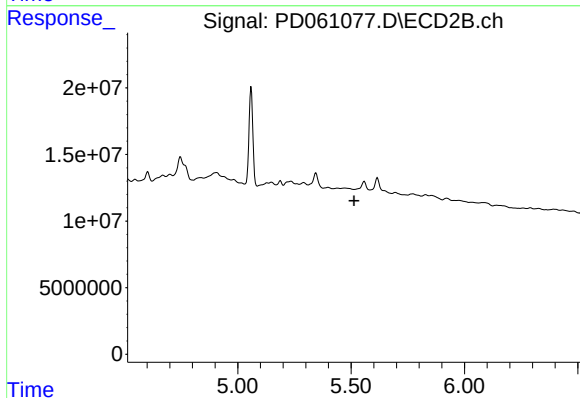


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.514 min
Response: 0
Conc: N.D.

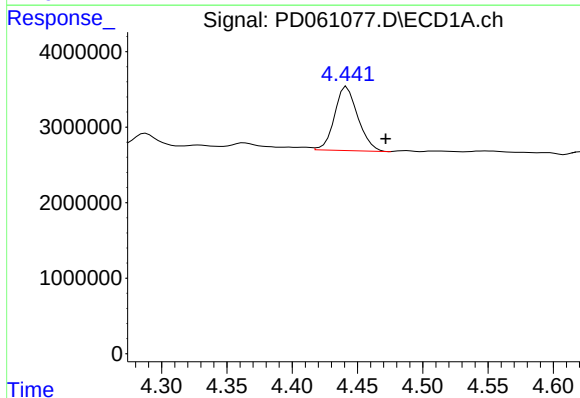


#6 beta-BHC

R.T.: 4.442 min
Delta R.T.: -0.030 min
Response: 10511994
Conc: 18.18 ng/ml

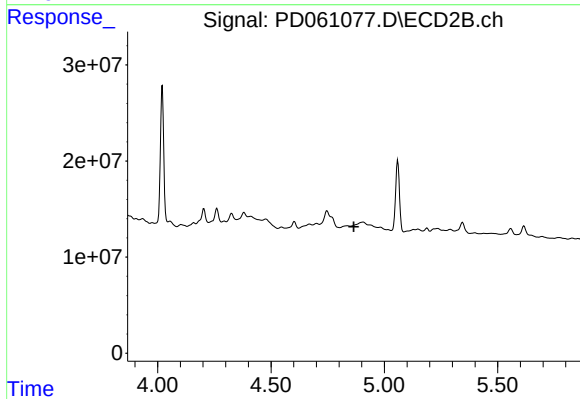

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.865 min
Response: 0
Conc: N.D.

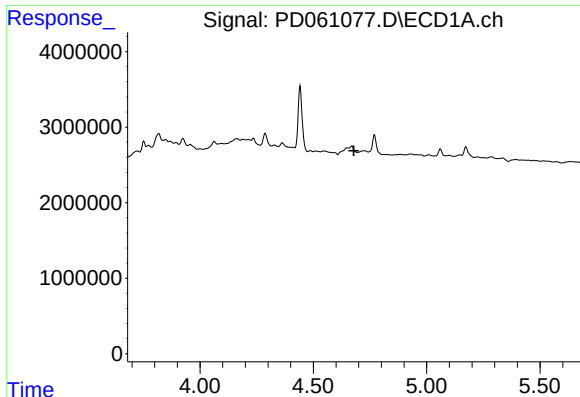

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.679 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

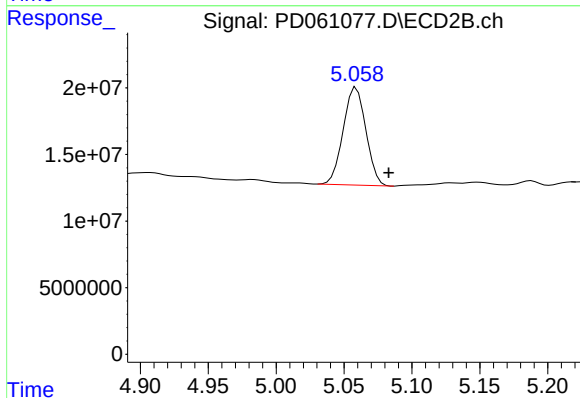


#7 delta-BHC

R.T.: 5.059 min
Delta R.T.: -0.024 min
Response: 85589344
Conc: 8.59 ng/ml

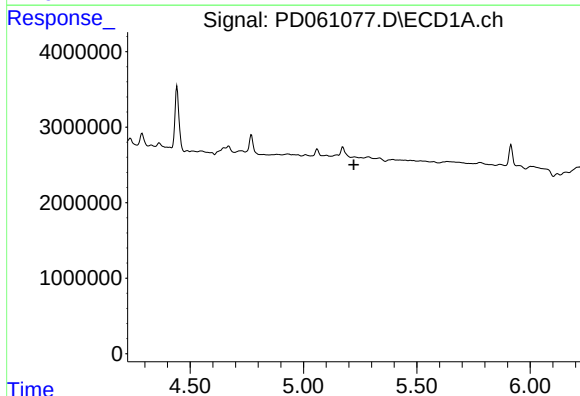


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.222 min
Response: 0
Conc: N.D.

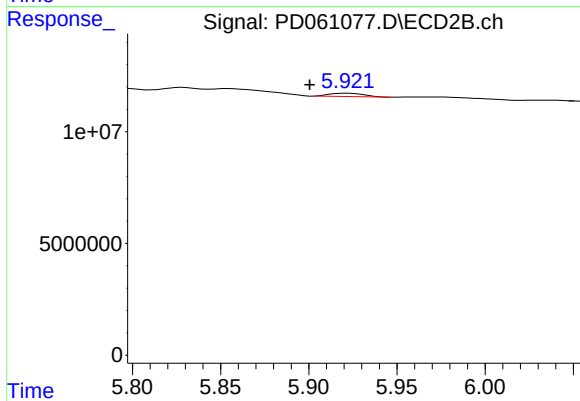

#8 Heptachlor epoxide


R.T.: 5.921 min
Delta R.T.: 0.021 min
Response: 2026660
Conc: 0.25 ng/ml

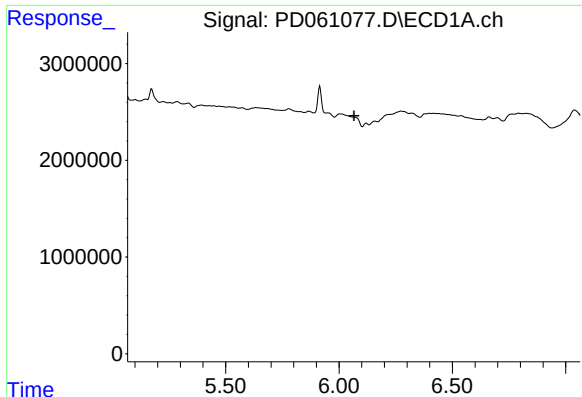

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

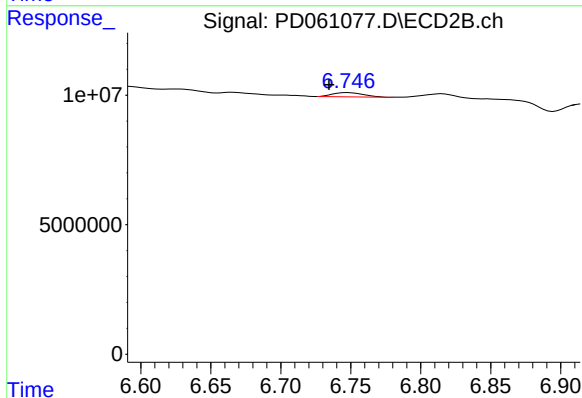


#14 Endrin

R.T.: 6.748 min
Delta R.T.: 0.013 min
Response: 2479331
Conc: 0.35 ng/ml

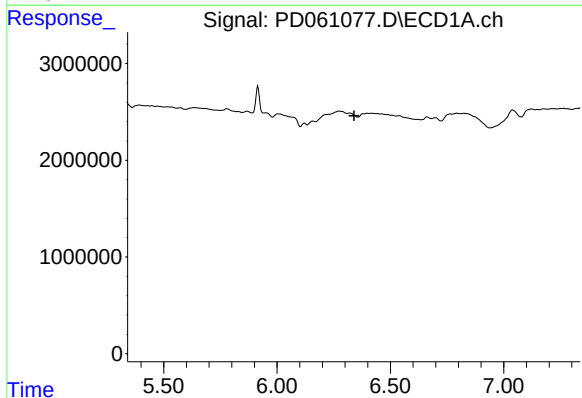


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.340 min
Response: 0
Conc: N.D.

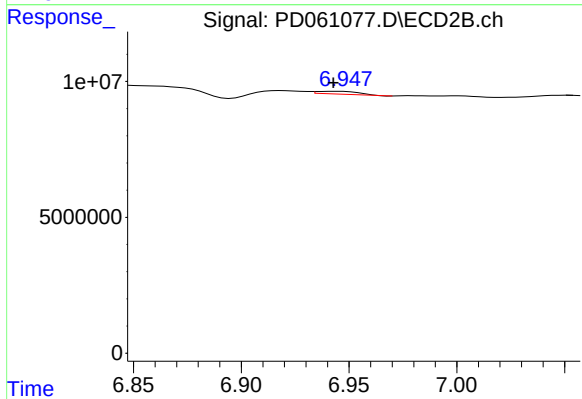

#15 Endosulfan II


R.T.: 6.946 min
Delta R.T.: 0.004 min
Response: 1433037
Conc: 0.20 ng/ml

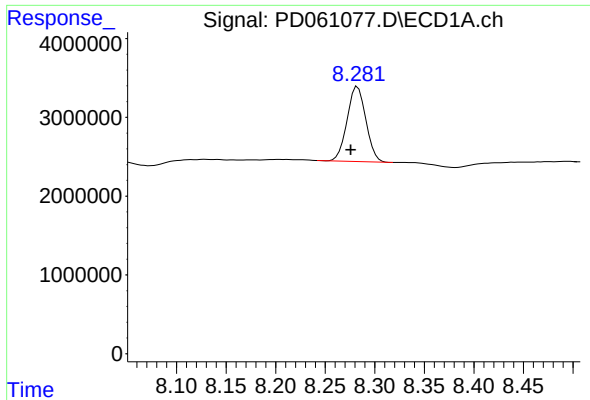

#28 Decachlorobiphenyl

R.T.: 8.283 min
Delta R.T.: 0.007 min
Response: 12530040
Conc: 14.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

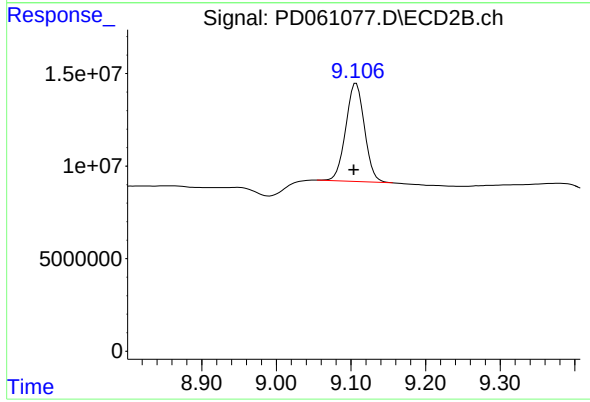

#28 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.003 min
Response: 92392673
Conc: 15.15 ng/ml