

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
 Data File : PD061088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 13:37
 Operator : DD\AJ
 Sample : M1255-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:16:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:48:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.021	17693351	131.0E6	20.036	19.386
28)	SA Decachlor...	8.276	9.105	16420961	117.1E6	19.068	19.209
Target Compounds							
7)	B delta-BHC	0.000	5.059f	0	19895192	N.D.	1.996 #
8)	B Heptachlo...	0.000	5.905	0	1826370	N.D.	0.226 #
10)	B gamma-Chl...	0.000	6.120f	0	3393785	N.D.	0.396 #
11)	B alpha-Chl...	0.000	6.226f	0	3801331	N.D.	0.449 #
13)	MA Dieldrin	0.000	6.541f	0	1298046	N.D.	0.151 #
14)	MA Endrin	0.000	6.760f	0	5969901	N.D.	0.848 #
15)	B Endosulfa...	0.000	6.913f	0	1442738	N.D.	0.197 #
17)	MA 4,4'-DDT	0.000	7.161	0	4660311	N.D.	0.702 #
19)	B Endosulfa...	0.000	7.266f	0	3524316	N.D.	0.501 #
25)	Chlordane-3	0.000	6.120	0	3393785	N.D.	3.208 #
26)	Chlordane-4	0.000	6.226f	0	3801331	N.D.	3.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
Data File : PD061088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 13:37
Operator : DD\AJ
Sample : M1255-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:48:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

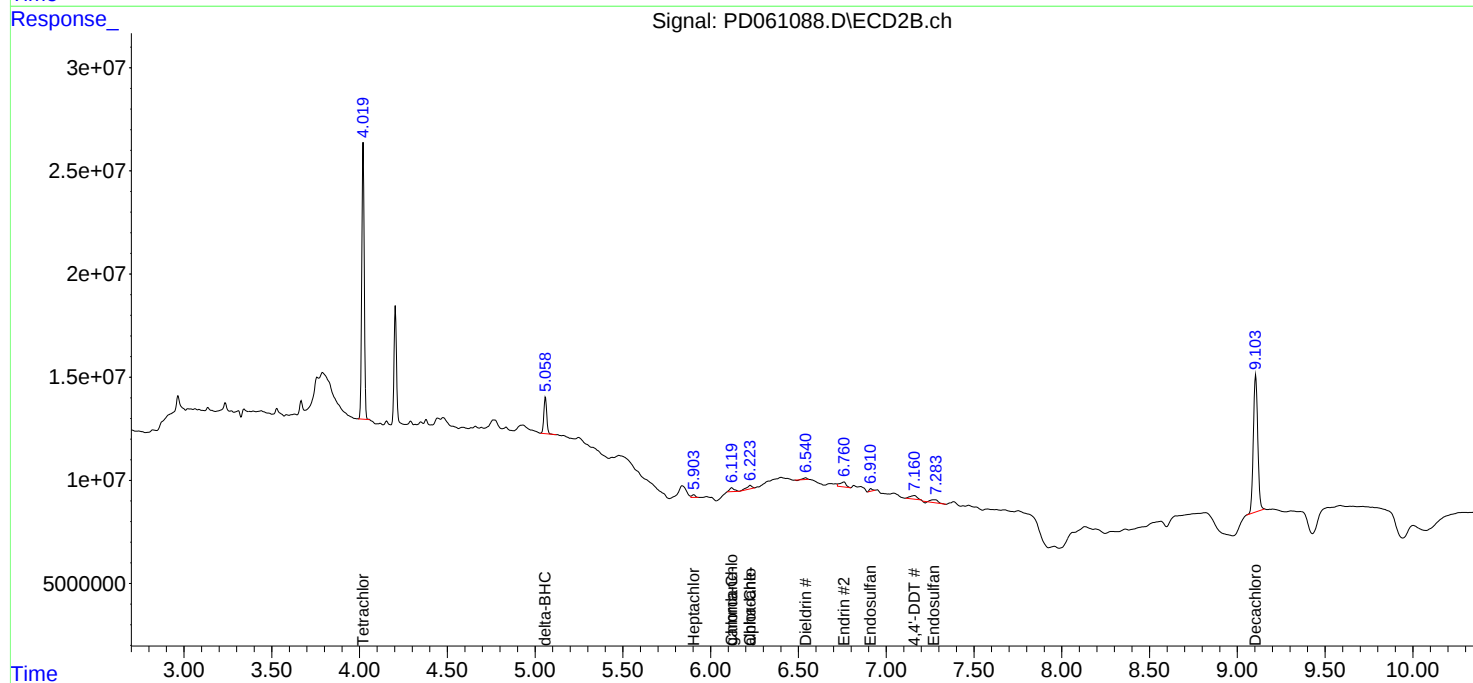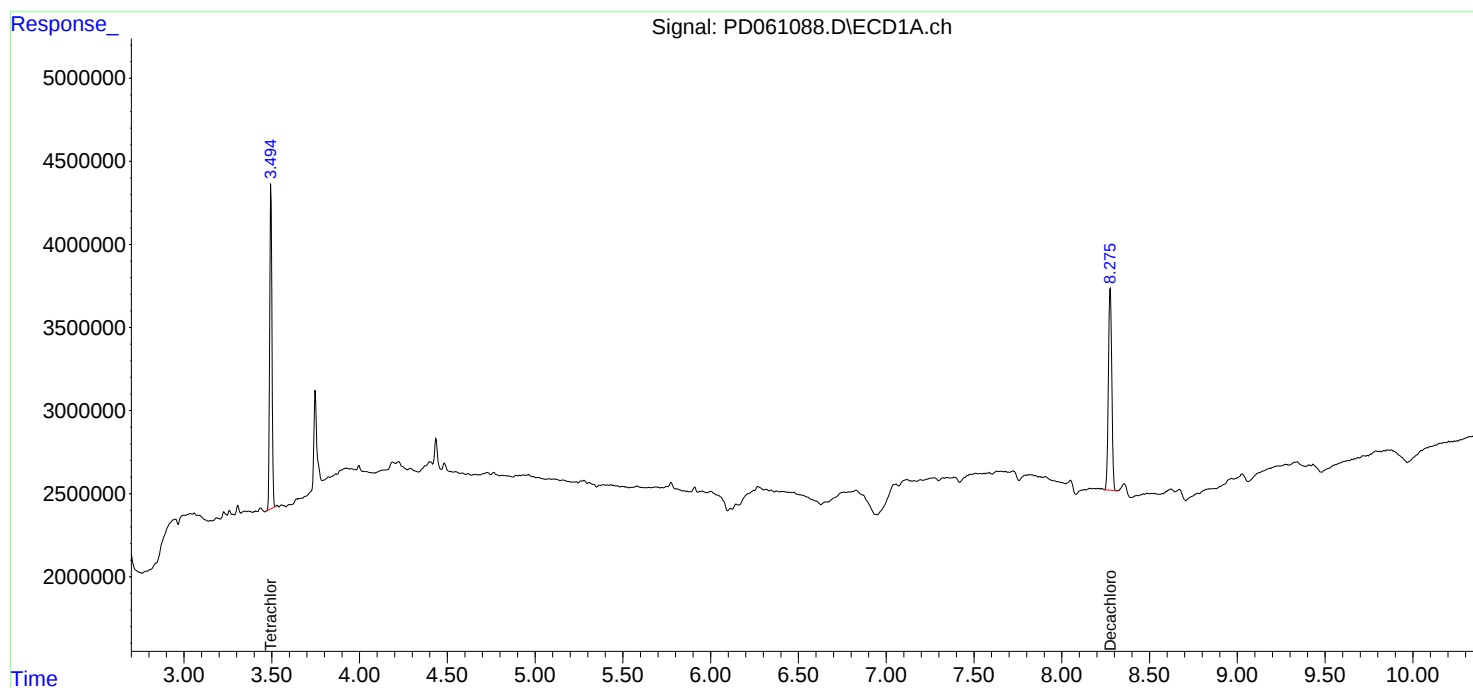


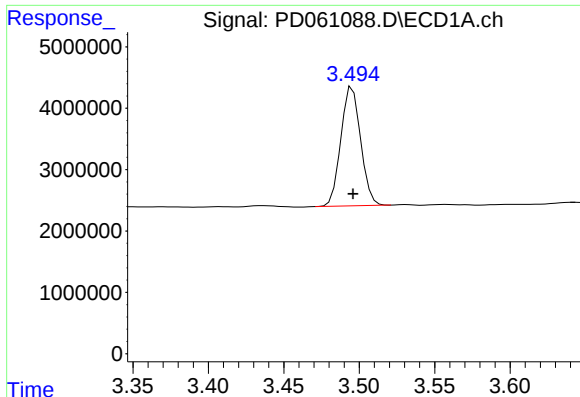

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 17693351
Conc: 20.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

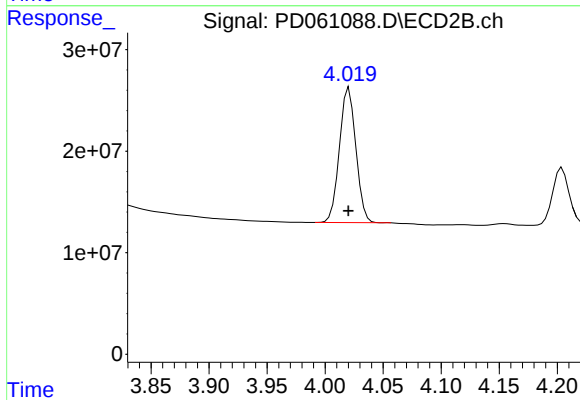


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 131022033
Conc: 19.39 ng/ml

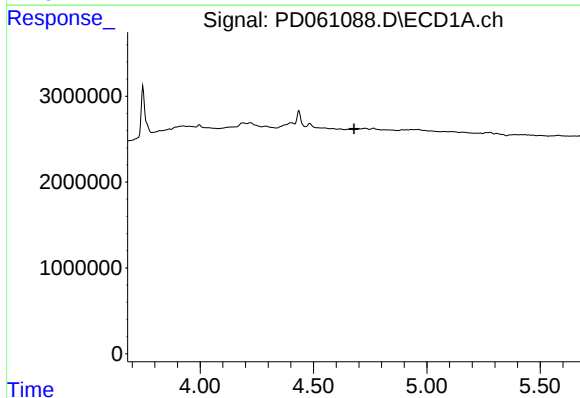


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.679 min
Response: 0
Conc: N.D.

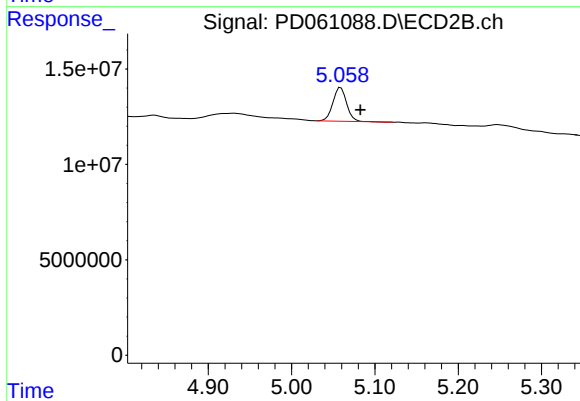

#7 delta-BHC


R.T.: 5.059 min
Delta R.T.: -0.024 min
Response: 19895192
Conc: 2.00 ng/ml

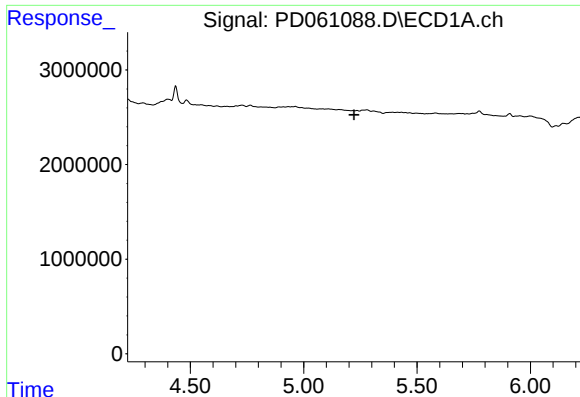

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

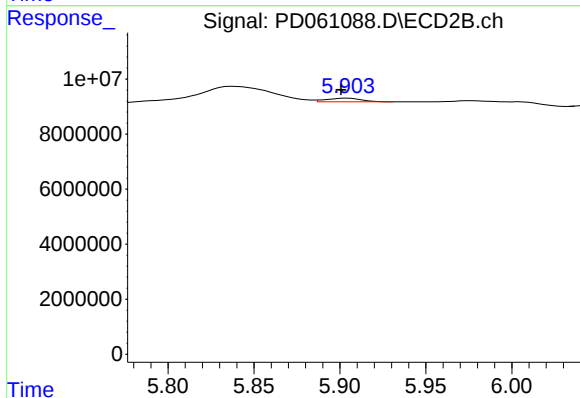


#8 Heptachlor epoxide

R.T.: 5.905 min
Delta R.T.: 0.004 min
Response: 1826370
Conc: 0.23 ng/ml

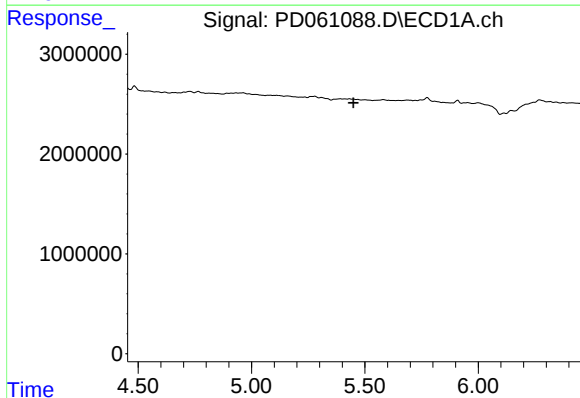


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.450 min
Response: 0
Conc: N.D.

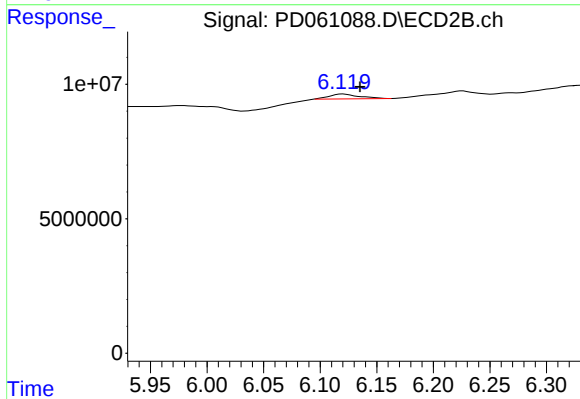

#10 gamma-Chlordane


R.T.: 6.120 min
Delta R.T.: -0.015 min
Response: 3393785
Conc: 0.40 ng/ml

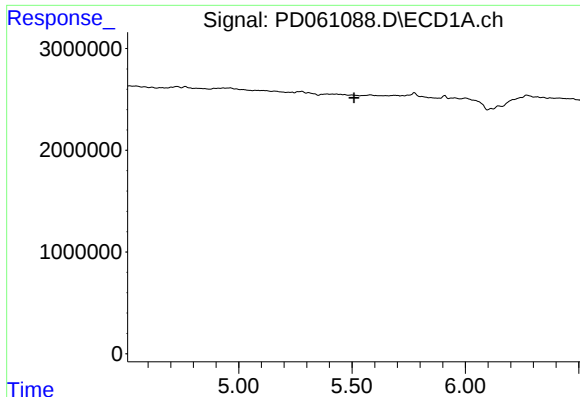

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

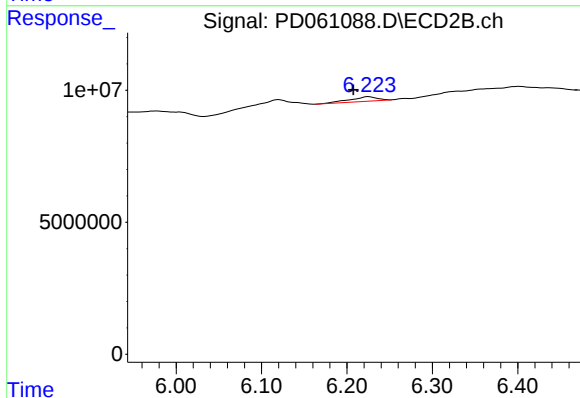


#11 alpha-Chlordane

R.T.: 6.226 min
Delta R.T.: 0.018 min
Response: 3801331
Conc: 0.45 ng/ml

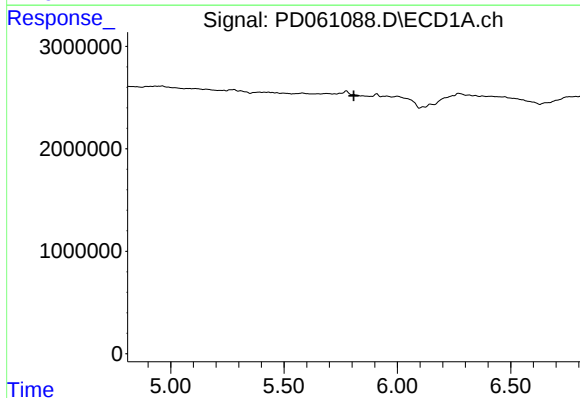


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.808 min
Response: 0
Conc: N.D.

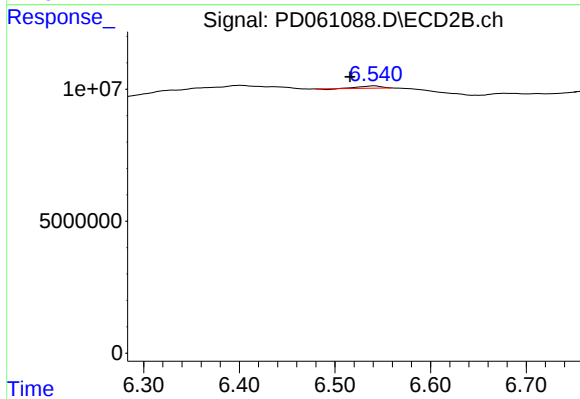

#13 Dieldrin


R.T.: 6.541 min
Delta R.T.: 0.026 min
Response: 1298046
Conc: 0.15 ng/ml

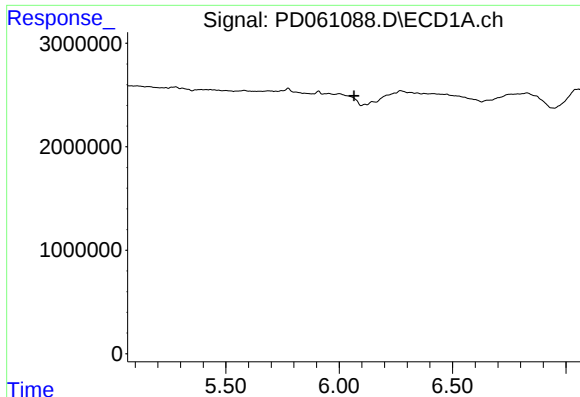

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.066 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

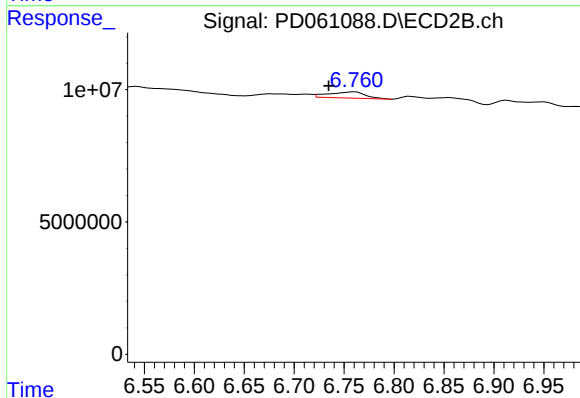


#14 Endrin

R.T.: 6.760 min
Delta R.T.: 0.026 min
Response: 5969901
Conc: 0.85 ng/ml

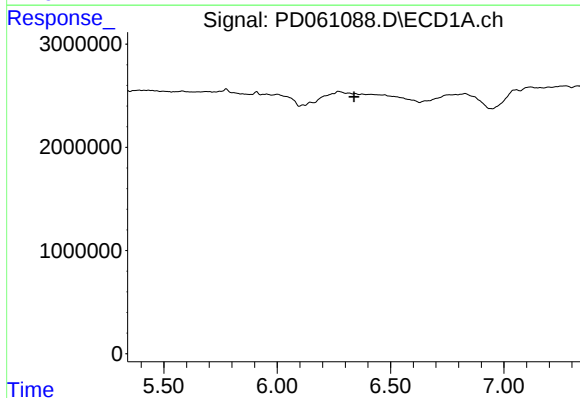


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.340 min
Response: 0
Conc: N.D.

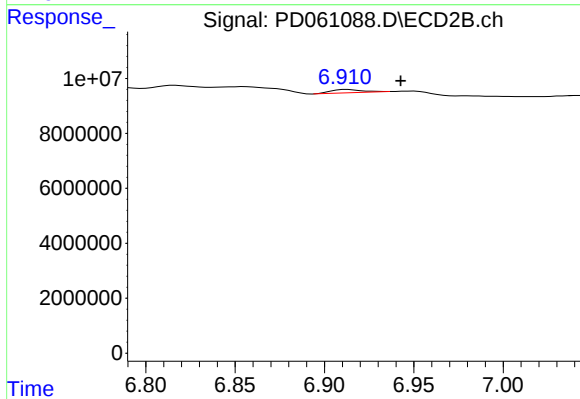

#15 Endosulfan II


R.T.: 6.913 min
Delta R.T.: -0.030 min
Response: 1442738
Conc: 0.20 ng/ml

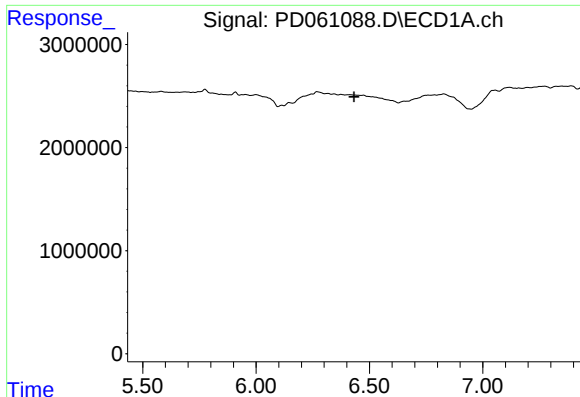

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.433 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

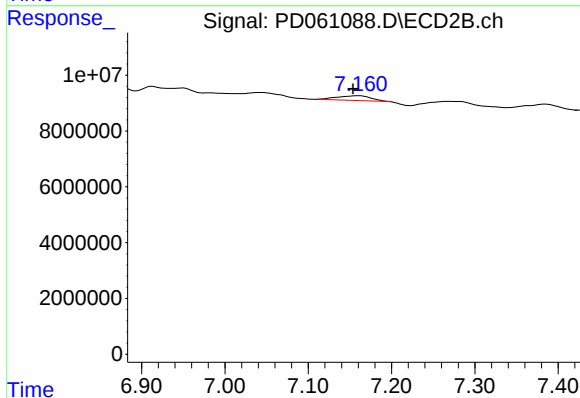


#17 4,4'-DDT

R.T.: 7.161 min
Delta R.T.: 0.008 min
Response: 4660311
Conc: 0.70 ng/ml

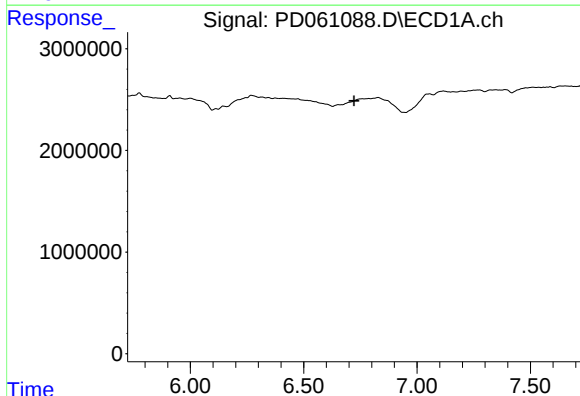


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.723 min
Response: 0
Conc: N.D.

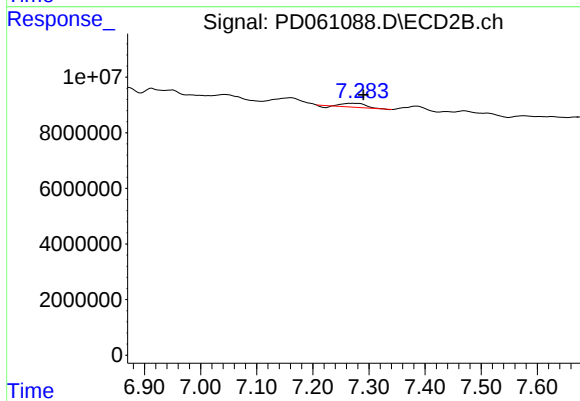

#19 Endosulfan Sulfate


R.T.: 7.266 min
Delta R.T.: -0.024 min
Response: 3524316
Conc: 0.50 ng/ml

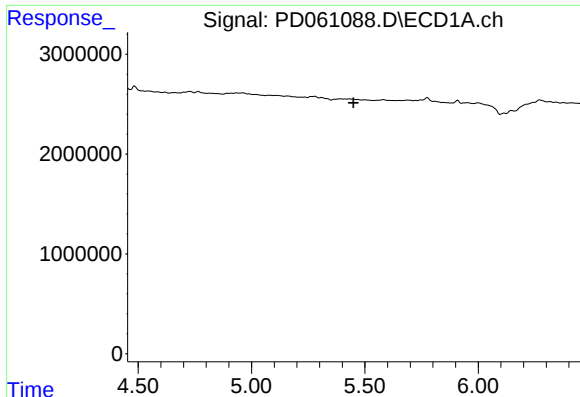

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.450 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

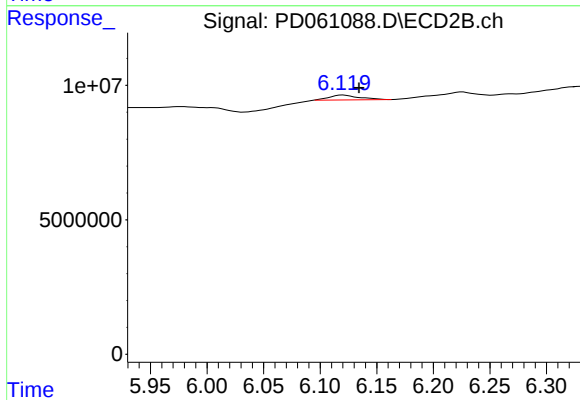


#25 Chlordane-3

R.T.: 6.120 min
Delta R.T.: -0.014 min
Response: 3393785
Conc: 3.21 ng/ml

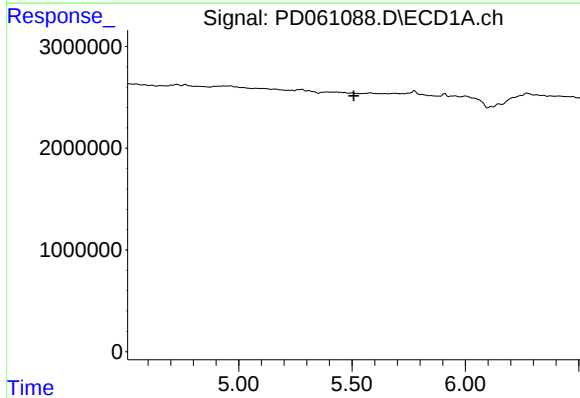


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

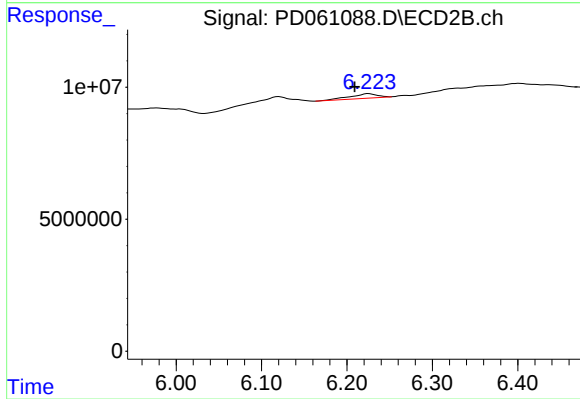

#26 Chlordane-4


R.T.: 6.226 min
Delta R.T.: 0.016 min
Response: 3801331
Conc: 3.09 ng/ml

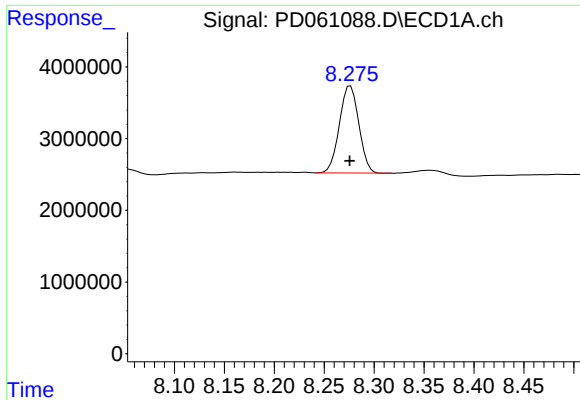

#28 Decachlorobiphenyl

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 16420961
Conc: 19.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

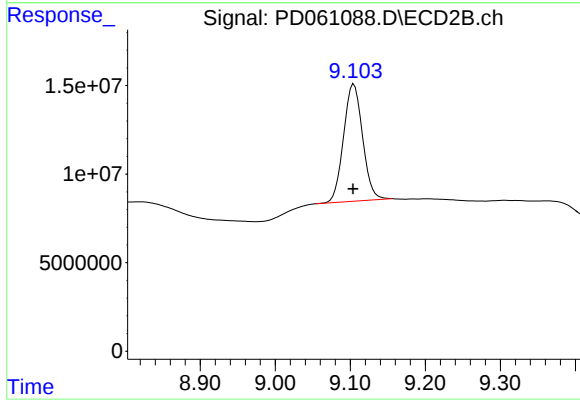

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 117141937
Conc: 19.21 ng/ml