

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 08:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:18:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
7) B	delta-BHC	0.000	5.199	0	2517526	N.D. 0.817 #
8) B	Heptachlo...	0.000	6.021	0	530344	N.D. 0.207 #
9) A	Endosulfan I	0.000	6.381	0	7822694	N.D. 2.941 #
10) B	gamma-Chl...	5.381f	0.000	8064089	0	1.948 N.D. #
11) B	alpha-Chl...	0.000	6.323	0	29994621	N.D. 10.193 #
13) MA	Dieldrin	5.697	0.000	3556674	0	0.889 N.D. #
14) MA	Endrin	5.985f	0.000	2550536	0	0.697 N.D. #
18) B	Endrin al...	6.389	0.000	1627878	0	0.531 N.D. #
25)	Chlordane-3	5.381f	0.000	8064089	0	22.355 N.D. #
26)	Chlordane-4	0.000	6.323	0	29994621	N.D. 68.207 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 08:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:18:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

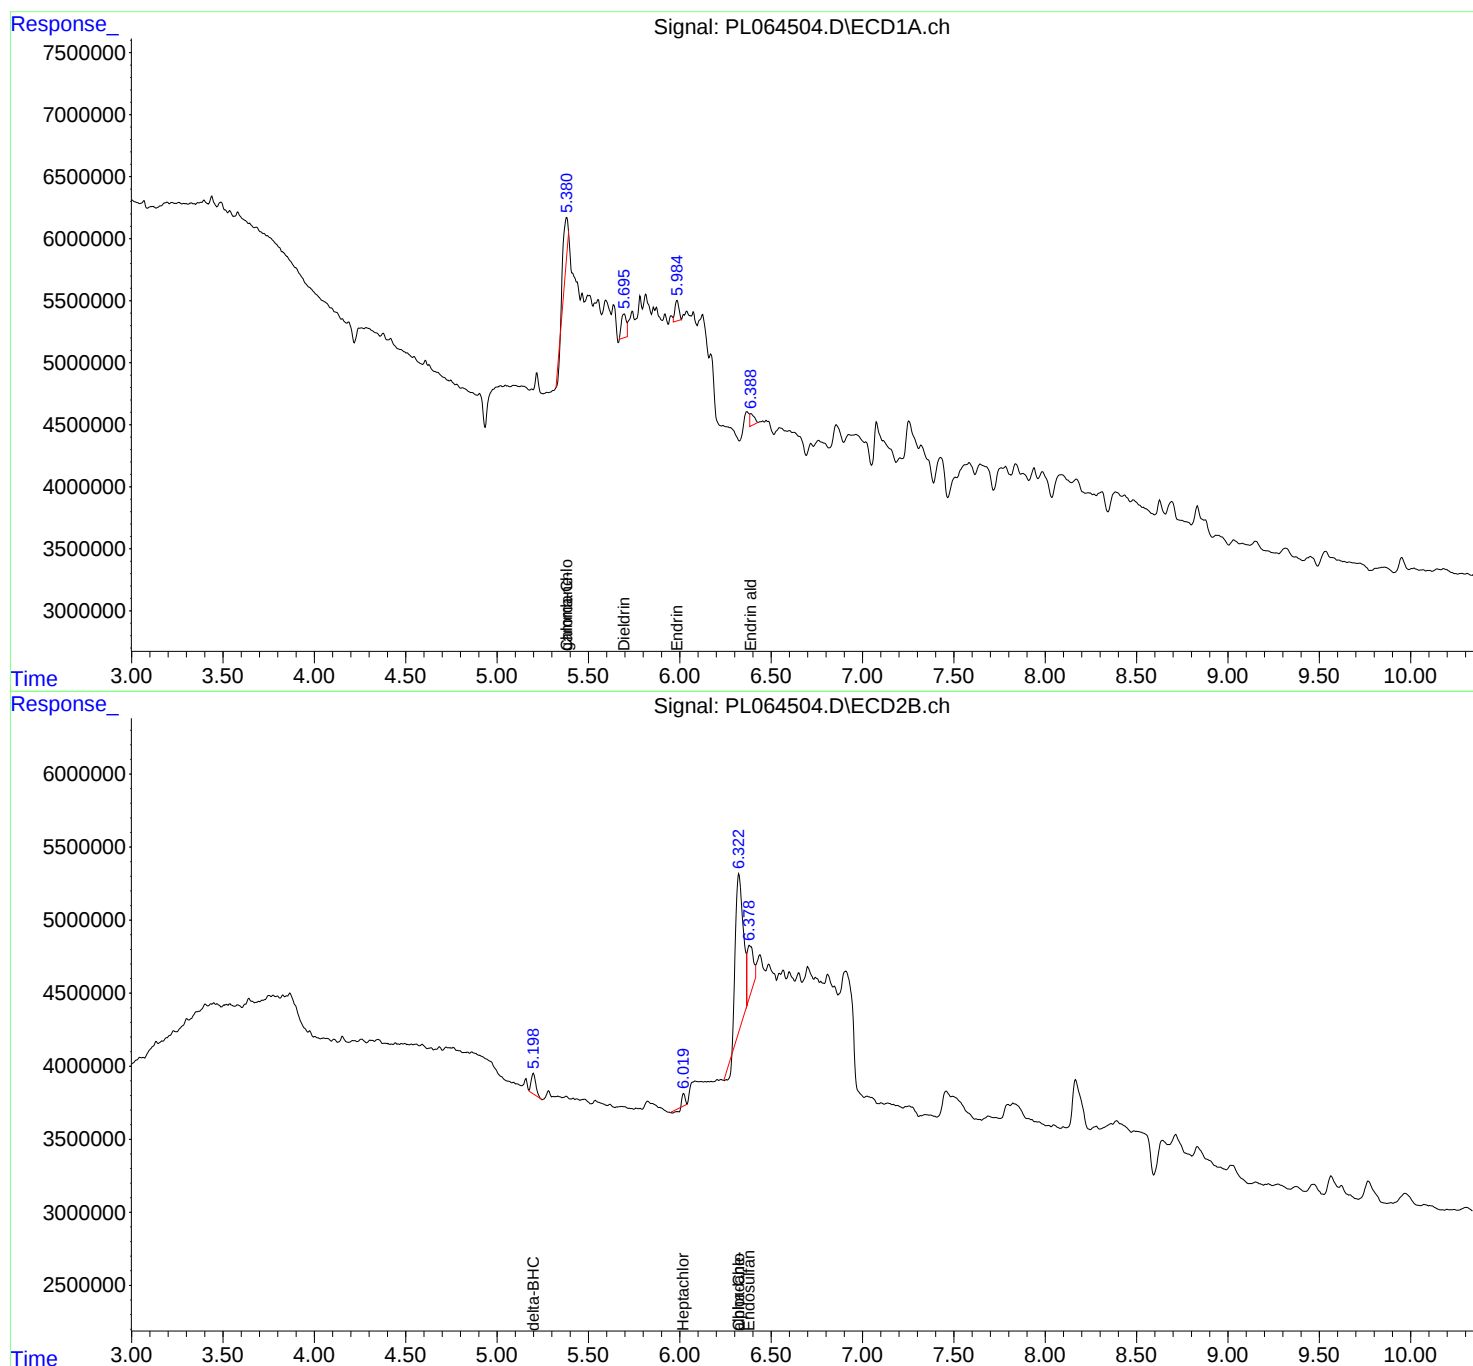


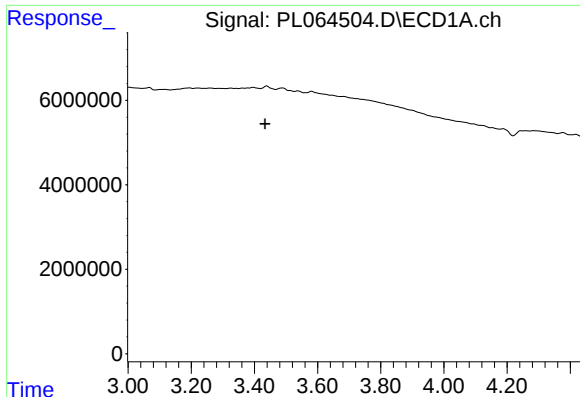

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.433 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

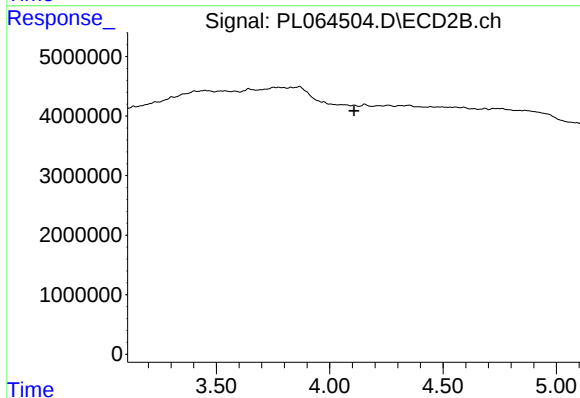


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

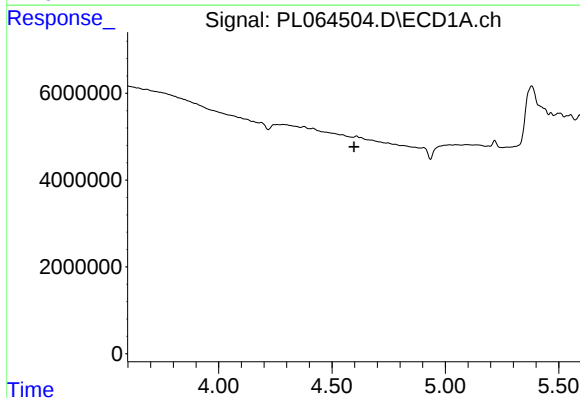


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

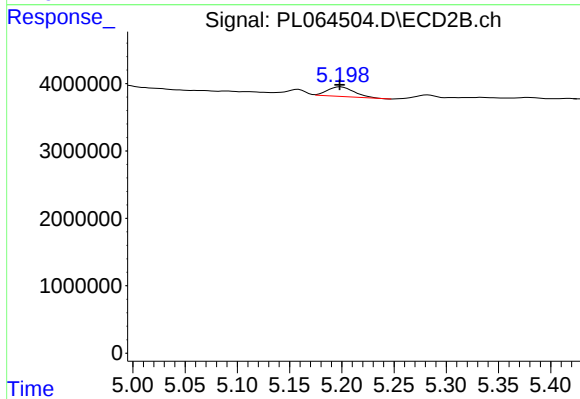

#7 delta-BHC


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 2517526
Conc: 0.82 ng/ml

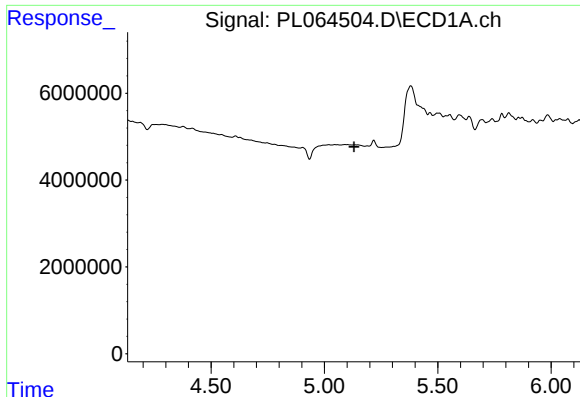

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.131 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

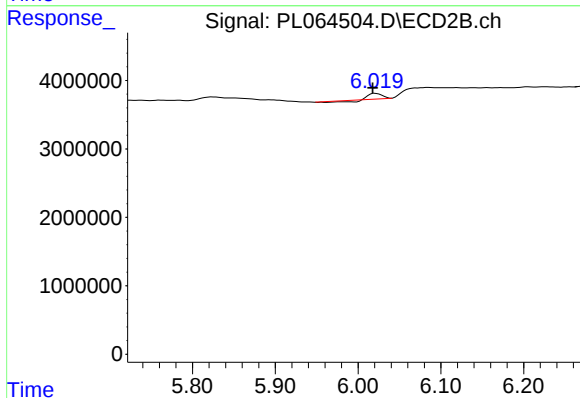


#8 Heptachlor epoxide

R.T.: 6.021 min
Delta R.T.: 0.003 min
Response: 530344
Conc: 0.21 ng/ml

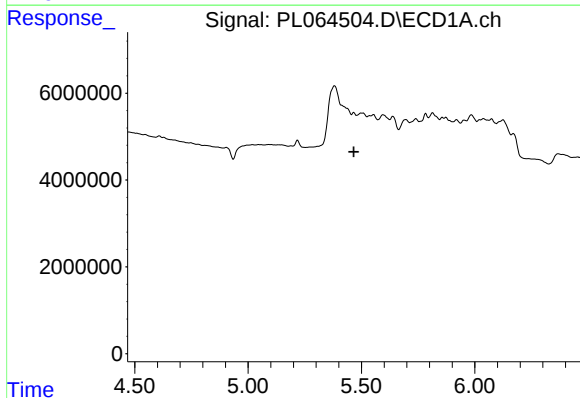


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.467 min
Response: 0
Conc: N.D.

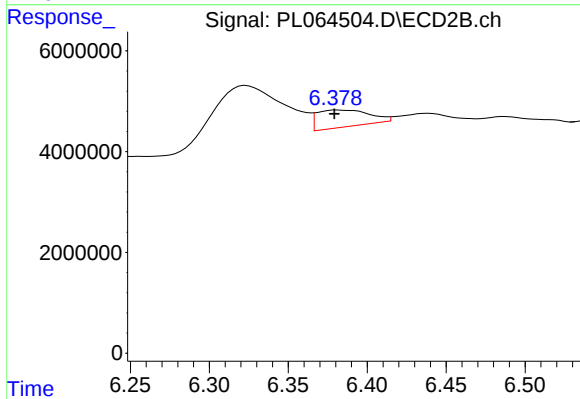

#9 Endosulfan I


R.T.: 6.381 min
Delta R.T.: 0.002 min
Response: 7822694
Conc: 2.94 ng/ml

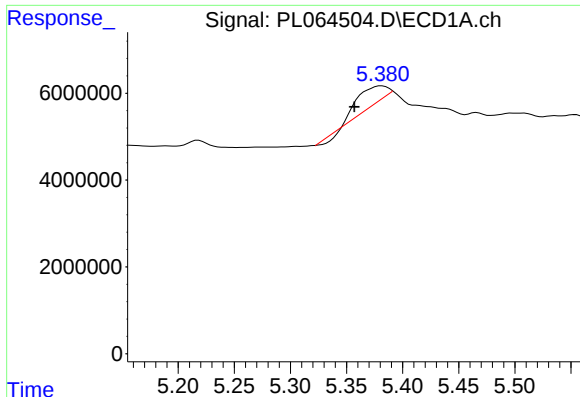

#10 gamma-Chlordane


R.T.: 5.381 min
Delta R.T.: 0.024 min
Response: 8064089
Conc: 1.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

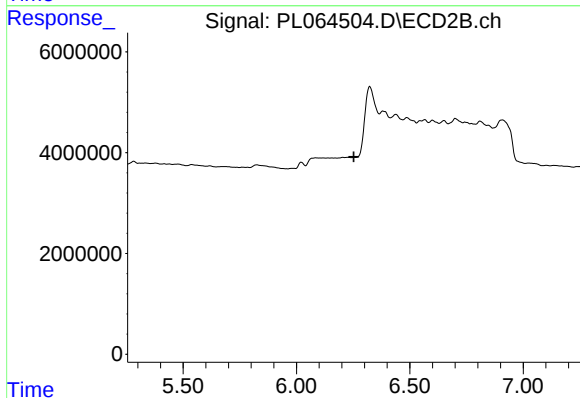


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.253 min
Response: 0
Conc: N.D.

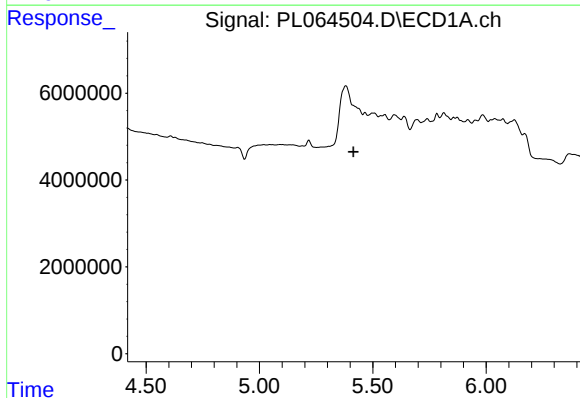


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.415 min
Response: 0
Conc: N.D.

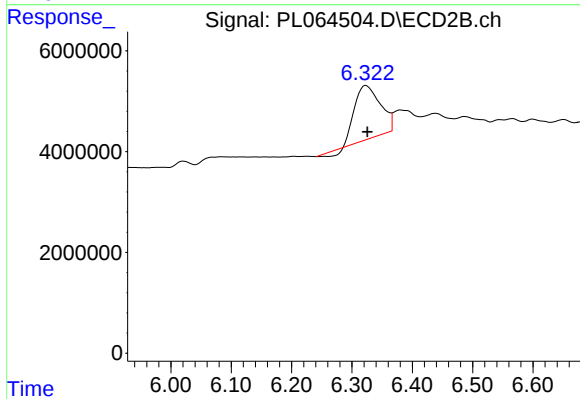

#11 alpha-Chlordane


R.T.: 6.323 min
Delta R.T.: -0.002 min
Response: 29994621
Conc: 10.19 ng/ml

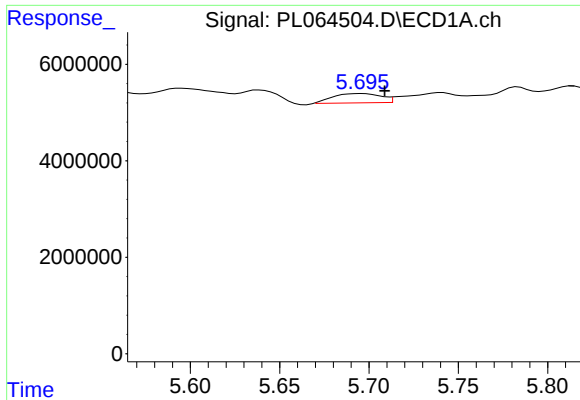

#13 Dieldrin


R.T.: 5.697 min
Delta R.T.: -0.012 min
Response: 3556674
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

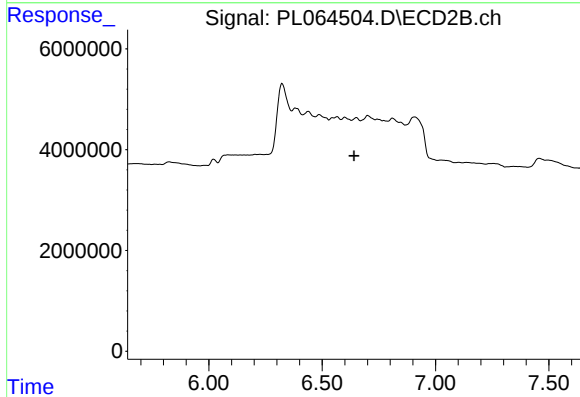


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.640 min
Response: 0
Conc: N.D.

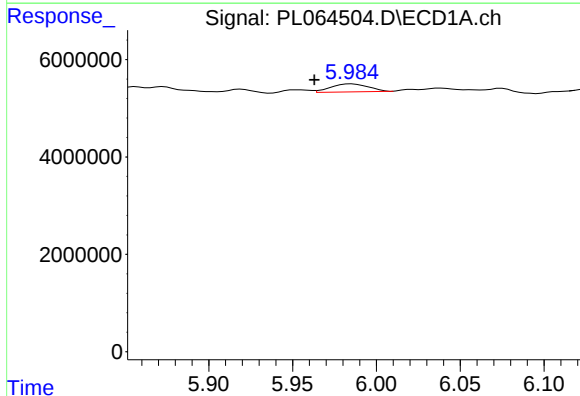


#14 Endrin

R.T.: 5.985 min
Delta R.T.: 0.022 min
Response: 2550536
Conc: 0.70 ng/ml

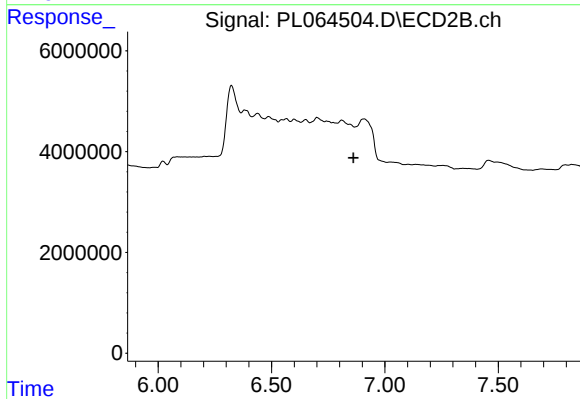

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

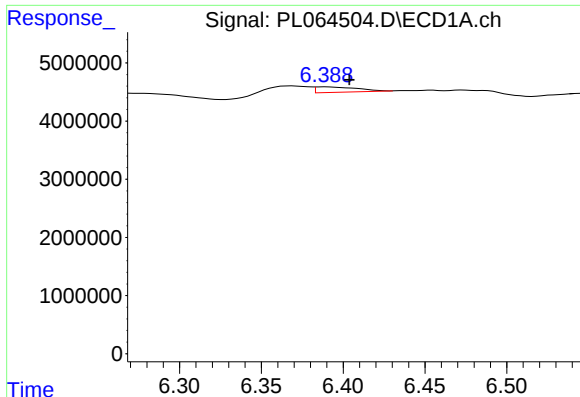

#18 Endrin aldehyde


R.T.: 6.389 min
Delta R.T.: -0.014 min
Response: 1627878
Conc: 0.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

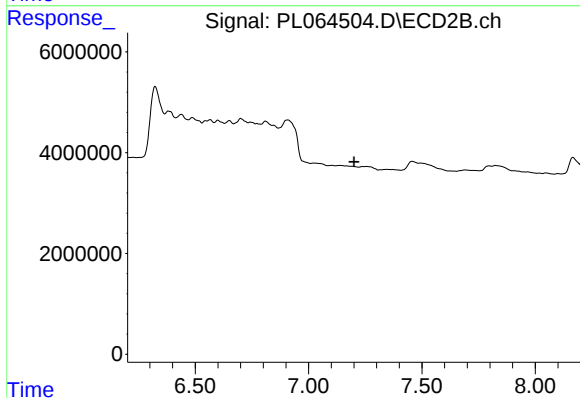


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

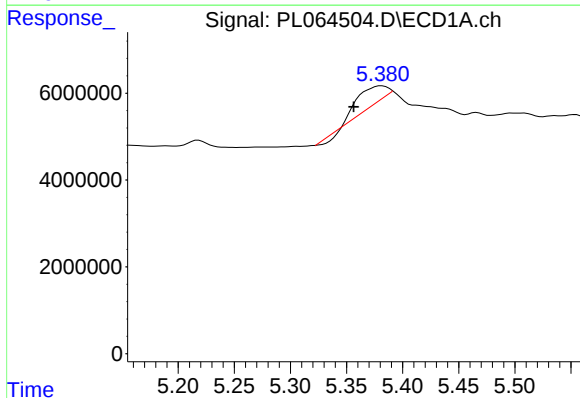


#25 Chlordane-3

R.T.: 5.381 min
Delta R.T.: 0.025 min
Response: 8064089
Conc: 22.36 ng/ml

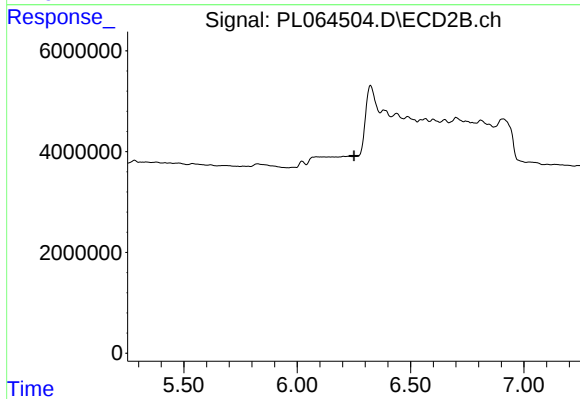

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.251 min
Response: 0
Conc: N.D.

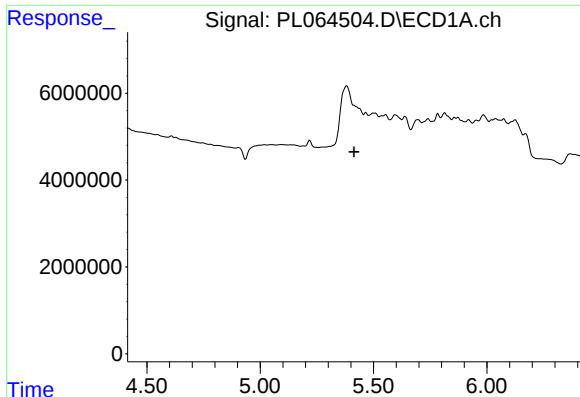

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

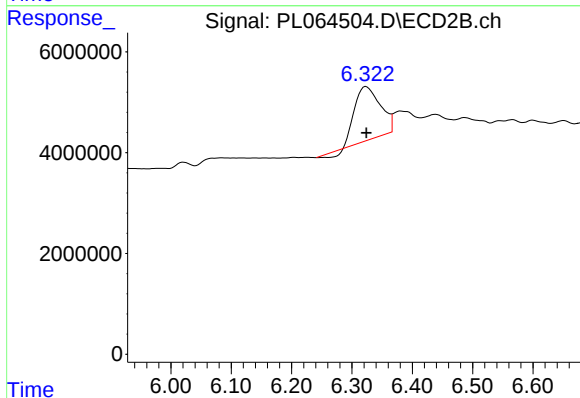


#26 Chlordane-4

R.T.: 6.323 min
Delta R.T.: 0.000 min
Response: 29994621
Conc: 68.21 ng/ml

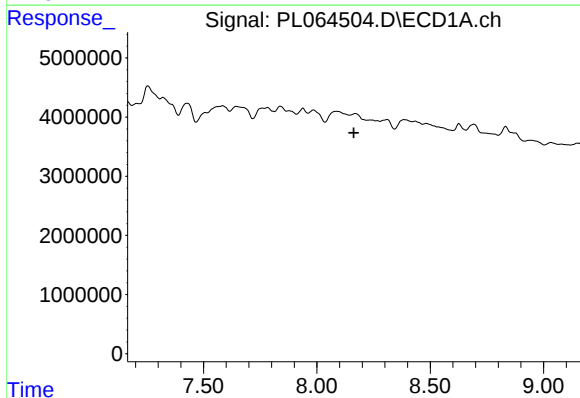

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.163 min
Response: 0
Conc: N.D.

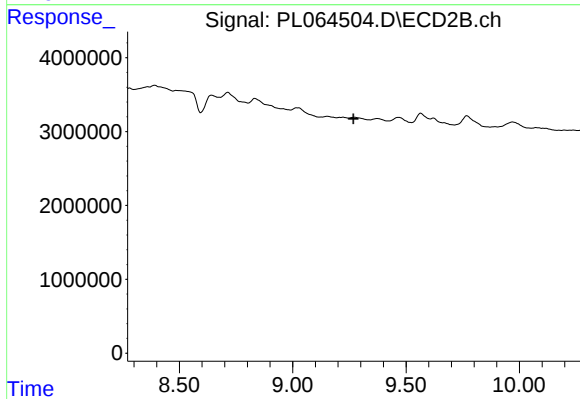

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.268 min
Response: 0
Conc: N.D.