

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 10:06
 Operator : AR\AJ
 Sample : M1242-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:19:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	4.108	29863316	23704183	9.810	9.951
28)	SA Decachlor...	8.172	9.273	34454704	22080400	10.933	10.785
Target Compounds							
23)	Chlordane-1	4.290	0.000	1118540	0	10.176	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 10:06
Operator : AR\AJ
Sample : M1242-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:19:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

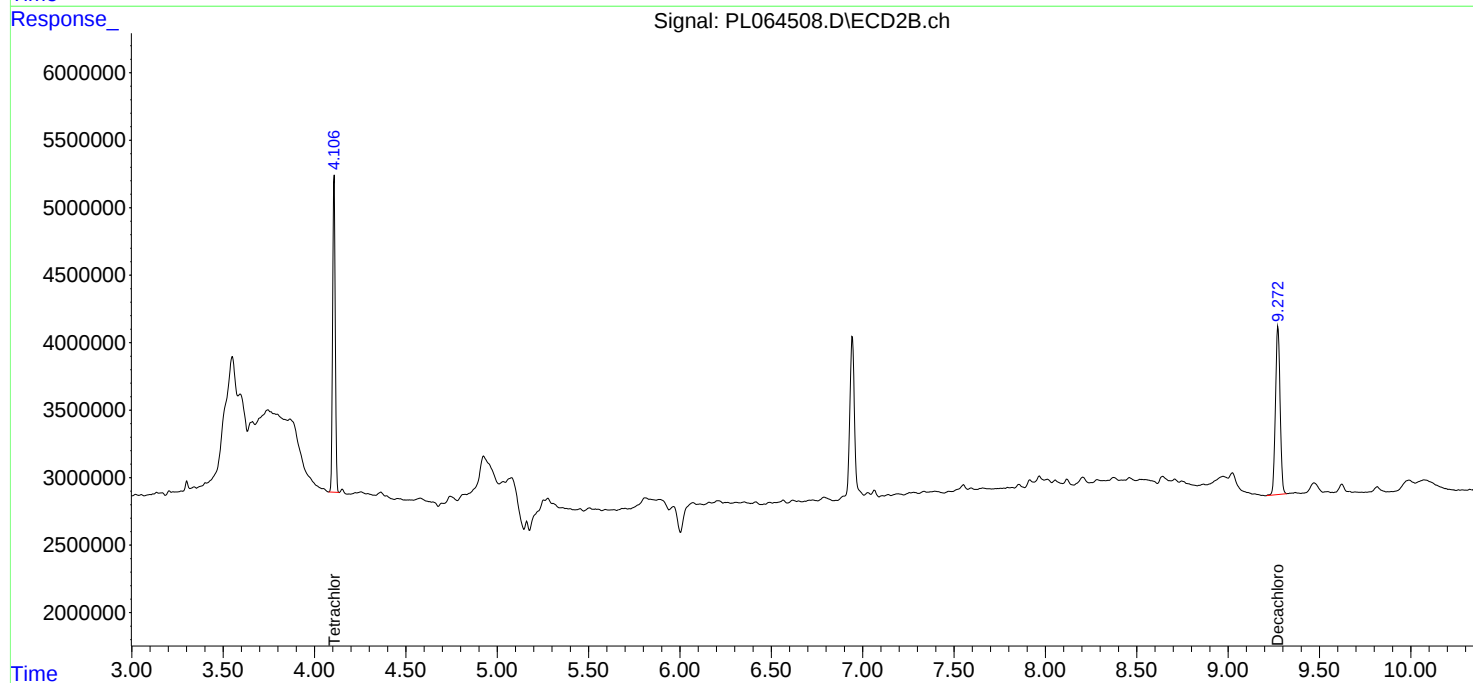


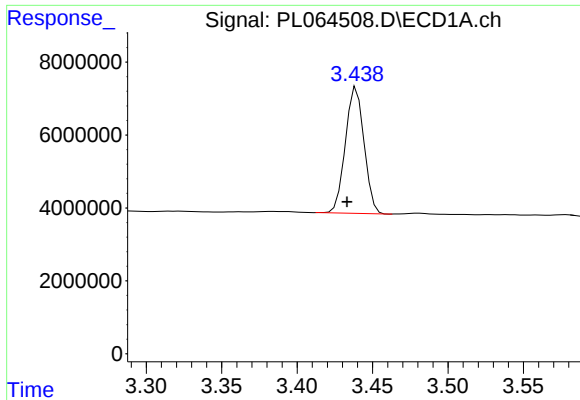

#1 Tetrachloro-m-xylene


R.T.: 3.440 min
Delta R.T.: 0.007 min
Response: 29863316
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

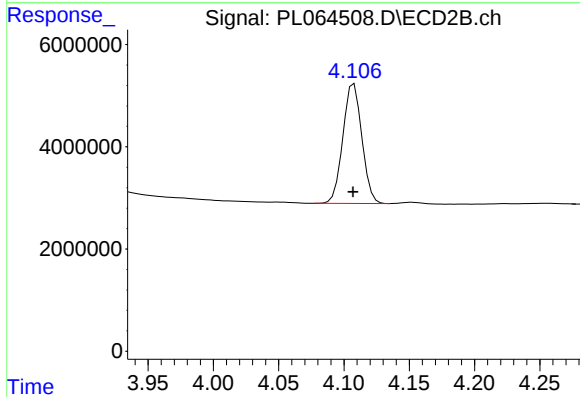


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 23704183
Conc: 9.95 ng/ml

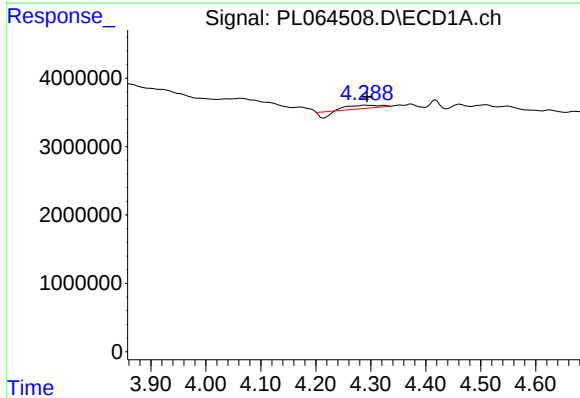


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: -0.003 min
Response: 1118540
Conc: 10.18 ng/ml

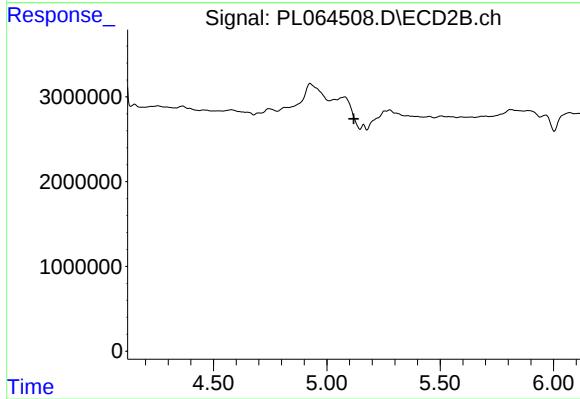

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

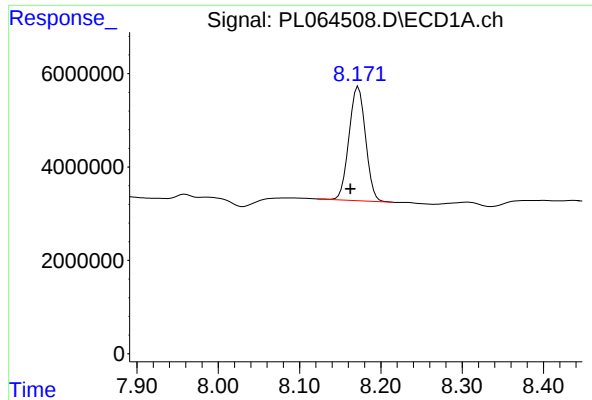

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.010 min
Response: 34454704
Conc: 10.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

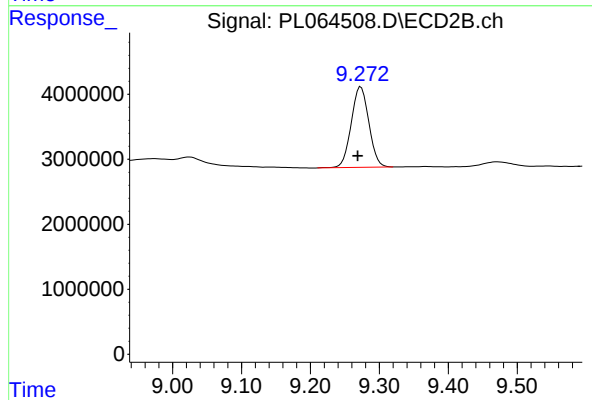

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.005 min
Response: 22080400
Conc: 10.78 ng/ml