

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 12:00
 Operator : AR\AJ
 Sample : PB134376BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:22:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	58693449	46562459	19.281	19.547
28)	SA Decachlor...	8.163	9.269	62293423	41087555	19.767	20.068
Target Compounds							
4)	MA Heptachlor	0.000	5.300	0	6417217	N.D.	1.841 #
6)	B beta-BHC	0.000	4.985	0	3160312	N.D.	1.868 #
10)	B gamma-Chl...	0.000	6.255	0	311287	N.D.	0.107 #
23)	Chlordane-1	4.319f	0.000	225800	0	2.054	N.D. #
25)	Chlordane-3	0.000	6.255	0	311287	N.D.	0.868 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 12:00
Operator : AR\AJ
Sample : PB134376BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:22:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

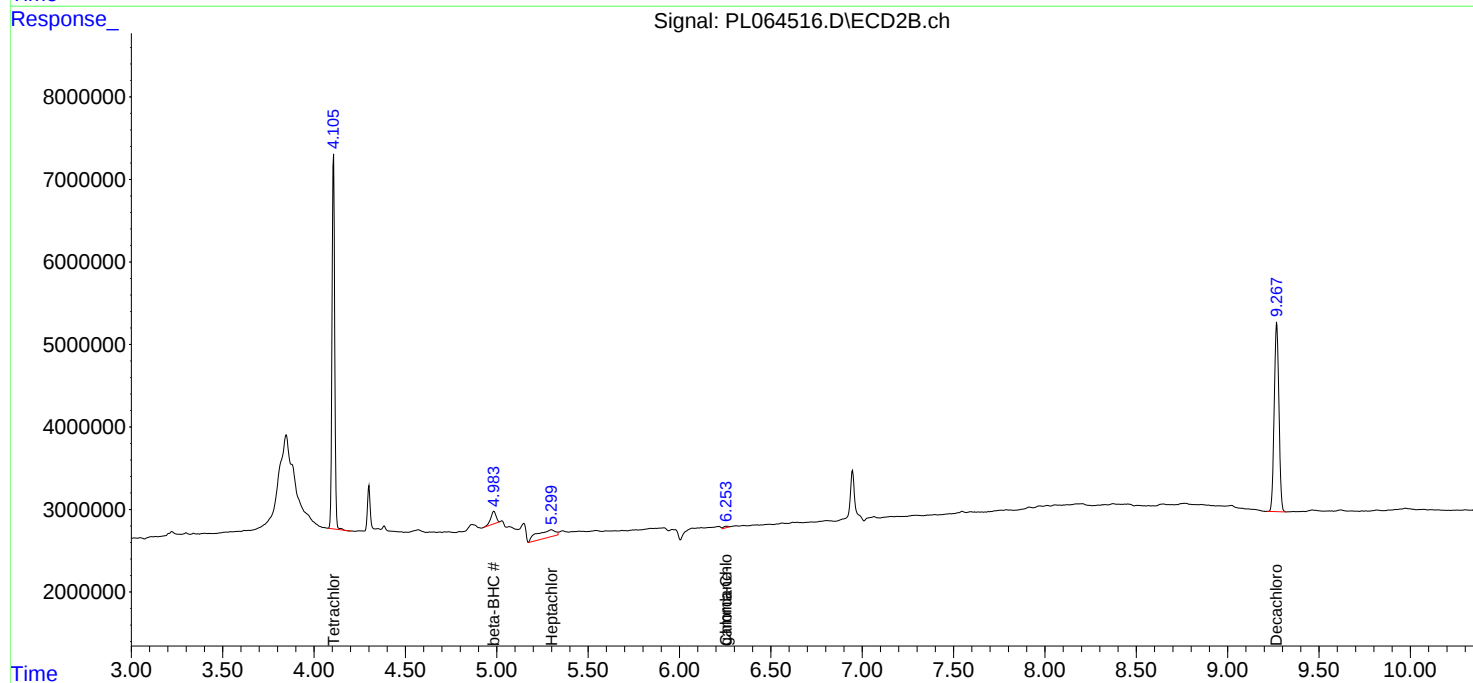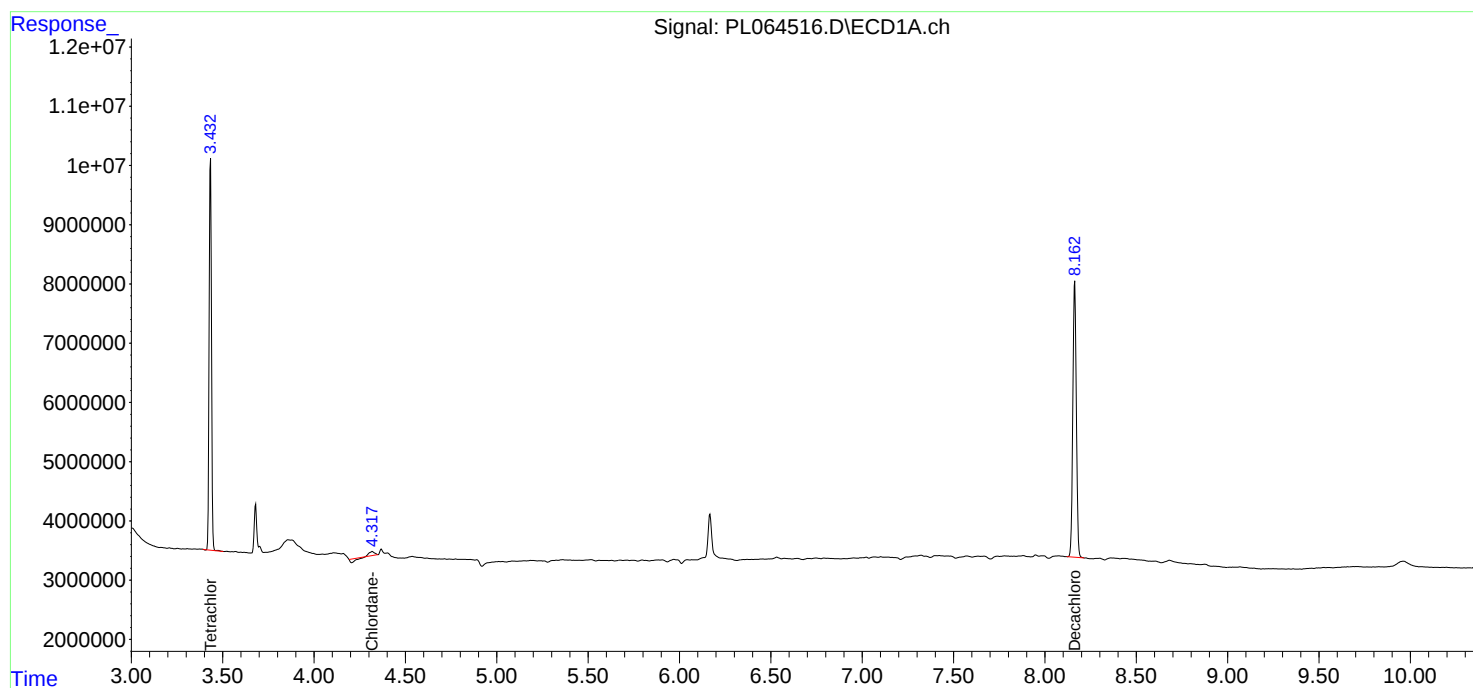


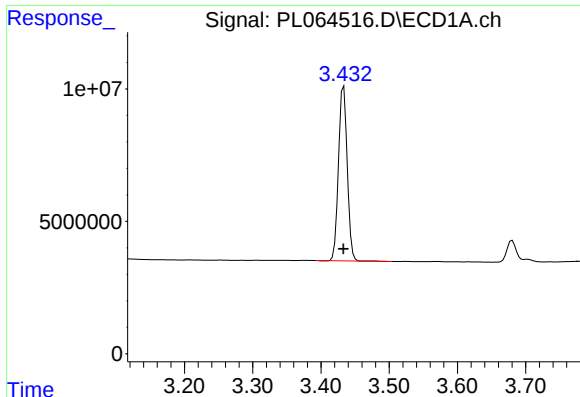

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 58693449
Conc: 19.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

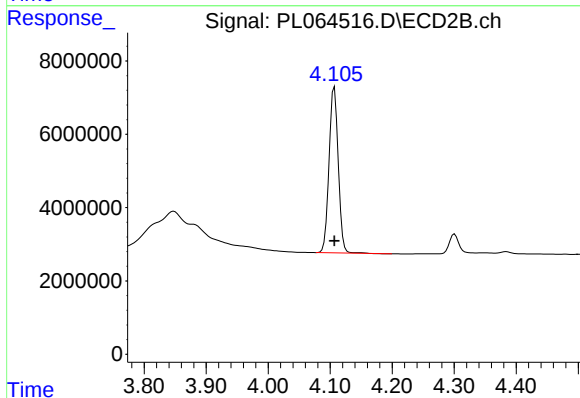


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 46562459
Conc: 19.55 ng/ml

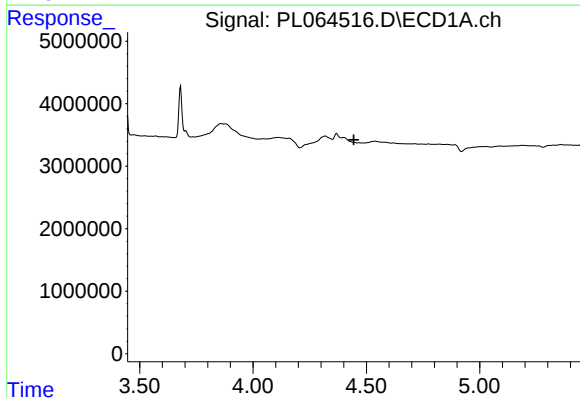


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

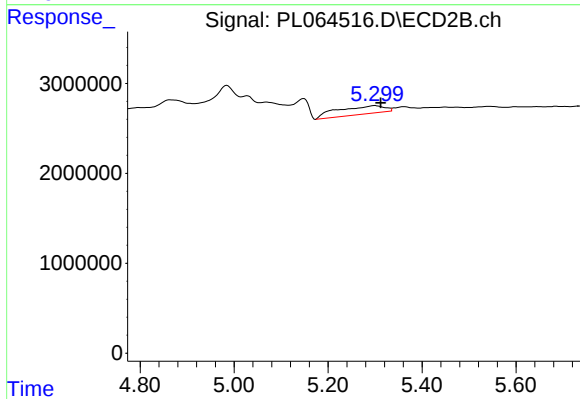

#4 Heptachlor


R.T.: 5.300 min
Delta R.T.: -0.012 min
Response: 6417217
Conc: 1.84 ng/ml

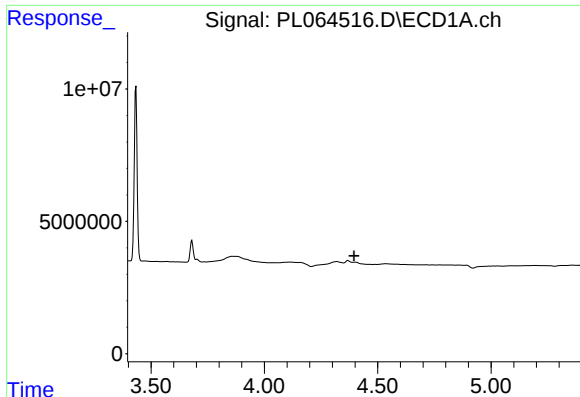

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

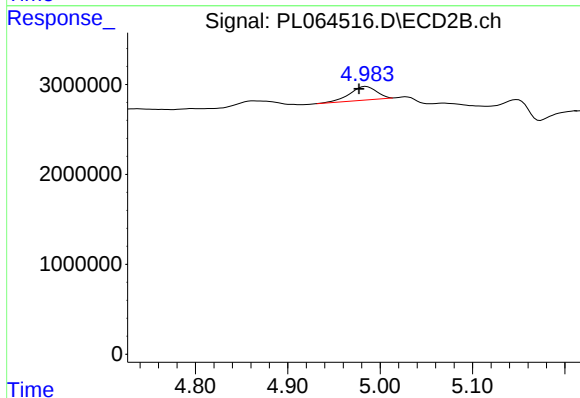


#6 beta-BHC

R.T.: 4.985 min
Delta R.T.: 0.008 min
Response: 3160312
Conc: 1.87 ng/ml

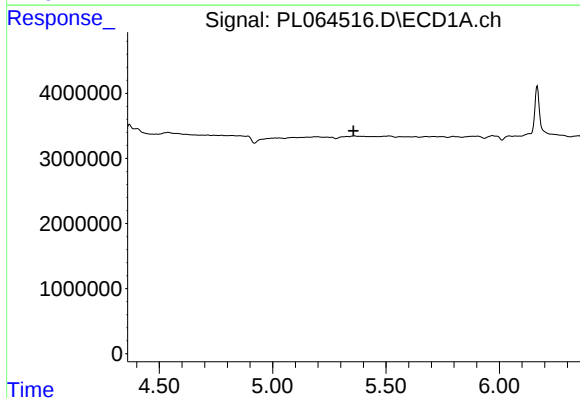


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

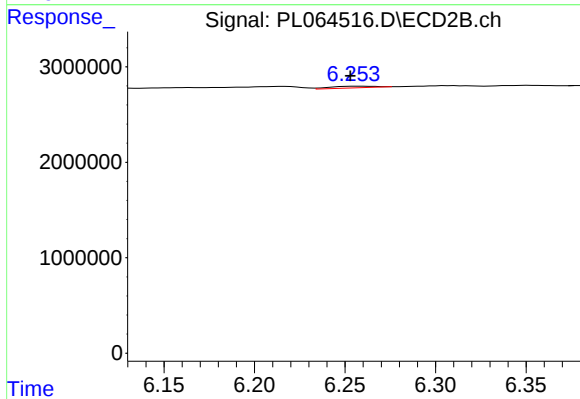

#10 gamma-Chlordane


R.T.: 6.255 min
Delta R.T.: 0.002 min
Response: 311287
Conc: 0.11 ng/ml

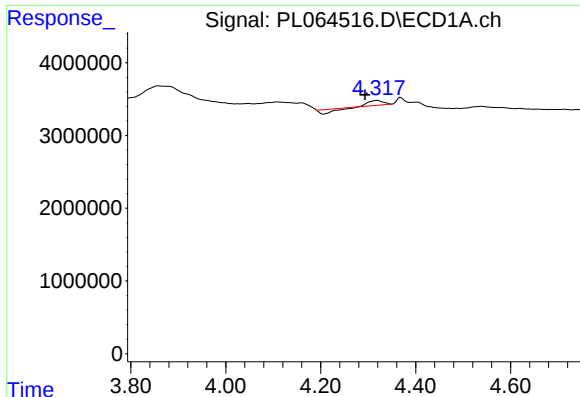

#23 Chlordane-1


R.T.: 4.319 min
Delta R.T.: 0.026 min
Response: 225800
Conc: 2.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

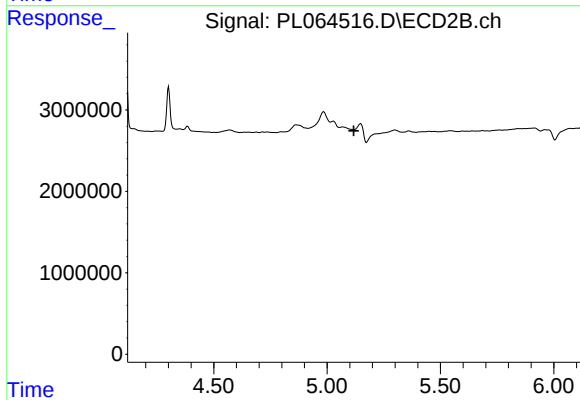


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

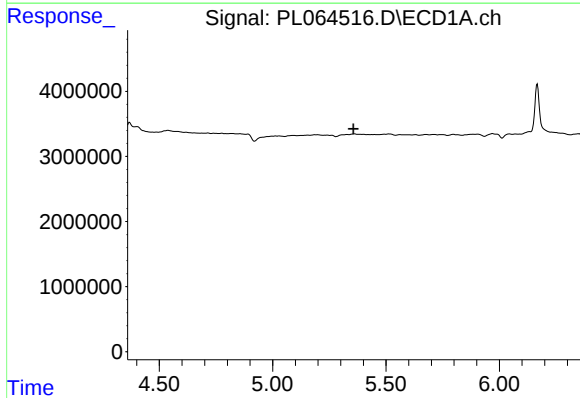


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

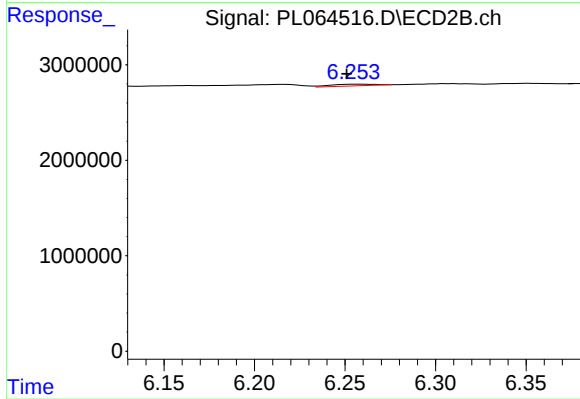

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: 0.004 min
Response: 311287
Conc: 0.87 ng/ml

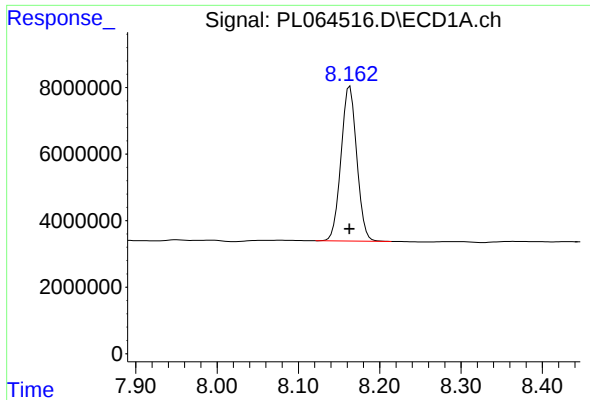

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 62293423
Conc: 19.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

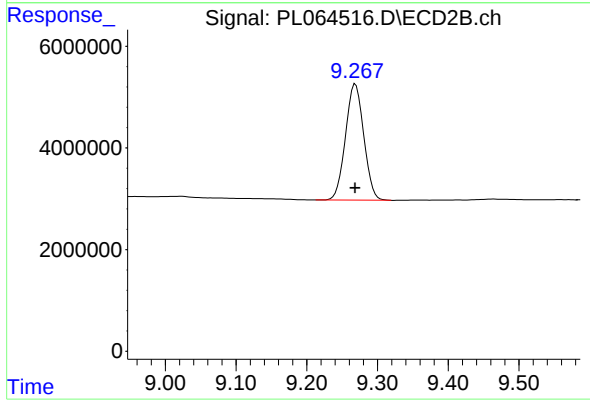

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 41087555
Conc: 20.07 ng/ml