

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 13:34
 Operator : AR\AJ
 Sample : M1251-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:23:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	35302074	26655518	11.597	11.190
28)	SA Decachlor...	8.164	9.269	35264834	18899473	11.190	9.231
Target Compounds							
2)	A alpha-BHC	0.000	4.531f	0	8841685	N.D.	2.557 #
4)	MA Heptachlor	0.000	5.307	0	8115572	N.D.	2.329 #
5)	MB Aldrin	4.666f	0.000	7220301	0	1.699	N.D. #
6)	B beta-BHC	0.000	4.986	0	4815020	N.D.	2.845 #
12)	B 4,4'-DDE	5.582	6.482	8211067	5650163	2.178	2.182
16)	A 4,4'-DDD	0.000	6.980	0	2015961	N.D.	0.876 #
17)	MA 4,4'-DDT	6.333	7.281	4575837	2140552	1.491	1.042 #
20)	A Methoxychlor	6.865f	0.000	5225649	0	2.893	N.D. #
23)	Chlordane-1	4.312f	0.000	1646910	0	14.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 13:34
Operator : AR\AJ
Sample : M1251-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:23:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

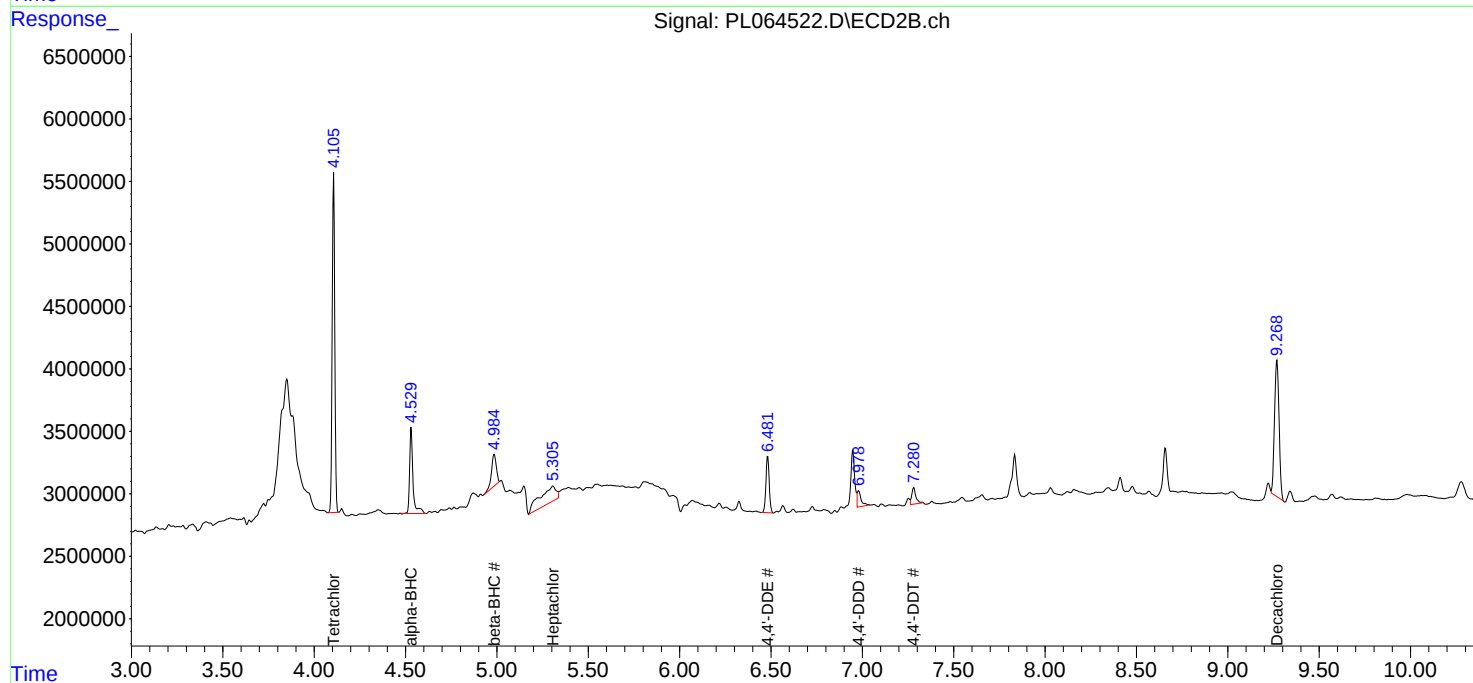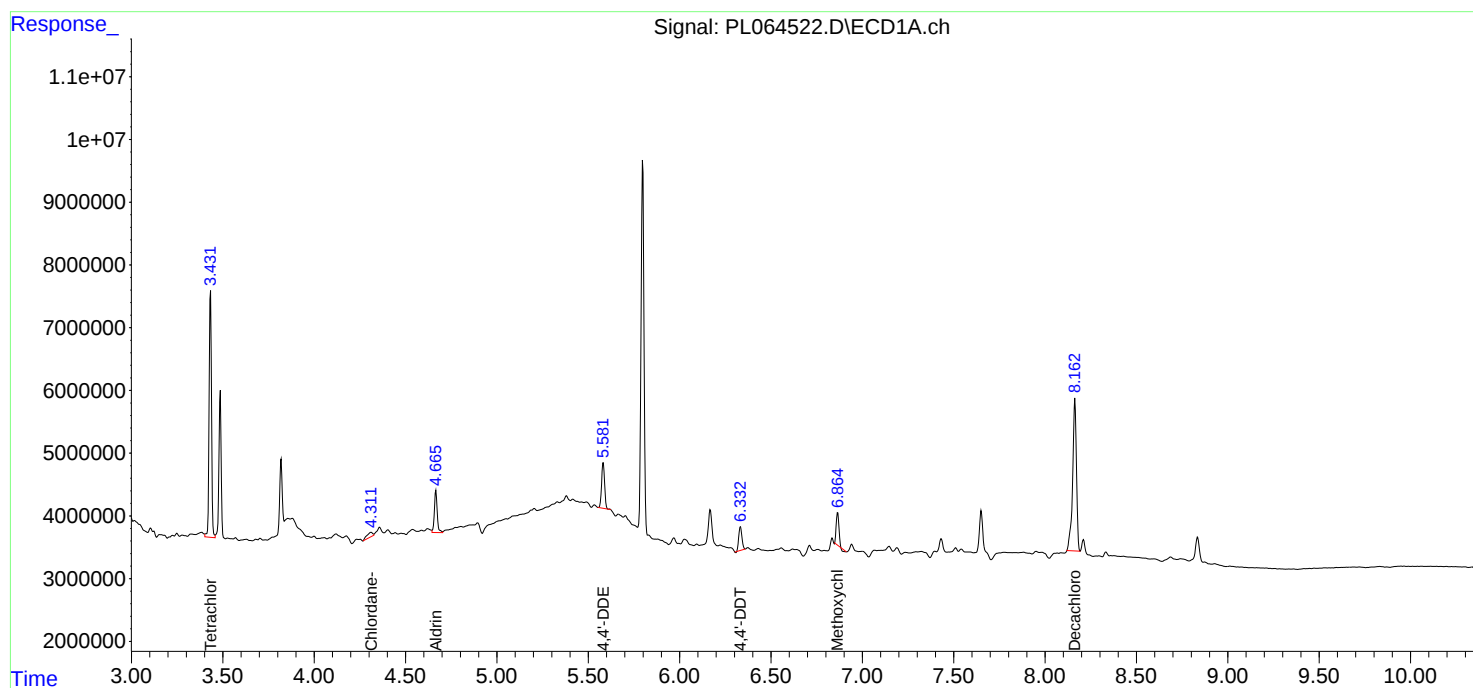


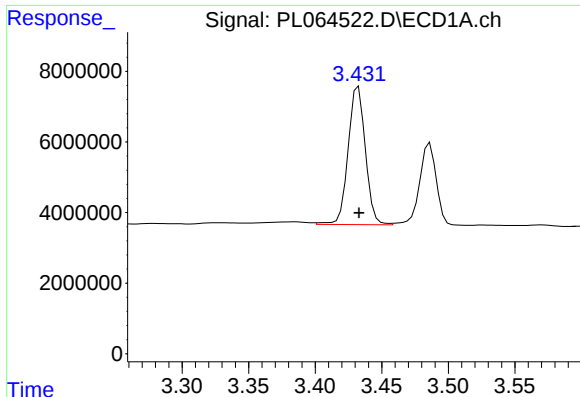

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 35302074
Conc: 11.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

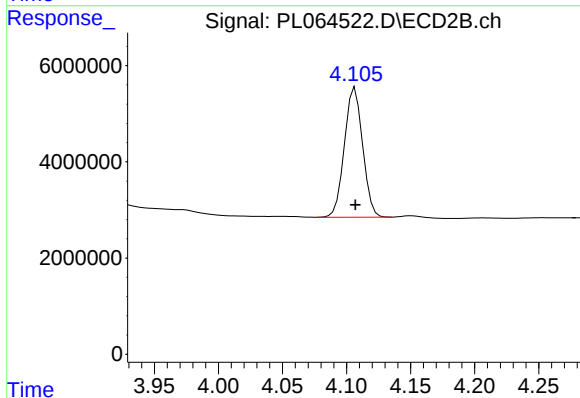


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 26655518
Conc: 11.19 ng/ml

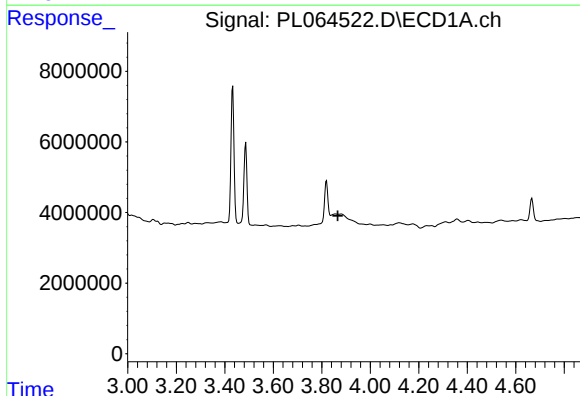


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.866 min
Response: 0
Conc: N.D.

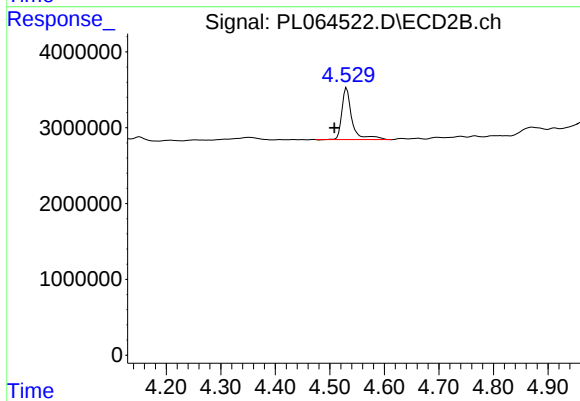

#2 alpha-BHC


R.T.: 4.531 min
Delta R.T.: 0.023 min
Response: 8841685
Conc: 2.56 ng/ml

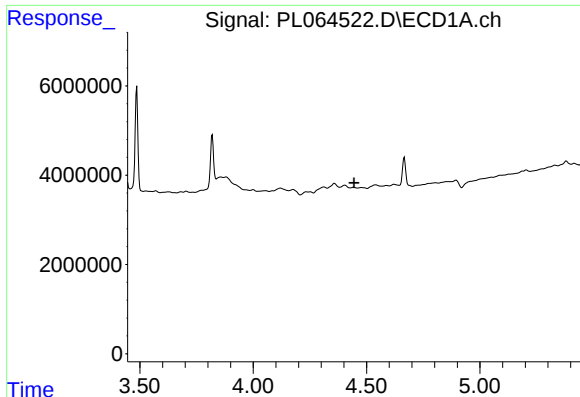

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

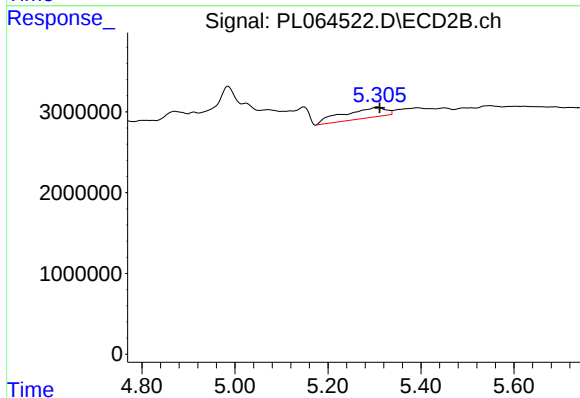


#4 Heptachlor

R.T.: 5.307 min
Delta R.T.: -0.005 min
Response: 8115572
Conc: 2.33 ng/ml

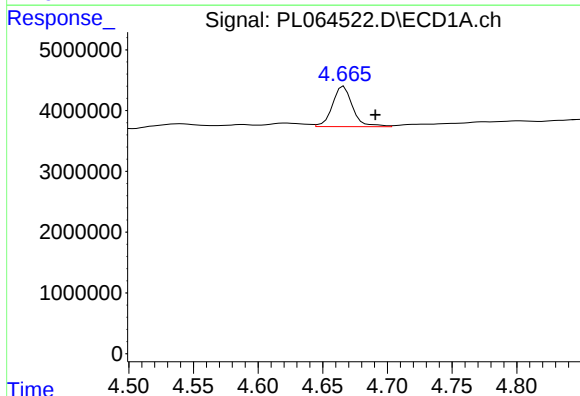


#5 Aldrin

R.T.: 4.666 min
Delta R.T.: -0.025 min
Response: 7220301
Conc: 1.70 ng/ml

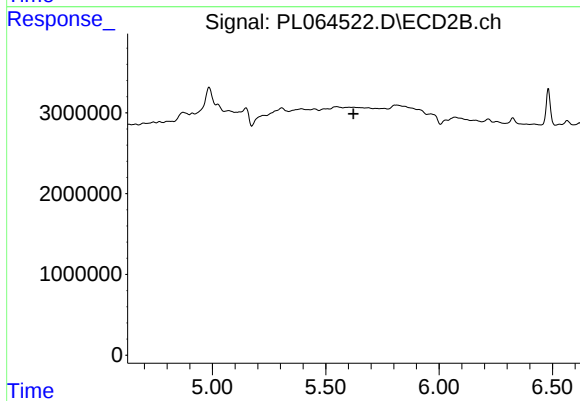

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

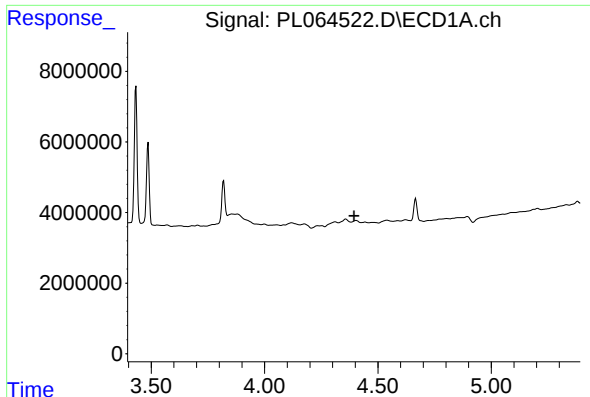

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

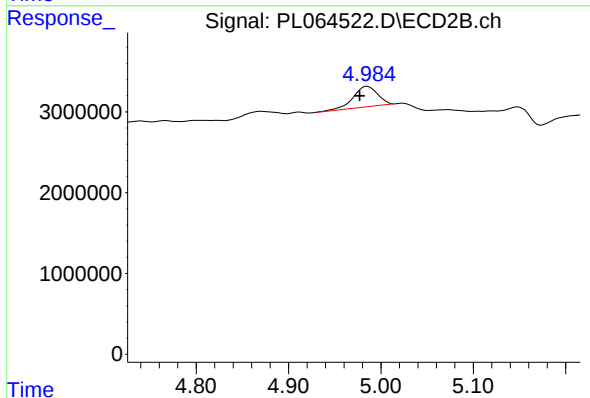


#6 beta-BHC

R.T.: 4.986 min
Delta R.T.: 0.008 min
Response: 4815020
Conc: 2.85 ng/ml

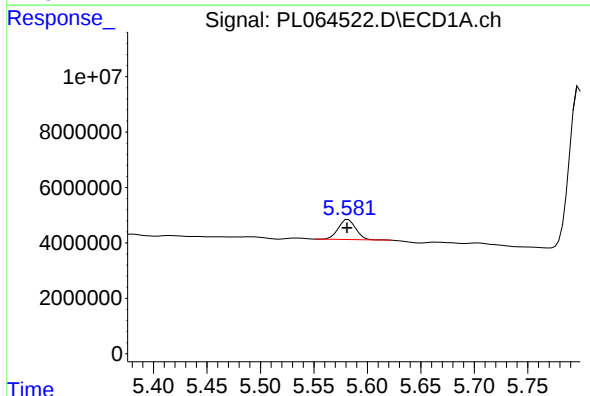


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 8211067
Conc: 2.18 ng/ml

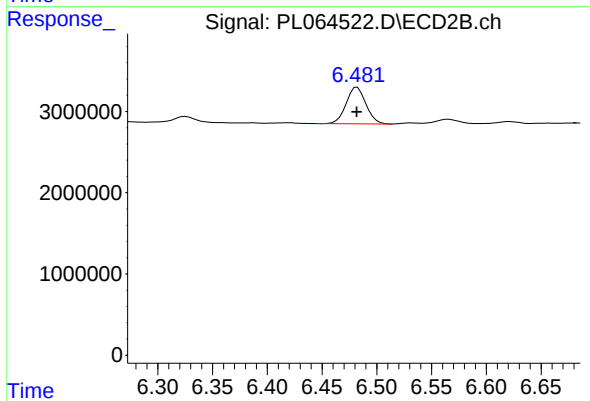

#12 4,4'-DDE


R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 5650163
Conc: 2.18 ng/ml

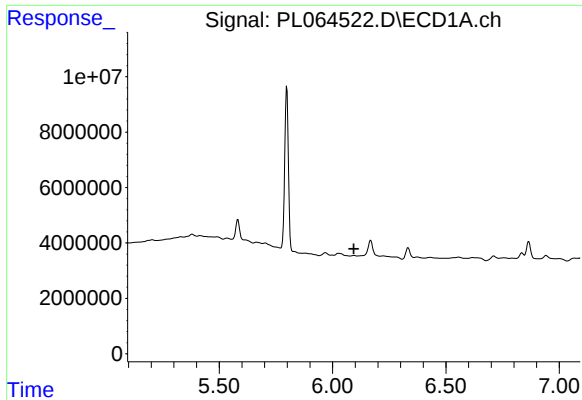

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

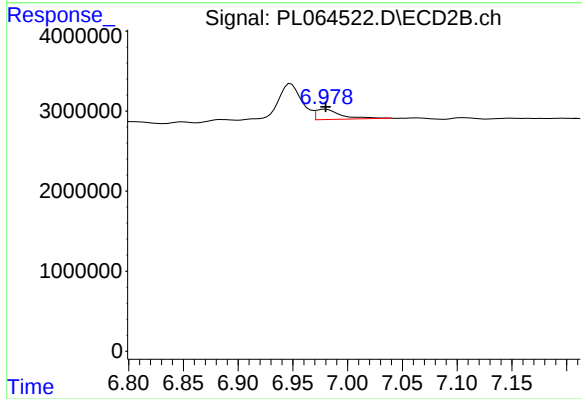


#16 4,4'-DDD

R.T.: 6.980 min
Delta R.T.: 0.000 min
Response: 2015961
Conc: 0.88 ng/ml

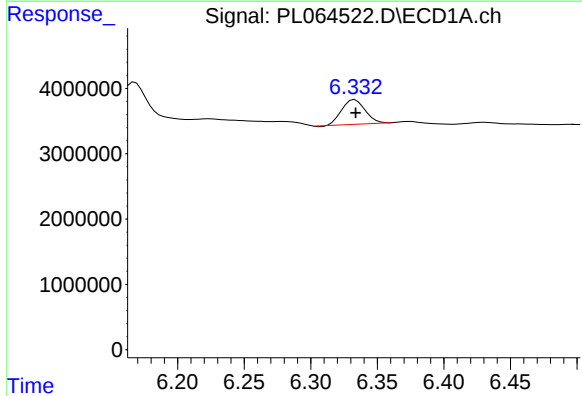


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 4575837
Conc: 1.49 ng/ml

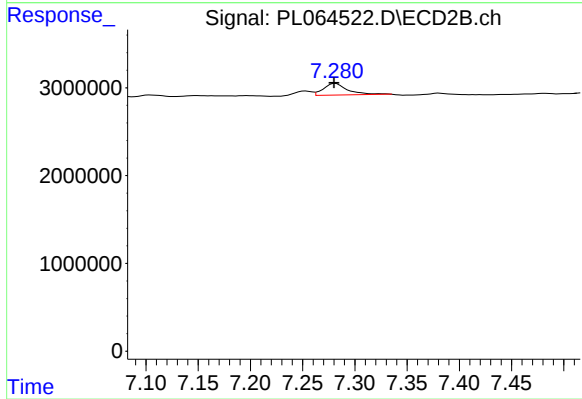

#17 4,4'-DDT


R.T.: 7.281 min
Delta R.T.: 0.001 min
Response: 2140552
Conc: 1.04 ng/ml

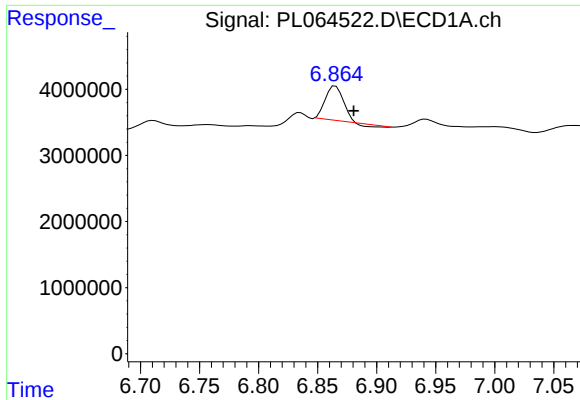

#20 Methoxychlor


R.T.: 6.865 min
Delta R.T.: -0.016 min
Response: 5225649
Conc: 2.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

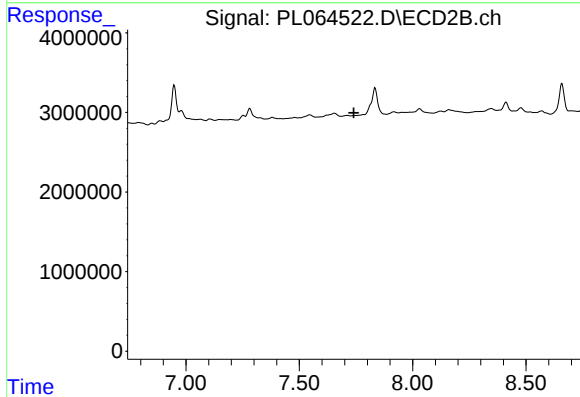


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

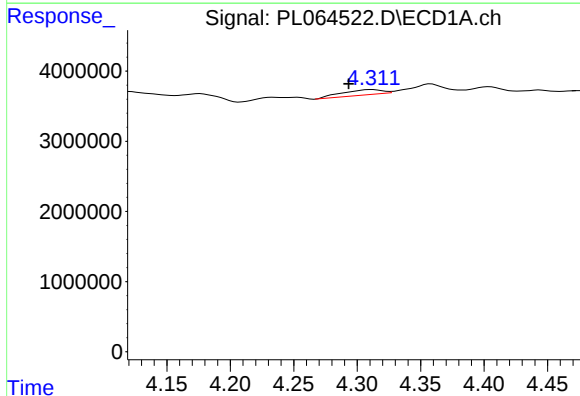


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.019 min
Response: 1646910
Conc: 14.98 ng/ml

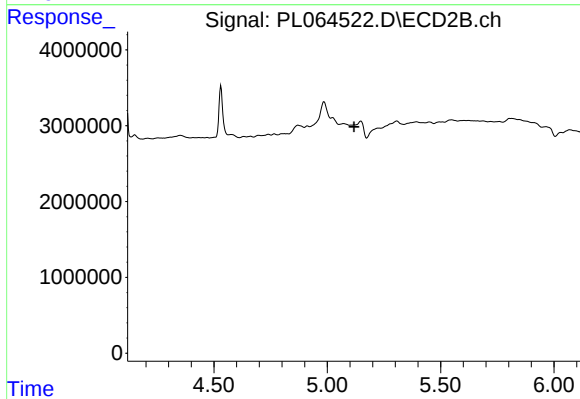

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

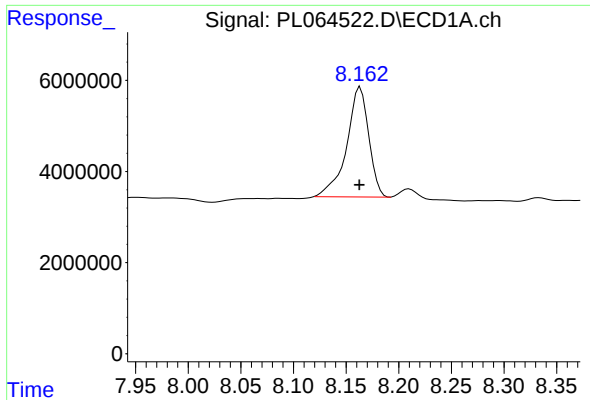

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.001 min
Response: 35264834
Conc: 11.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

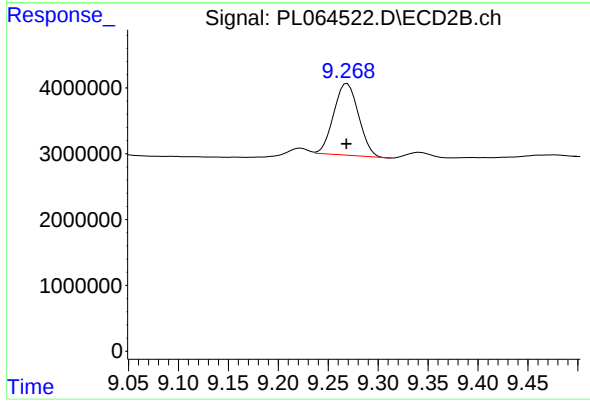

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 18899473
Conc: 9.23 ng/ml