

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 15:33
 Operator : AR\AJ
 Sample : PB134402BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:26:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.108	57080498	45186668	18.751	18.970
28)	SA Decachlor...	8.169	9.272	63206601	40989431	20.057	20.020
Target Compounds							
6)	B beta-BHC	0.000	4.957f	0	6649067	N.D.	3.929 #
15)	B Endosulfa...	0.000	7.066	0	1686007	N.D.	0.683 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 15:33
Operator : AR\AJ
Sample : PB134402BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:26:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

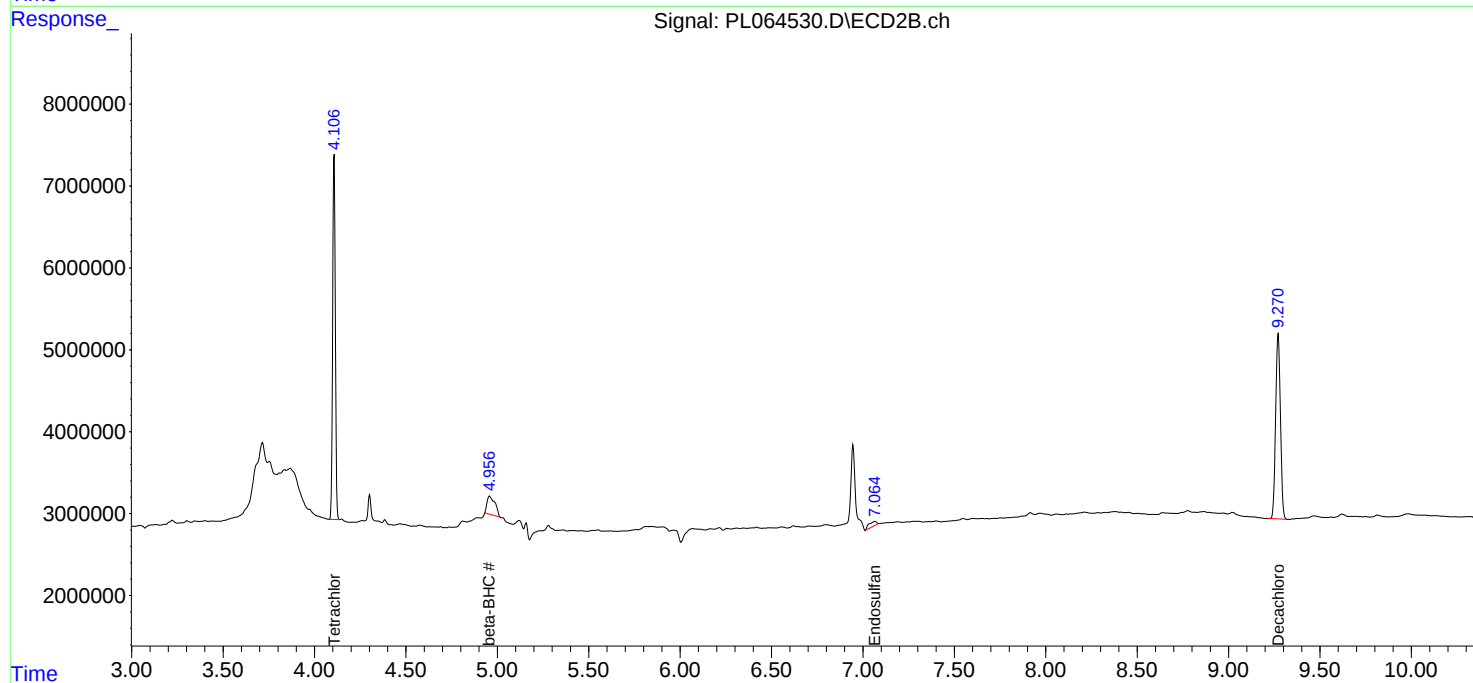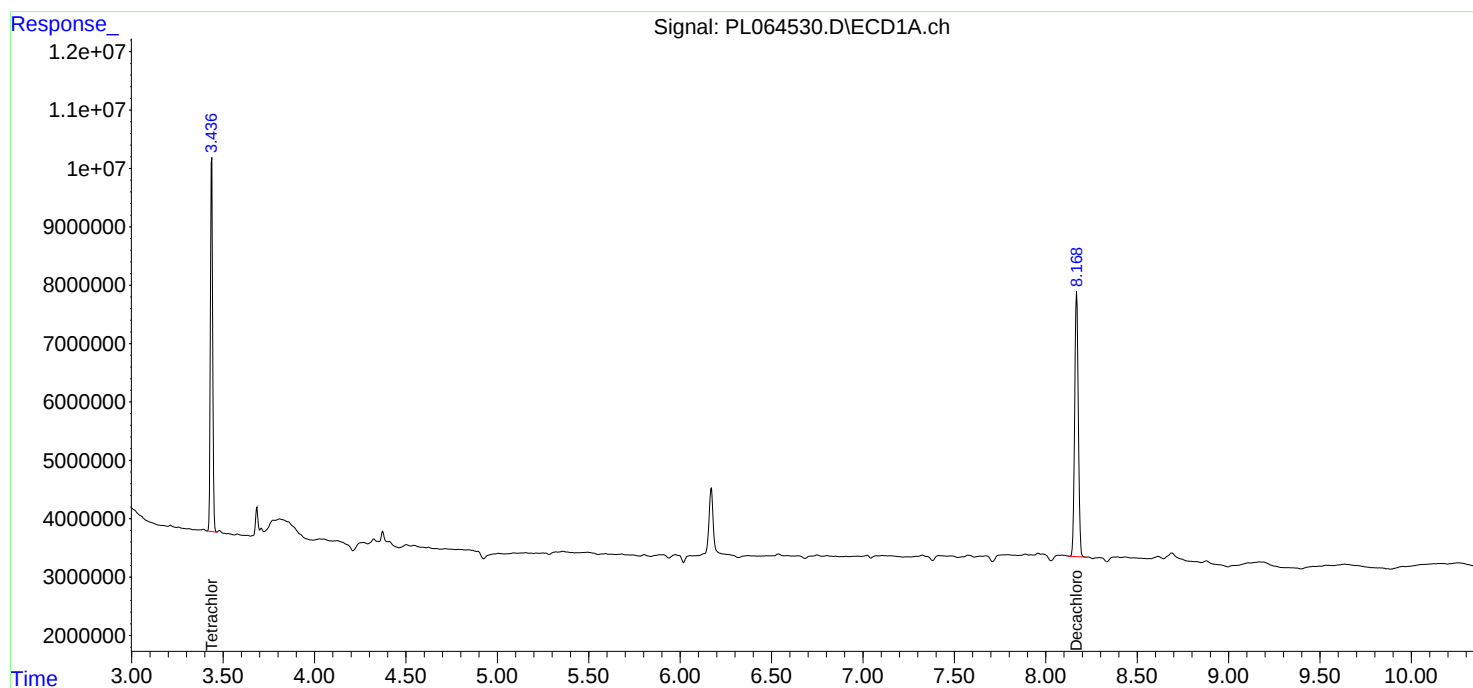


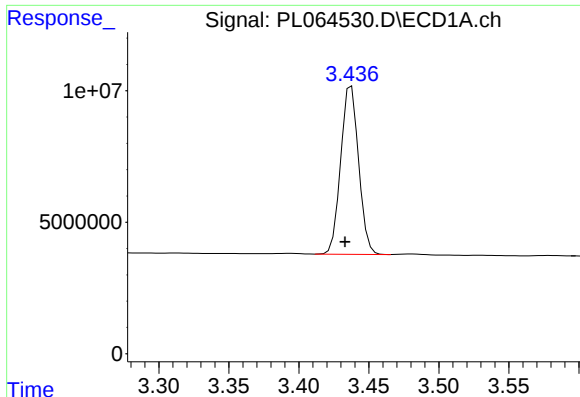

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.005 min
Response: 57080498
Conc: 18.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

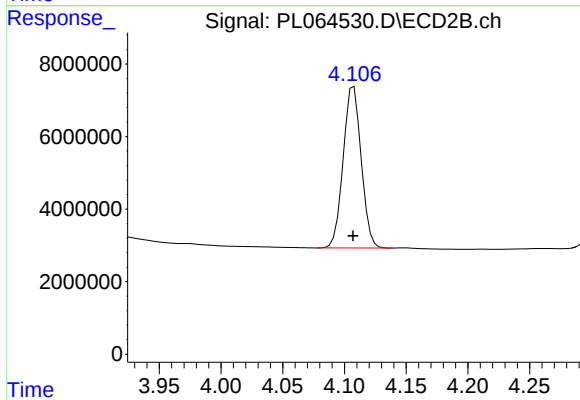


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 45186668
Conc: 18.97 ng/ml

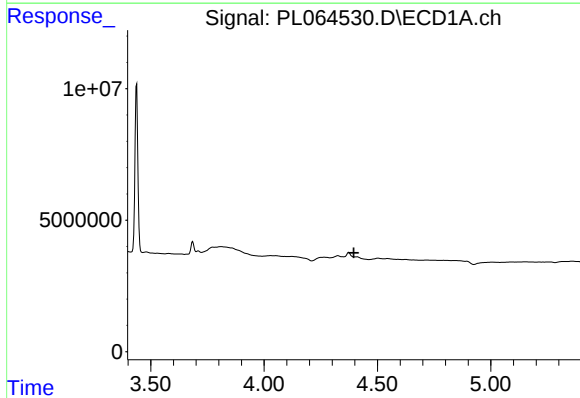


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.395 min
Response: 0
Conc: N.D.

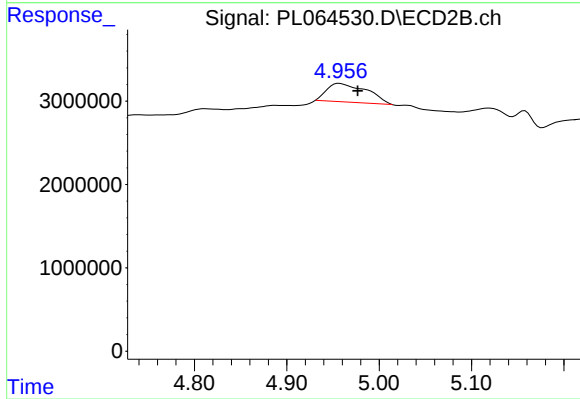

#6 beta-BHC


R.T.: 4.957 min
Delta R.T.: -0.020 min
Response: 6649067
Conc: 3.93 ng/ml

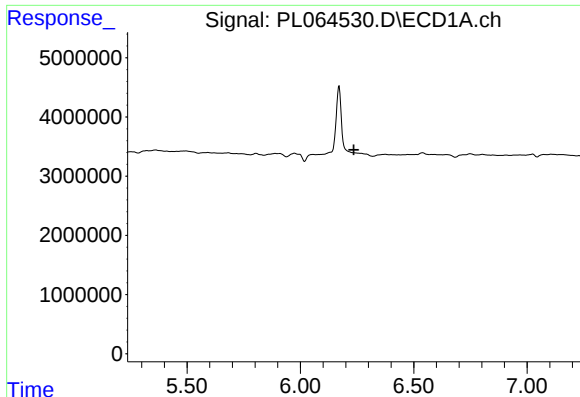

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

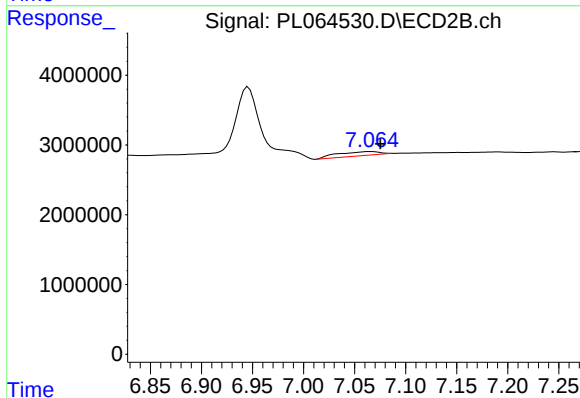


#15 Endosulfan II

R.T.: 7.066 min
Delta R.T.: -0.009 min
Response: 1686007
Conc: 0.68 ng/ml

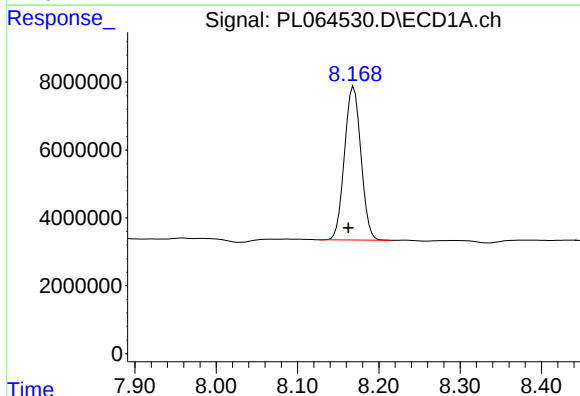

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.007 min
Response: 63206601
Conc: 20.06 ng/ml

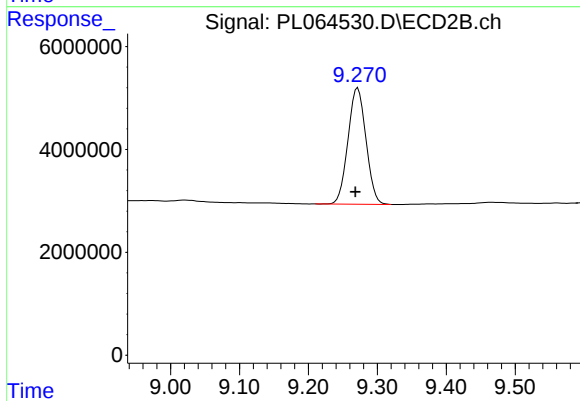

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.003 min
Response: 40989431
Conc: 20.02 ng/ml