

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 19:44
 Operator : AR\AJ
 Sample : M1271-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:31:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.106	40318908	30325030	13.245	12.731
28)	SA Decachlor...	8.161	9.266	41114252	28147827	13.046	13.748
Target Compounds							
6)	B beta-BHC	0.000	4.983	0	3203927	N.D.	1.893 #
10)	B gamma-Chl...	5.380f	6.253	1112478	2320484	0.269	0.798 #
11)	B alpha-Chl...	0.000	6.325	0	4132560	N.D.	1.404 #
14)	MA Endrin	5.967	0.000	3349553	0	0.916	N.D. #
17)	MA 4,4'-DDT	6.333	0.000	1522652	0	0.496	N.D. #
23)	Chlordane-1	4.319f	0.000	1554963	0	14.146	N.D. #
25)	Chlordane-3	5.380f	6.253	1112478	2320484	3.084	6.473 #
26)	Chlordane-4	0.000	6.325	0	4132560	N.D.	9.397 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 19:44
Operator : AR\AJ
Sample : M1271-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:31:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

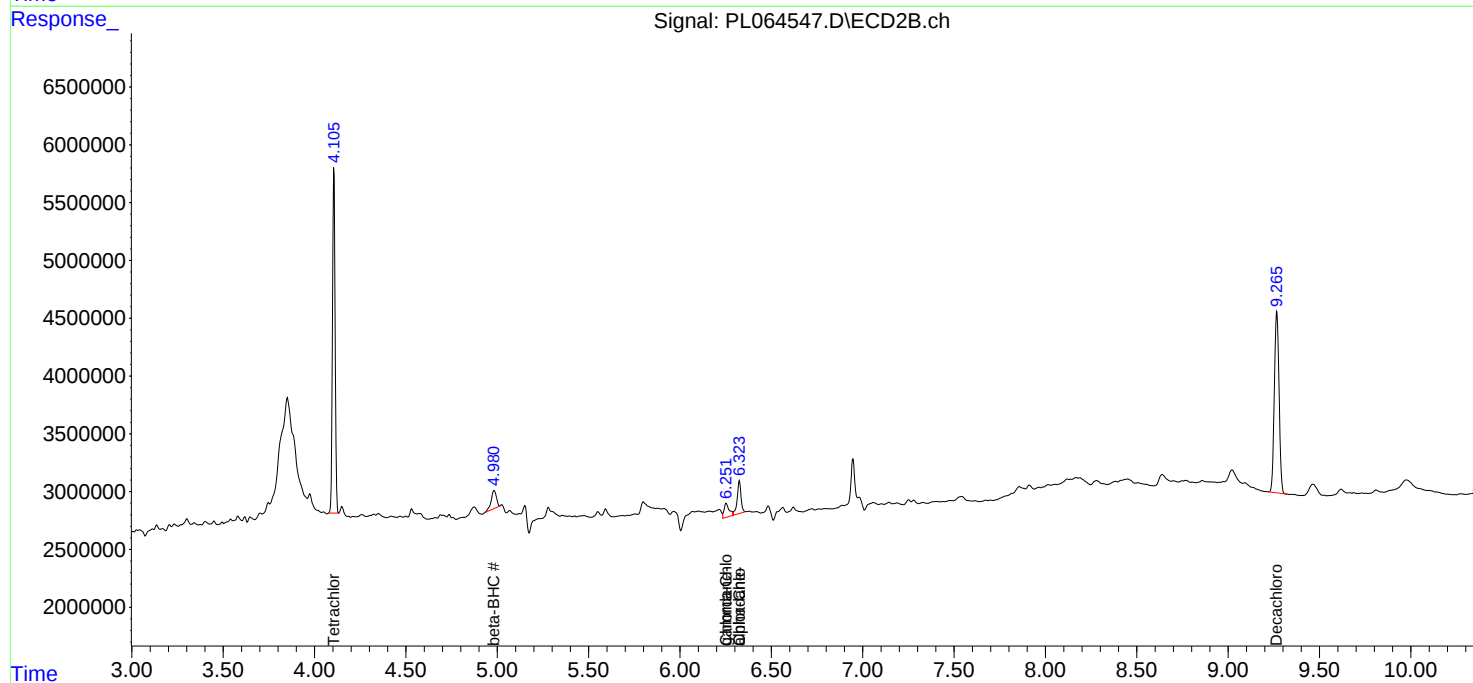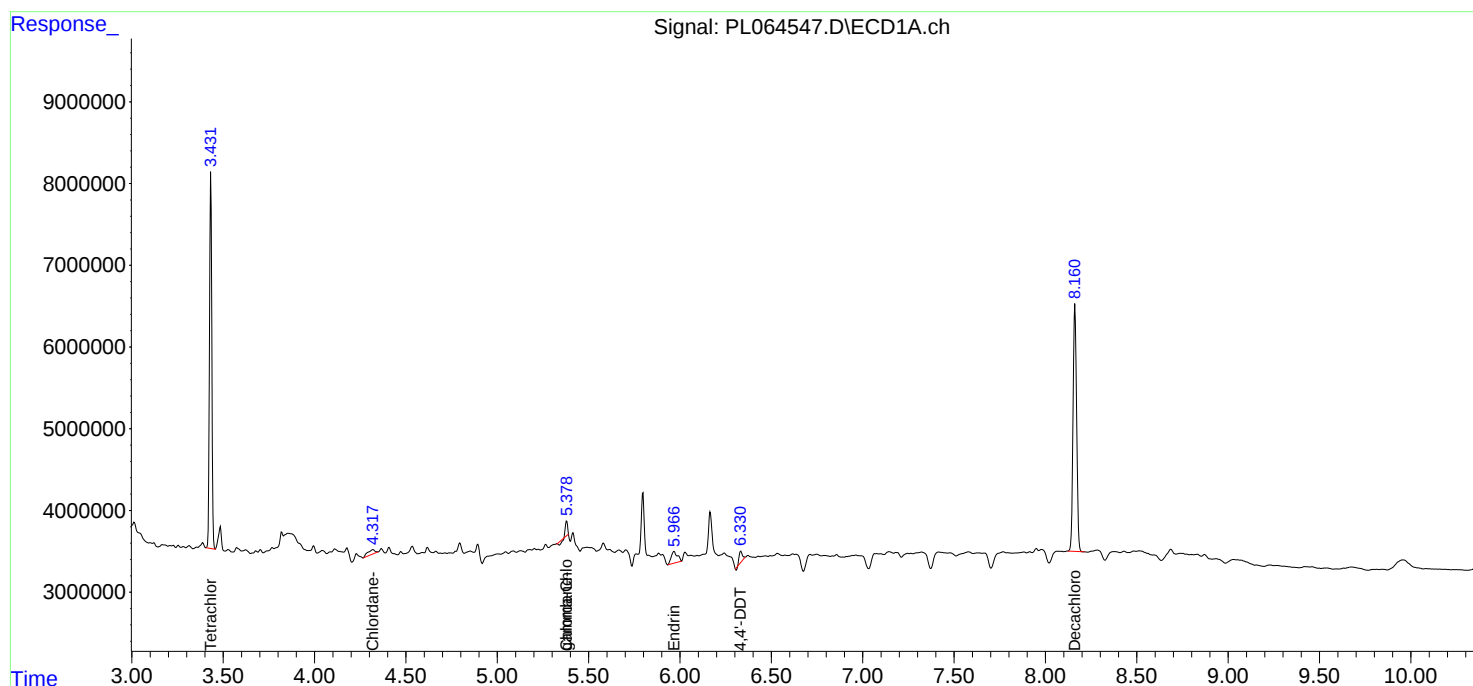


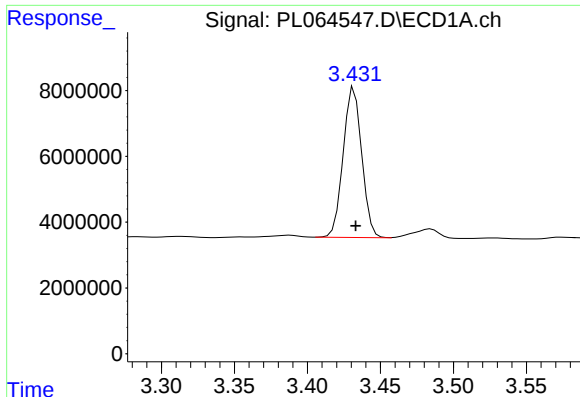

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 40318908
Conc: 13.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

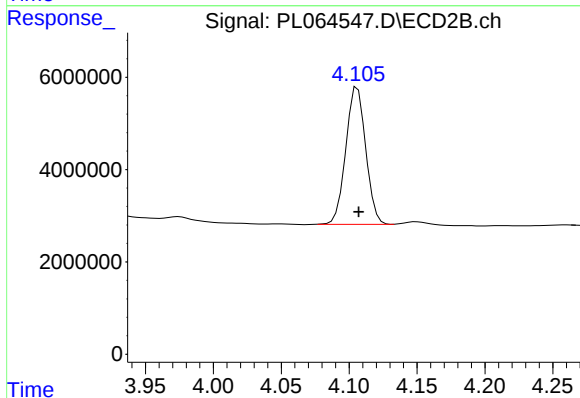


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.000 min
Response: 30325030
Conc: 12.73 ng/ml

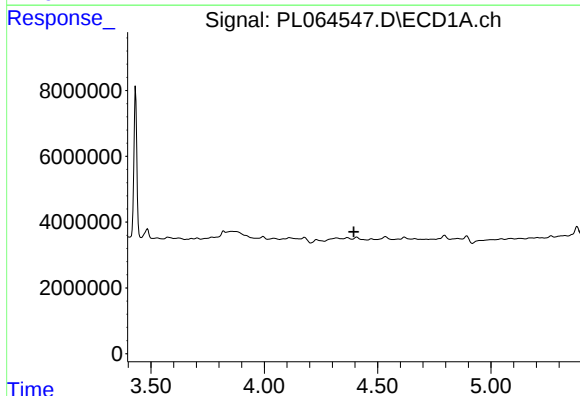


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.395 min
Response: 0
Conc: N.D.

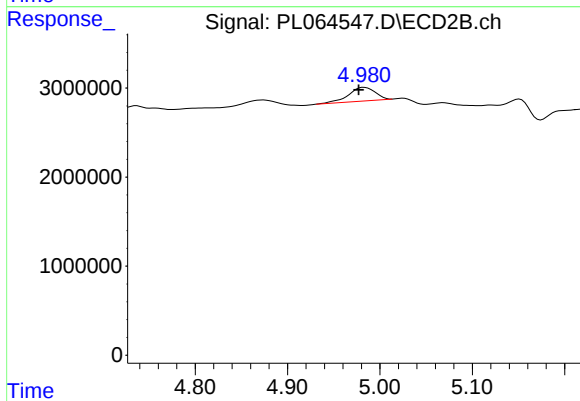

#6 beta-BHC


R.T.: 4.983 min
Delta R.T.: 0.006 min
Response: 3203927
Conc: 1.89 ng/ml

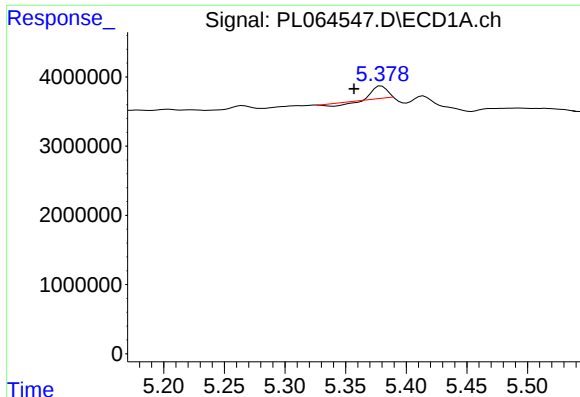

#10 gamma-Chlordane


R.T.: 5.380 min
Delta R.T.: 0.023 min
Response: 1112478
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

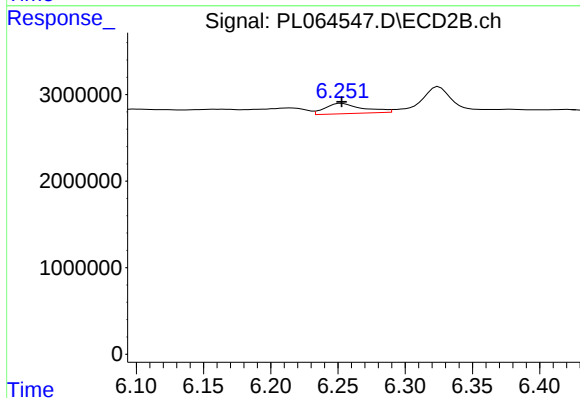


#10 gamma-Chlordane

R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 2320484
Conc: 0.80 ng/ml

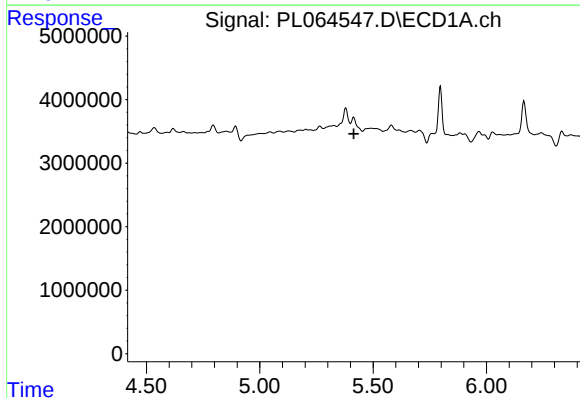


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.415 min
Response: 0
Conc: N.D.

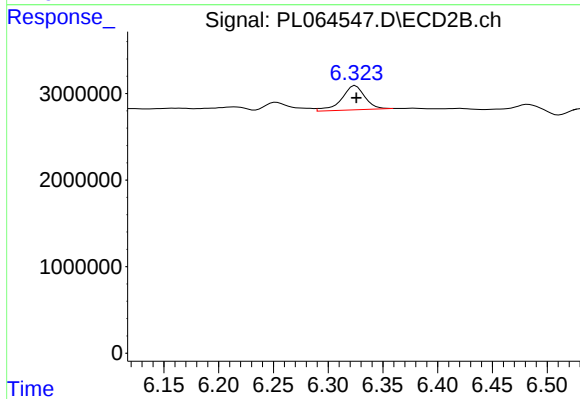

#11 alpha-Chlordane


R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 4132560
Conc: 1.40 ng/ml

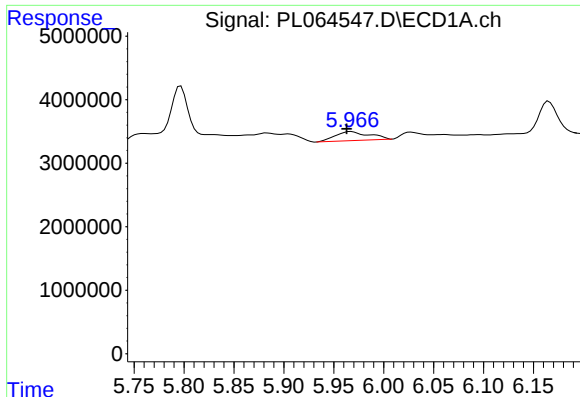

#14 Endrin


R.T.: 5.967 min
Delta R.T.: 0.004 min
Response: 3349553
Conc: 0.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

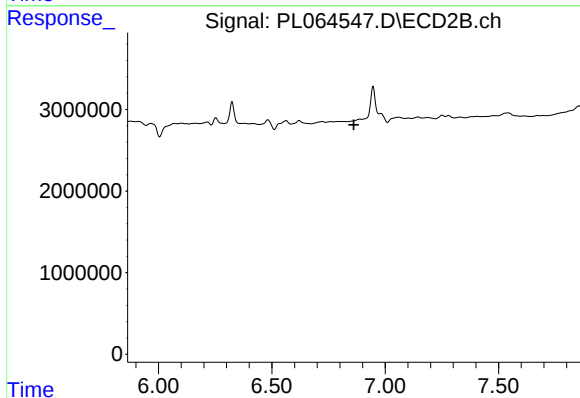


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

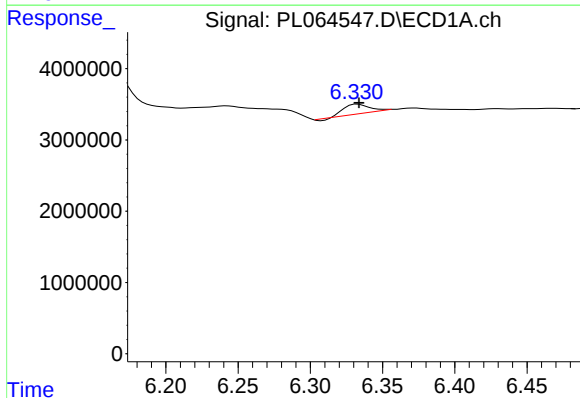


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: -0.001 min
Response: 1522652
Conc: 0.50 ng/ml

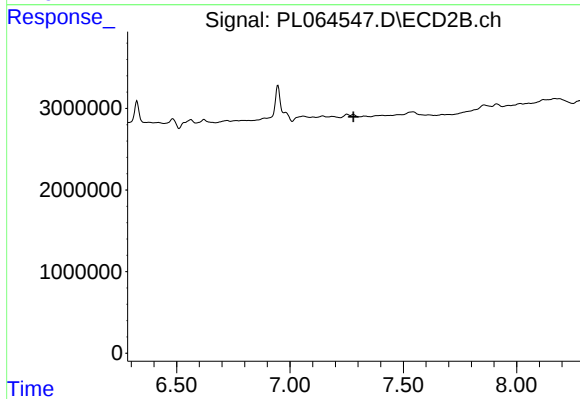

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.280 min
Response: 0
Conc: N.D.

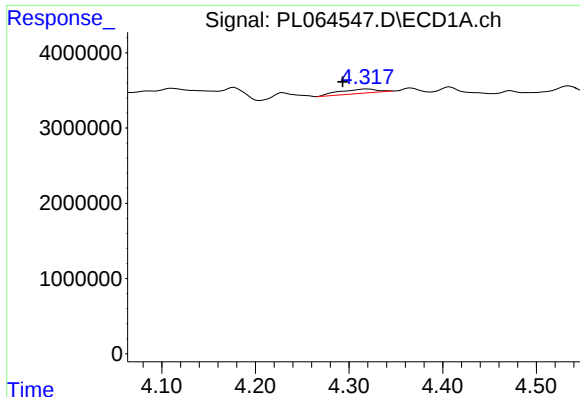

#23 Chlordane-1


R.T.: 4.319 min
Delta R.T.: 0.026 min
Response: 1554963
Conc: 14.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

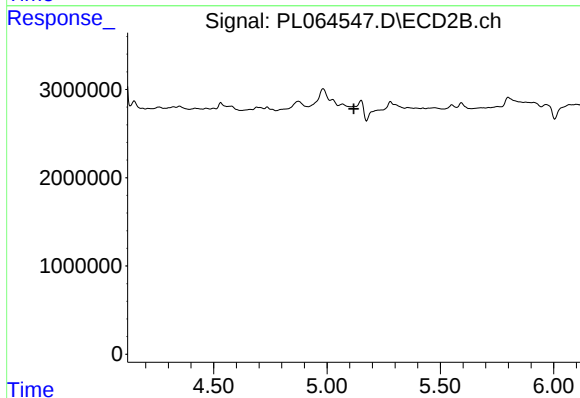


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

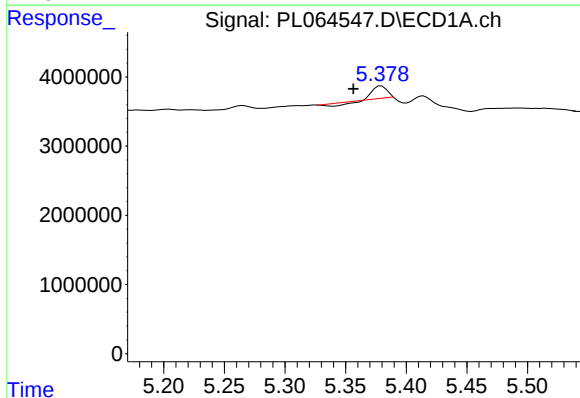


#25 Chlordane-3

R.T.: 5.380 min
Delta R.T.: 0.023 min
Response: 1112478
Conc: 3.08 ng/ml

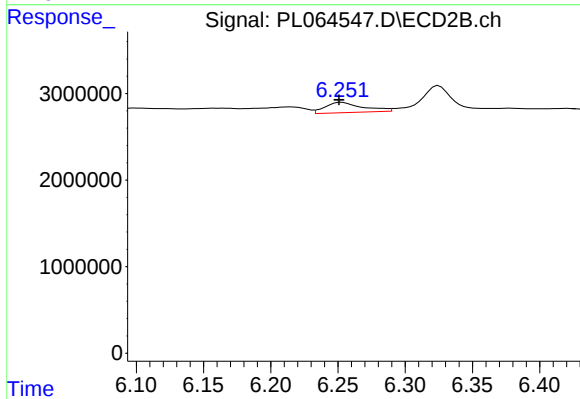

#25 Chlordane-3


R.T.: 6.253 min
Delta R.T.: 0.002 min
Response: 2320484
Conc: 6.47 ng/ml

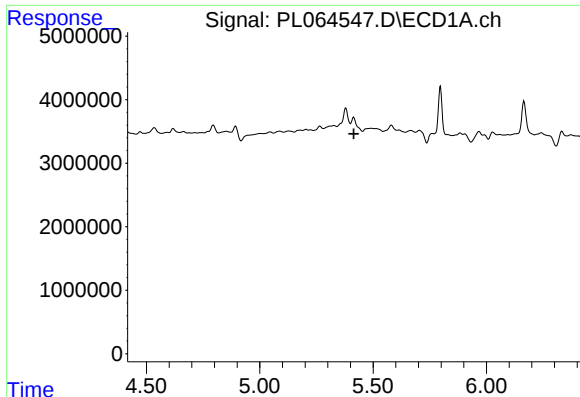

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

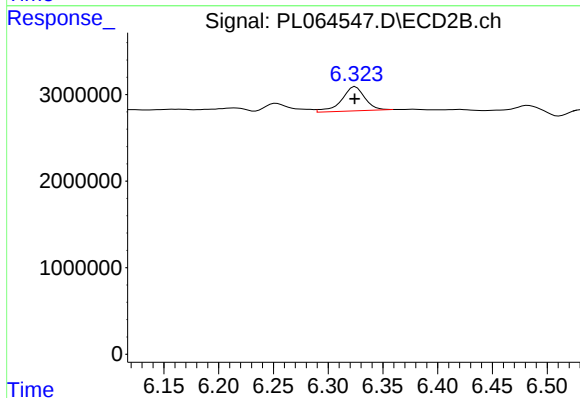


#26 Chlordane-4

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 4132560
Conc: 9.40 ng/ml

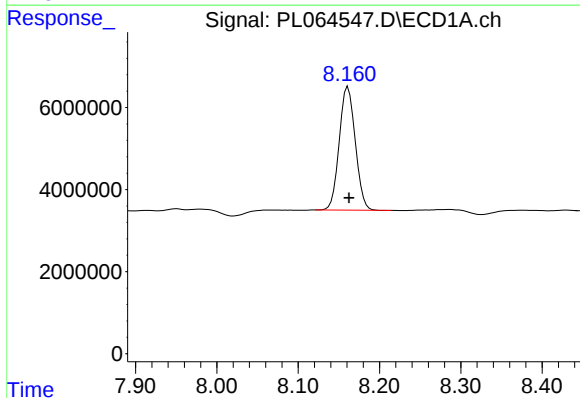

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: -0.001 min
Response: 41114252
Conc: 13.05 ng/ml

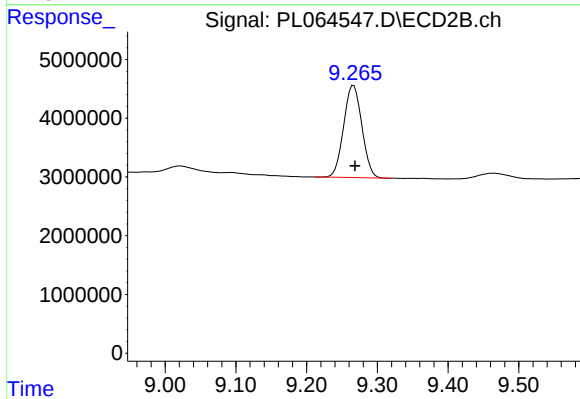

#28 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.002 min
Response: 28147827
Conc: 13.75 ng/ml