

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
 Data File : PD061087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 13:23
 Operator : DD\AJ
 Sample : M1254-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CRT-5

Manual Integrations
 APPROVED

Sohil
 2/1/2021 3:10:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:16:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 01:48:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.020	19224039	128.8E6	21.770	19.053
28)	SA Decachlor...	8.276	9.103	14932022	110.5E6	17.339	18.115m
Target Compounds							
16)	A 4,4'-DDD	6.191	6.850	8452128	124.2E6	8.677m	18.723m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012921\
Data File : PD061087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 13:23
Operator : DD\AJ
Sample : M1254-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CRT-5


Manual Integrations
APPROVED

Sohil
2/1/2021 3:10:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:16:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012821.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 01:48:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

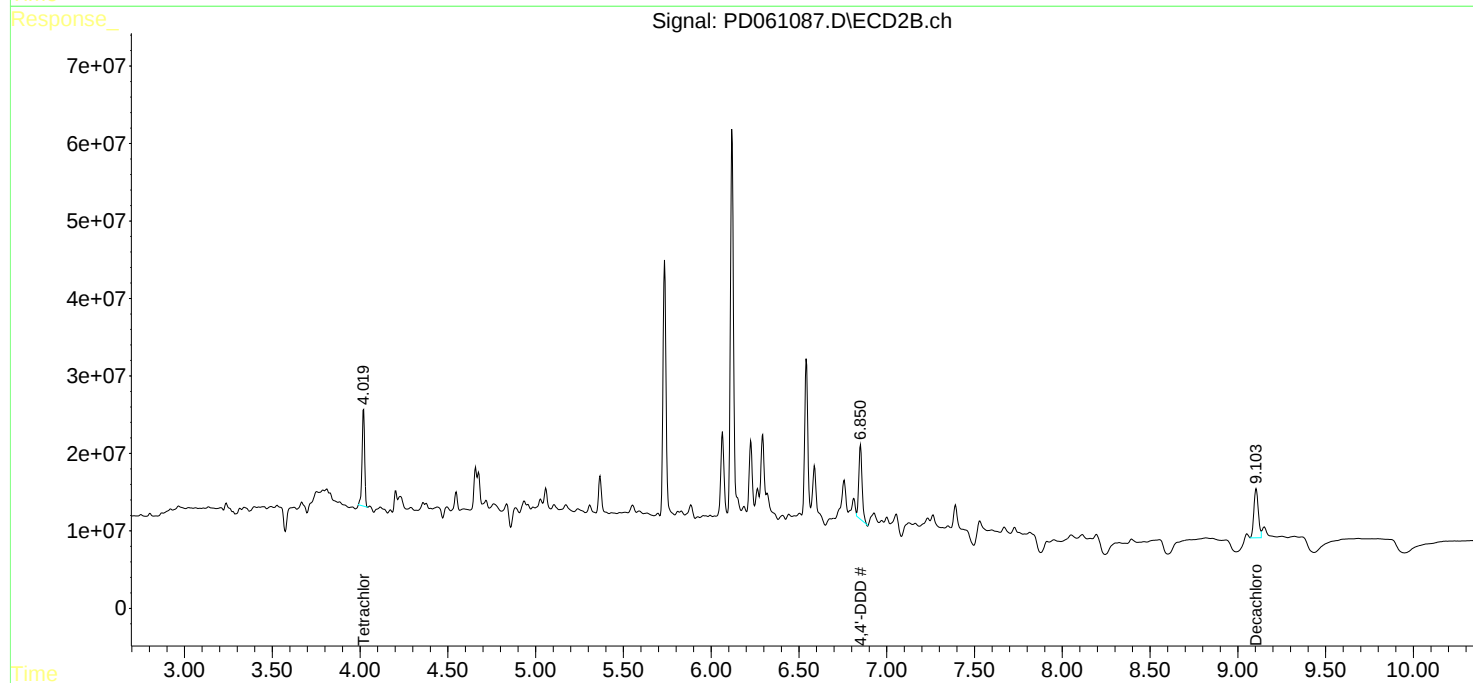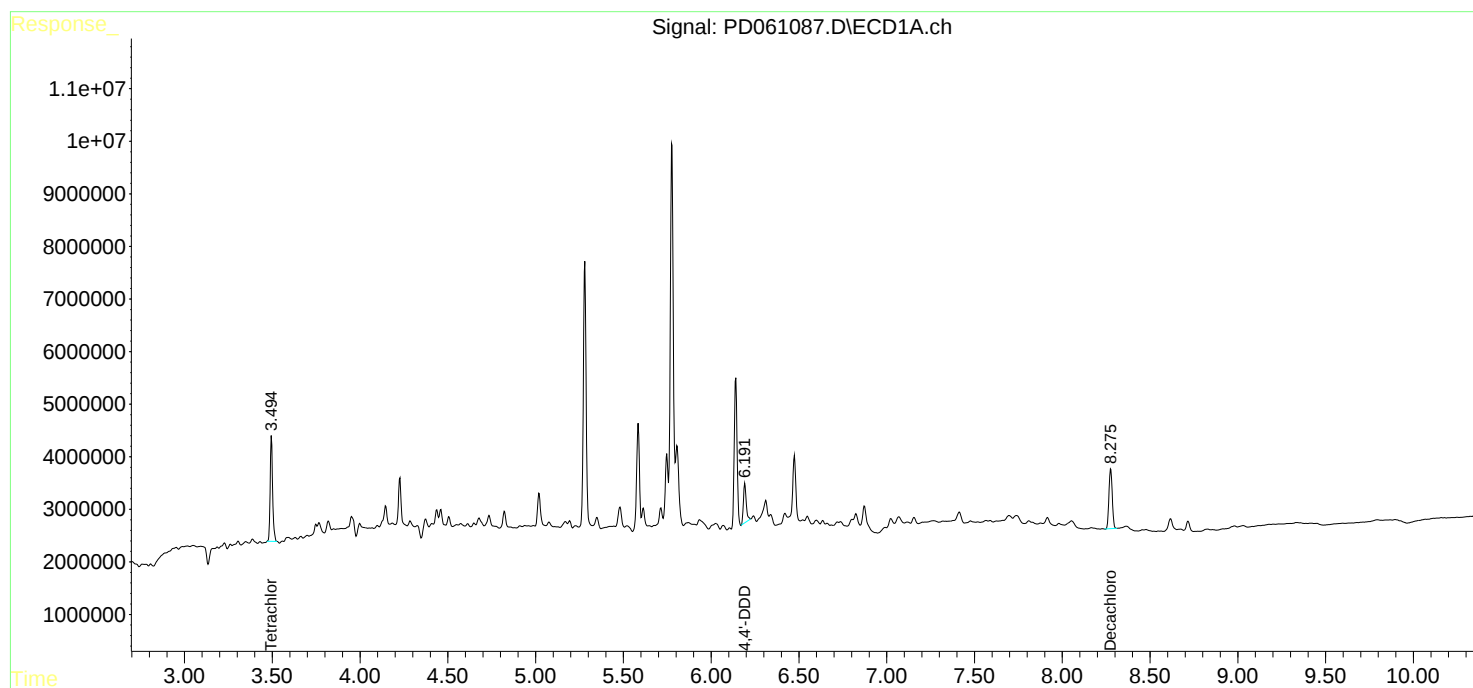

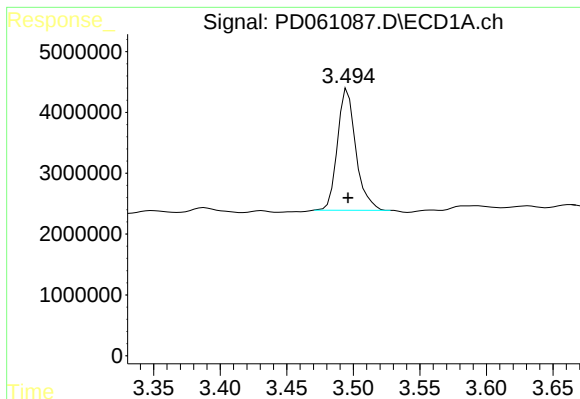


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 19224039
Conc: 21.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
CRT-5


Manual Integrations
APPROVED

Sohil
2/1/2021 3:10:42 PM

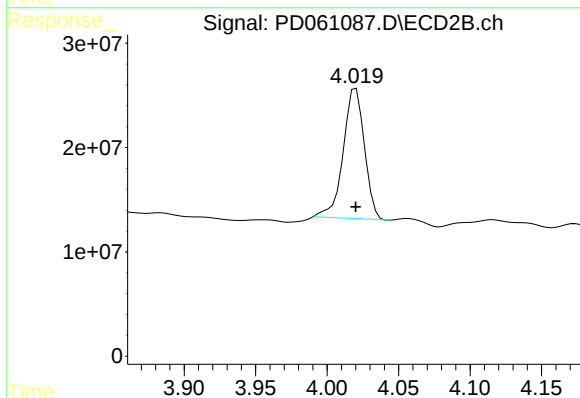


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 128768661
Conc: 19.05 ng/ml

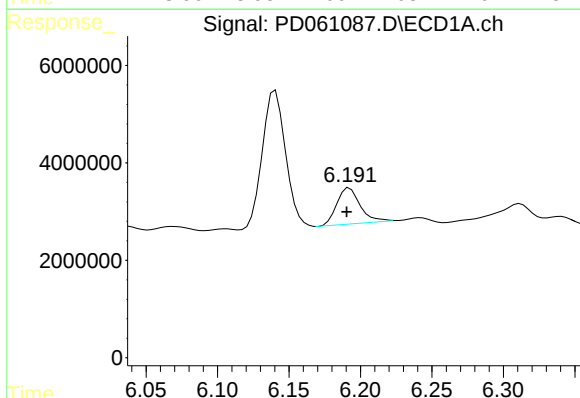


#16 4,4'-DDD

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 8452128
Conc: 8.68 ng/ml m

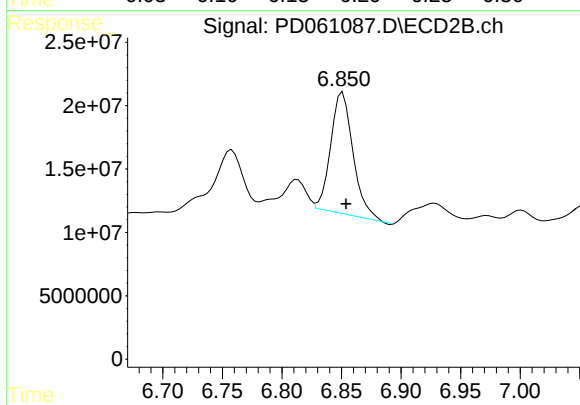

#16 4,4'-DDD

R.T.: 6.850 min
Delta R.T.: -0.004 min
Response: 124227062
Conc: 18.72 ng/ml m

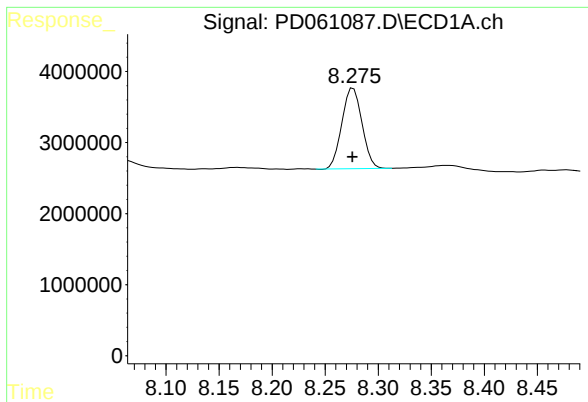


#28 Decachlorobiphenyl

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 14932022
Conc: 17.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
CRT-5

Manual Integrations
APPROVED

Sohil
2/1/2021 3:10:42 PM

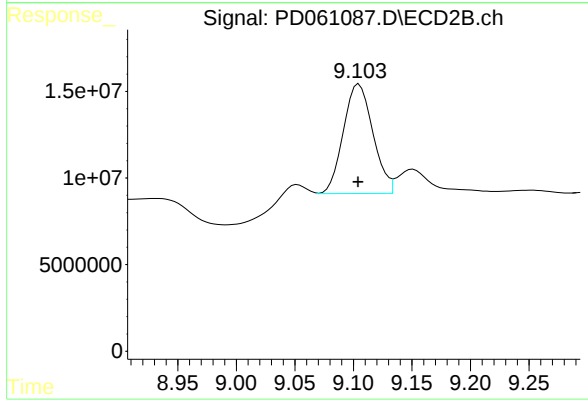

#28 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.000 min
Response: 110471954
Conc: 18.12 ng/ml m