

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
 Data File : PD080952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 15:20
 Operator : AR\AJ
 Sample : PB158678BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK678

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 09:24:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.574	2.793	31238604	56491677	21.952	22.124
27)	SA Decachlor...	9.127	7.936	50593514	71476448	25.760	26.731
Target Compounds							
2)	A alpha-BHC	0.000	3.262f	0	7662	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.642	0	377270	N.D.	<MDL
4)	MA Heptachlor	0.000	3.959	0	86554	N.D.	<MDL
5)	MB Aldrin	0.000	4.226	0	82930	N.D.	<MDL
6)	B beta-BHC	0.000	3.924	0	113779	N.D.	<MDL
15)	B Endosulfa...	0.000	5.913f	0	183075	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
Data File : PD080952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 15:20
Operator : AR\AJ
Sample : PB158678BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 09:24:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

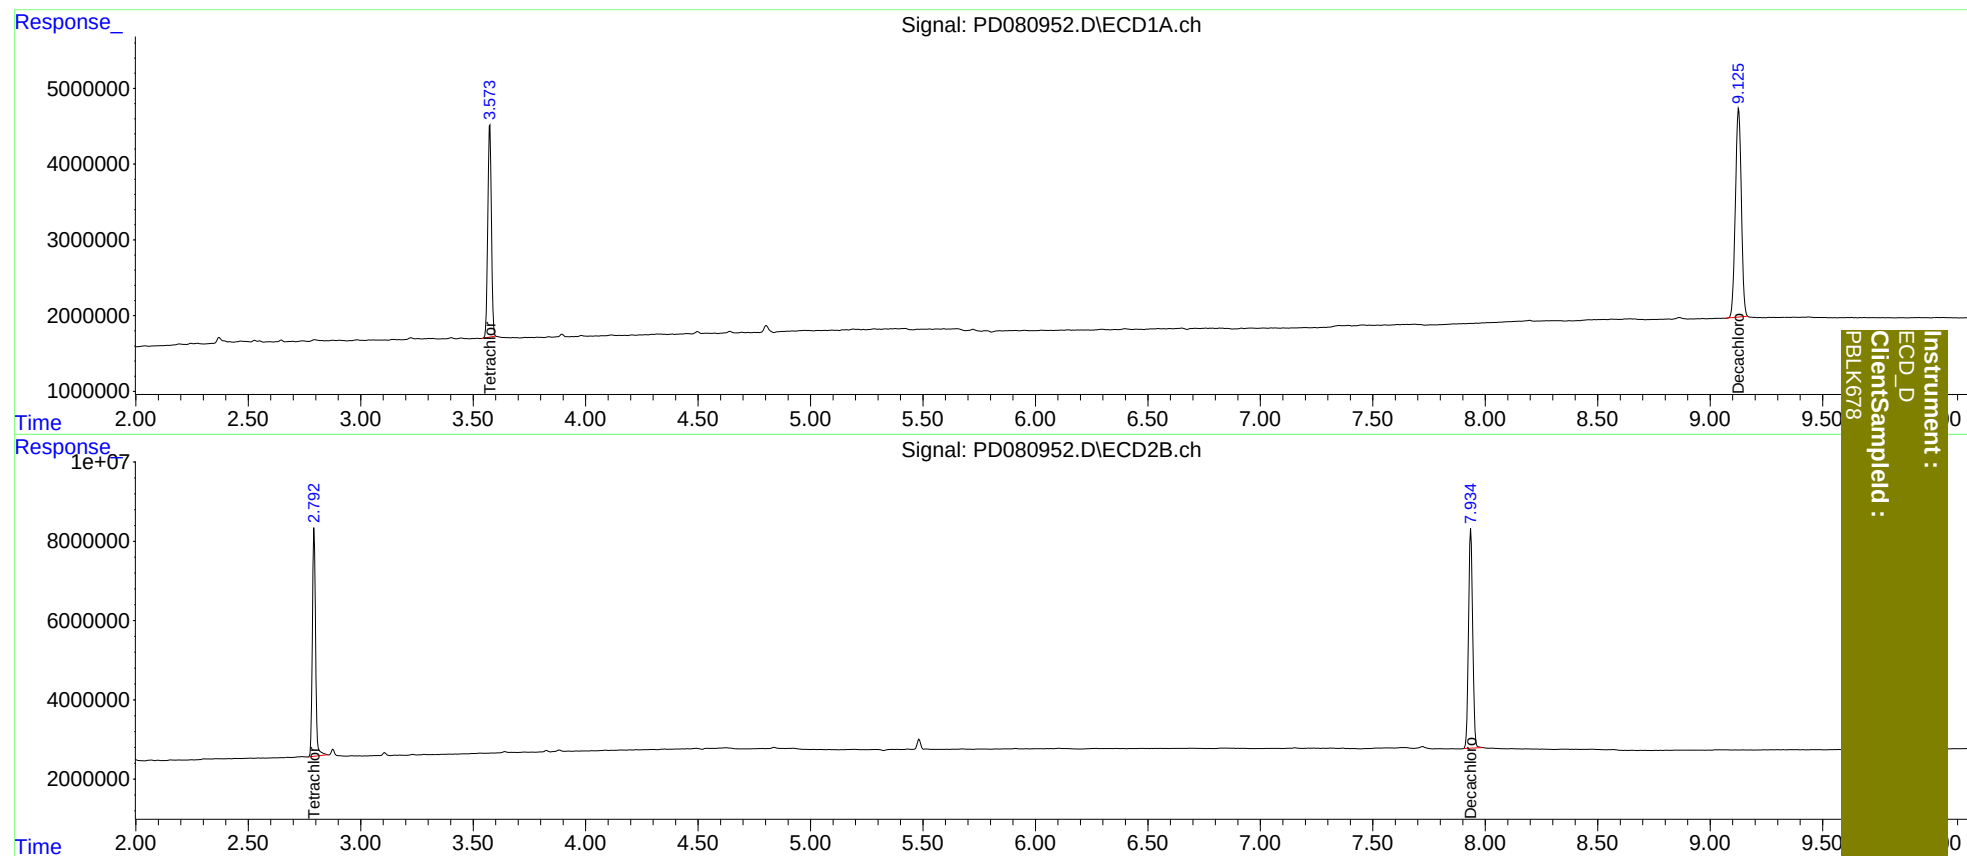


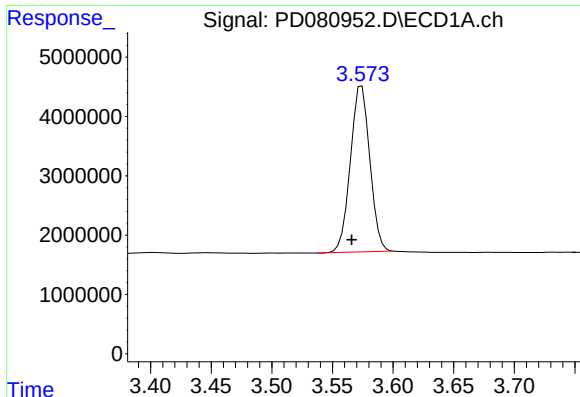

#1 Tetrachloro-m-xylene


R.T.: 3.574 min
Delta R.T.: 0.008 min
Response: 31238604
Conc: 21.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK678

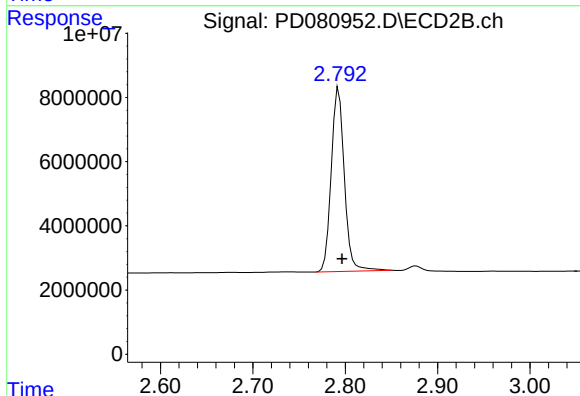


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: -0.003 min
Response: 56491677
Conc: 22.12 ng/ml

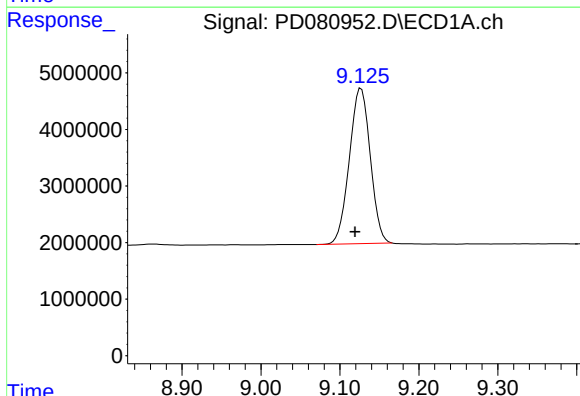

#27 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.008 min
Response: 50593514
Conc: 25.76 ng/ml

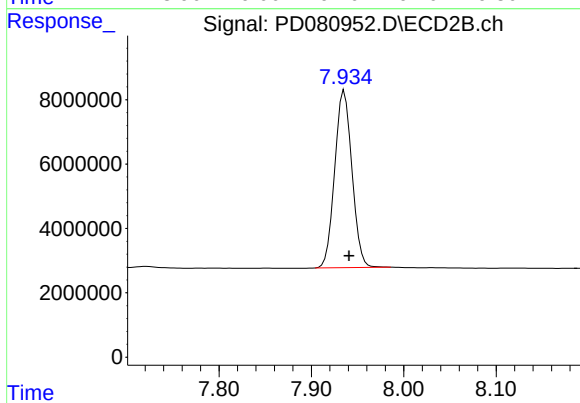

#27 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: -0.005 min
Response: 71476448
Conc: 26.73 ng/ml