

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
 Data File : PD080955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 16:21
 Operator : AR\AJ
 Sample : P1238-04MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH703MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2024
 Supervised By : Ankita Jodhani 01/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 09:44:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.796	29051097	50876528	20.415	19.925
27)	SA Decachlor...	9.116	7.935	45954527	61843519	23.398	23.128
Target Compounds							
2)	A alpha-BHC	4.024	3.298	132.5E6	220.8E6	56.260	53.961
3)	MA gamma-BHC...	4.357	3.627	126.3E6	199.4E6	55.170	52.248
4)	MA Heptachlor	4.951	3.968	127.5E6	191.7E6	52.719	51.908
5)	MB Aldrin	5.294	4.248	121.5E6	187.8E6	53.681	51.324
6)	B beta-BHC	4.552	3.922	52498107	82770075	50.910	46.917
7)	B delta-BHC	4.801	4.153	130.7E6	207.8E6	54.782	52.799
8)	B Heptachlo...	5.720	4.750	117.2E6	180.4E6	53.797	52.534
9)	A Endosulfan I	6.108	5.120	111.2E6	169.0E6	52.399	52.537
10)	B trans-Chl...	5.977	4.999	113.6E6	178.3E6	55.083	53.551
11)	B cis-Chlor...	6.056	5.064	116.4E6	180.2E6	54.844	52.470
12)	B 4,4'-DDE	6.228	5.252	220.8E6	343.9E6	112.323	109.191
13)	MA Dieldrin	6.383	5.384	243.3E6	382.4E6	109.011	108.065
14)	MA Endrin	6.613	5.659	204.4E6	336.7E6	112.243	113.443
15)	B Endosulfa...	6.832	5.952	207.3E6	325.9E6	105.959	109.800
16)	A 4,4'-DDD	6.745	5.806	179.6E6	289.7E6	107.542	106.956
17)	MA 4,4'-DDT	7.060	6.057	201.0E6	302.1E6	118.550	112.199
18)	B Endrin al...	6.962	6.132	156.3E6	237.3E6	108.527	105.964
19)	B Endosulfa...	7.197	6.354	199.9E6	306.2E6	111.595	109.425
20)	A Methoxychlor	7.535	6.632	485.4E6	704.0E6	525.508	497.324
21)	B Endrin ke...	7.681	6.860	225.7E6	354.6E6	114.902m	112.717

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
Data File : PD080955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 16:21
Operator : AR\AJ
Sample : P1238-04MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 09:44:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

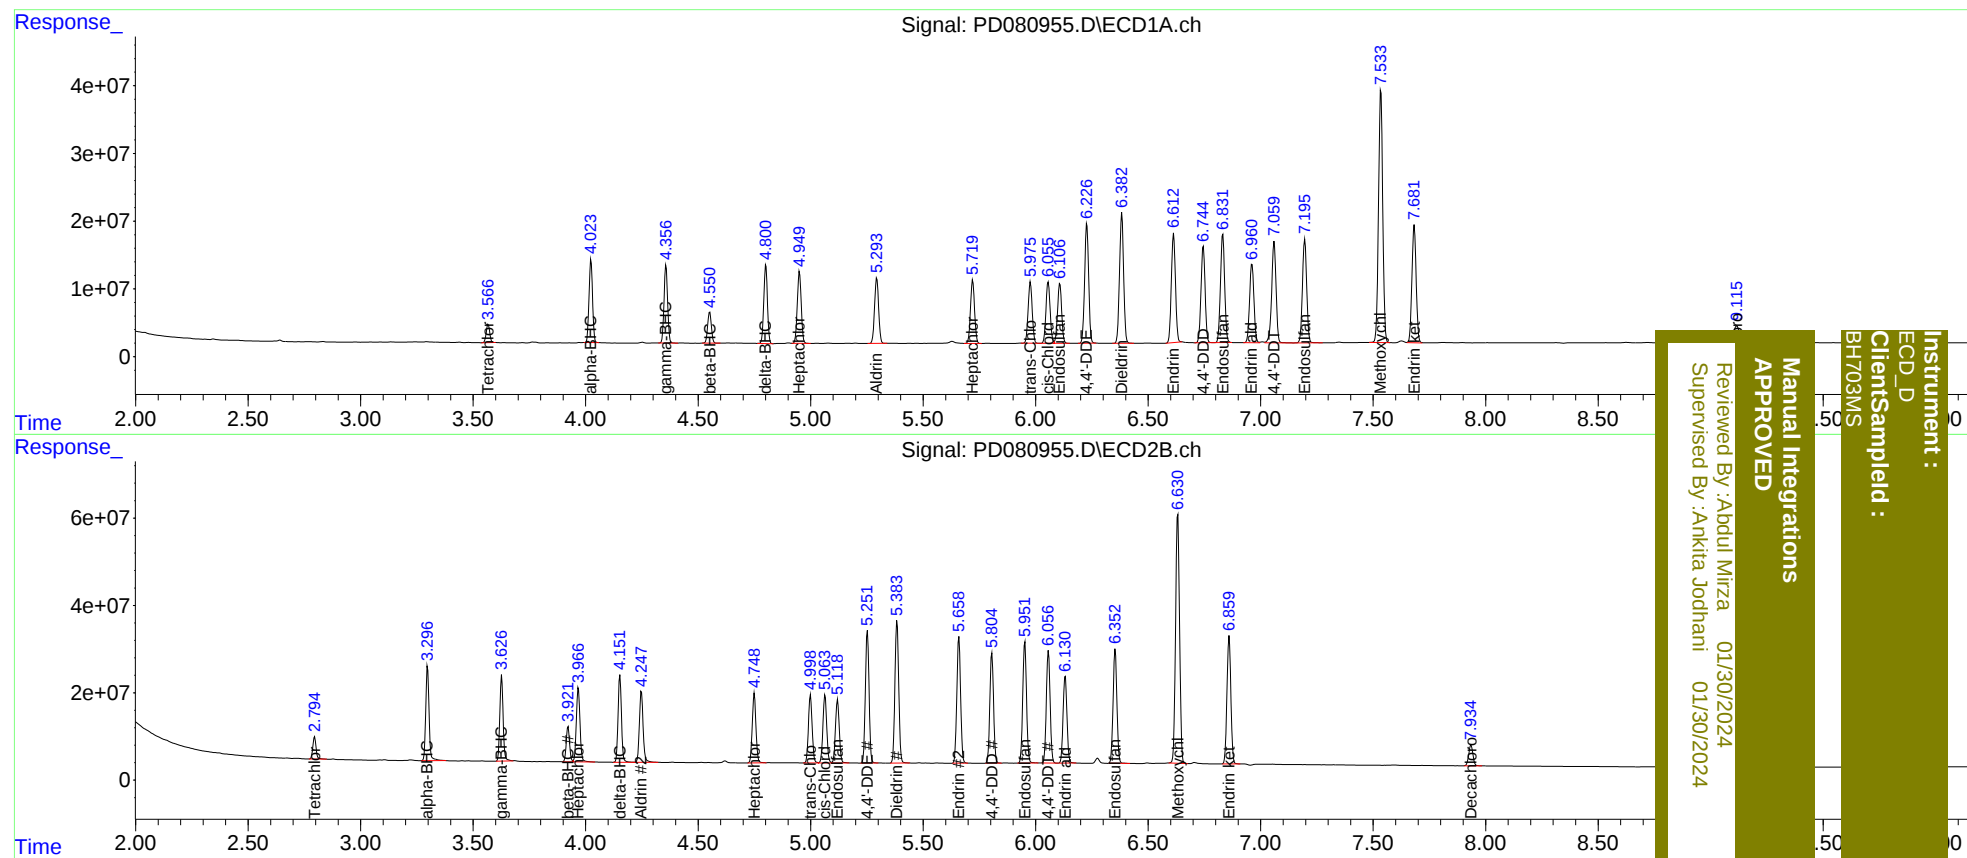

Instrument :
ECD_D
ClientSampled :
BH703MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/30/2024
Supervised By: Ankita Jodhani 01/30/2024