

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
 Data File : PD080956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2024 16:34
 Operator : AR\AJ
 Sample : P1238-05MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH703MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/30/2024
 Supervised By :Ankita Jodhani 01/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 09:46:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.796	29841793	50101559	20.971	19.621
27)	SA Decachlor...	9.115	7.935	45427090	60884527	23.129	22.769
Target Compounds							
2)	A alpha-BHC	4.024	3.298	137.9E6	217.0E6	58.566	53.032
3)	MA gamma-BHC...	4.357	3.628	129.7E6	196.4E6	56.646	51.459
4)	MA Heptachlor	4.950	3.968	130.7E6	189.9E6	54.038	51.413
5)	MB Aldrin	5.294	4.249	123.6E6	185.0E6	54.621	50.558
6)	B beta-BHC	4.552	3.923	53337528	81695956	51.724	46.308
7)	B delta-BHC	4.801	4.153	134.1E6	204.6E6	56.230	51.990
8)	B Heptachlo...	5.720	4.750	117.9E6	177.9E6	54.115	51.809
9)	A Endosulfan I	6.107	5.120	111.9E6	166.8E6	52.706	51.863
10)	B trans-Chl...	5.976	5.000	114.6E6	175.7E6	55.560	52.755
11)	B cis-Chlor...	6.056	5.064	117.3E6	177.6E6	55.263	51.711
12)	B 4,4'-DDE	6.227	5.253	222.7E6	338.7E6	113.305	107.542
13)	MA Dieldrin	6.383	5.384	245.1E6	376.7E6	109.819	106.456
14)	MA Endrin	6.613	5.660	204.8E6	331.8E6	112.473	111.793
15)	B Endosulfa...	6.831	5.953	204.4E6	320.5E6	104.467	107.996
16)	A 4,4'-DDD	6.745	5.807	179.5E6	284.6E6	107.523	105.071
17)	MA 4,4'-DDT	7.060	6.057	196.2E6	297.3E6	115.681	110.430
18)	B Endrin al...	6.961	6.132	151.8E6	233.2E6	105.376	104.121
19)	B Endosulfa...	7.195	6.355	199.3E6	302.3E6	111.258	108.036
20)	A Methoxychlor	7.534	6.632	472.4E6	695.0E6	511.429	490.937
21)	B Endrin ke...	7.681	6.861	212.0E6	348.0E6	107.905m	110.612

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012924\
Data File : PD080956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2024 16:34
Operator : AR\AJ
Sample : P1238-05MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 09:46:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

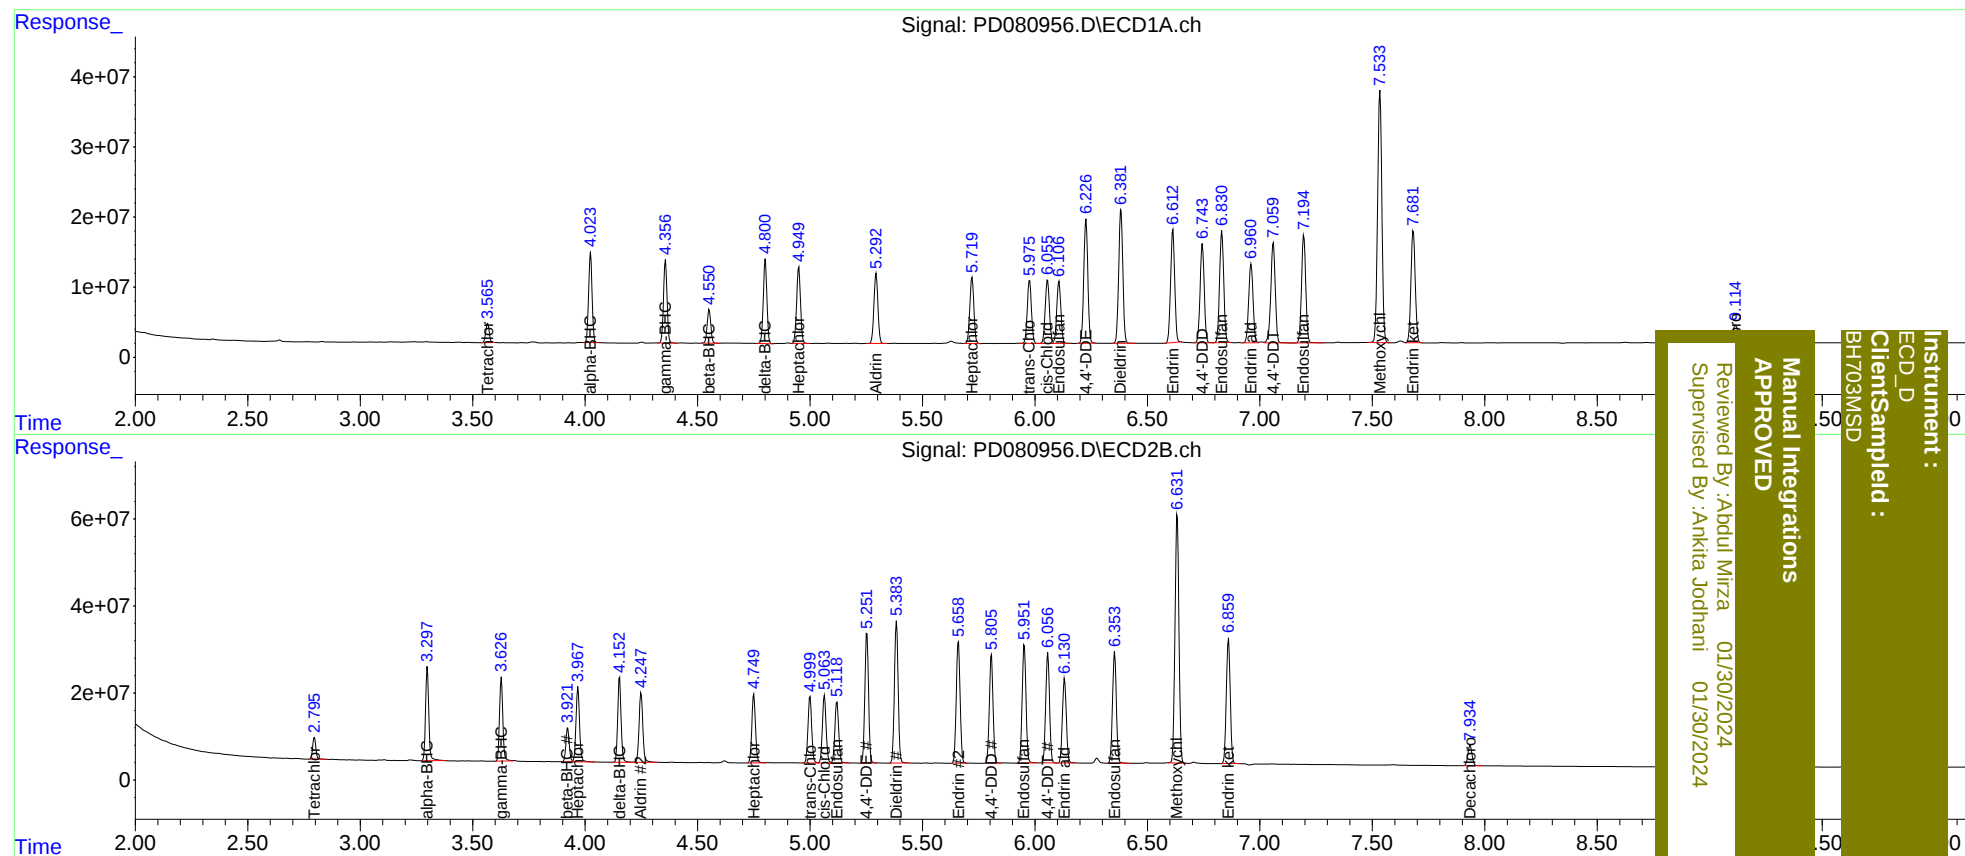

Instrument :
ECD_D
Client Sampled :
BH703MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/30/2024
Supervised By: Ankita Jodhani 01/30/2024