

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 14:02
 Operator : AR\AJ
 Sample : Q1184-10MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2959MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 07:38:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.881	39407692	375.3E6	19.337	30.349 #
27)	SA Decachlor...	9.091	8.086	66514866	327.7E6	19.895	22.627
Target Compounds							
2)	A alpha-BHC	4.007	3.397	225.2E6	1059.8E6	54.205	53.519
3)	MA gamma-BHC...	4.336	3.734	222.9E6	985.5E6	55.401m	53.804
4)	MA Heptachlor	4.938	4.090	193.2E6	890.8E6	47.255	47.730
5)	MB Aldrin	5.281	4.376	182.8E6	842.9E6	45.644	46.637
6)	B beta-BHC	4.522	4.031	81416815	413.0E6	45.331	48.413
7)	B delta-BHC	4.771	4.268	219.8E6	983.5E6	53.188	52.696
8)	B Heptachlo...	5.701	4.880	184.9E6	856.5E6	49.483	50.606
9)	A Endosulfan I	6.083	5.256	169.2E6	802.7E6	48.568m	50.575
10)	B trans-Chl...	5.956	5.134	175.3E6	894.5E6	47.582	49.753
11)	B cis-Chlor...	6.036	5.199	185.4E6	878.2E6	49.866m	50.740
12)	B 4,4'-DDE	6.204	5.385	342.2E6	1649.8E6	97.164m	100.727
13)	MA Dieldrin	6.358	5.522	384.6E6	1681.8E6	100.876	100.764
14)	MA Endrin	6.585	5.798	317.1E6	1521.6E6	97.694	101.831
15)	B Endosulfa...	6.797	6.090	300.4E6	1465.3E6	93.305	98.907
16)	A 4,4'-DDD	6.716	5.939	267.9E6	1368.4E6	97.433	102.354
17)	MA 4,4'-DDT	7.032	6.194	292.1E6	1413.2E6	100.776	102.550
18)	B Endrin al...	6.926	6.268	225.1E6	1093.7E6	89.342	94.867
19)	B Endosulfa...	7.158	6.492	290.4E6	1433.9E6	94.059m	98.637
20)	A Methoxychlor	7.505	6.766	708.1E6	2844.9E6	446.907	461.886
21)	B Endrin ke...	7.642	7.002	315.7E6	1531.2E6	91.702	96.409

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 14:02
Operator : AR\AJ
Sample : Q1184-10MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 07:38:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

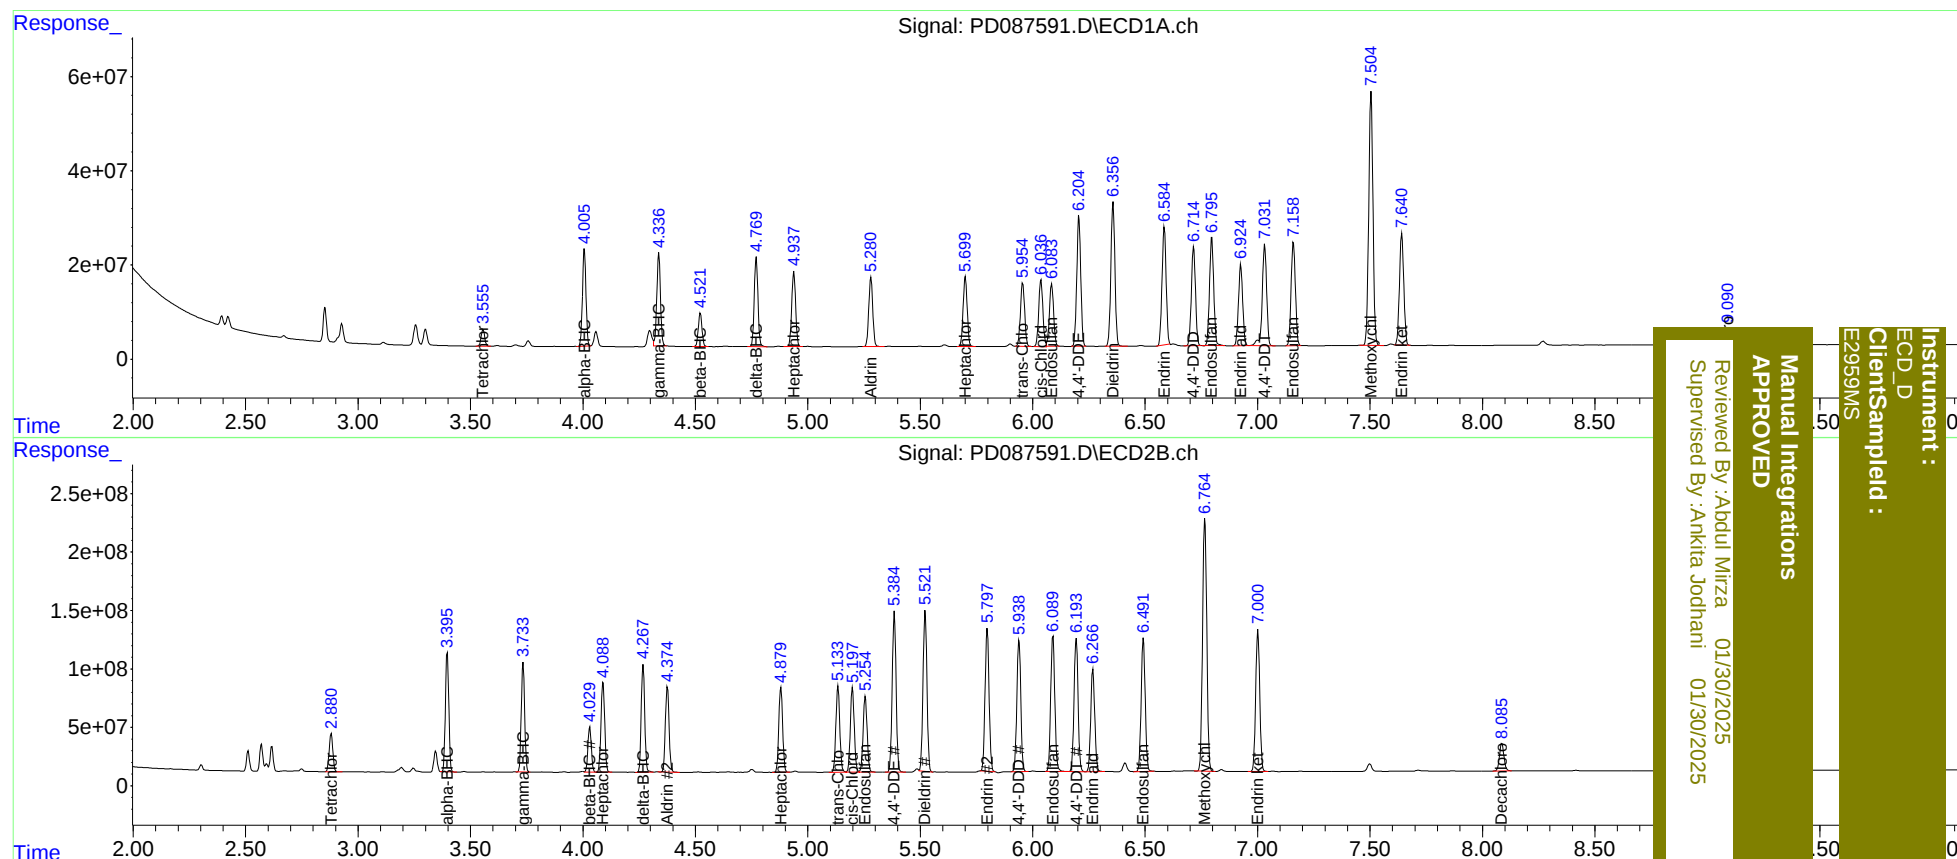

Instrument :
ECD_D
ClientSampled :
EZ959MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 01/30/2025
Supervised By: Ankita Jodhani 01/30/2025