

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
 Data File : PD087603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 16:51
 Operator : AR\AJ
 Sample : Q1174-15MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E2944MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/30/2025
 Supervised By : Ankita Jodhani 01/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 07:42:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.556	2.882	38588064	267.5E6	18.934	21.626
27) SA Decachlor...	9.090	8.086	62186242	290.1E6	18.600	20.029
Target Compounds						
2) A alpha-BHC	4.006	3.397	214.3E6	1011.8E6	51.595	51.095
3) MA gamma-BHC...	4.338	3.734	205.2E6	924.5E6	51.003	50.475
4) MA Heptachlor	4.938	4.089	190.7E6	865.4E6	46.650	46.368
5) MB Aldrin	5.280	4.375	186.2E6	863.7E6	46.492	47.789
6) B beta-BHC	4.522	4.030	76768502	386.1E6	42.743	45.259
7) B delta-BHC	4.771	4.267	203.8E6	918.2E6	49.315	49.197
8) B Heptachlo...	5.700	4.880	170.2E6	793.5E6	45.561	46.884
9) A Endosulfan I	6.083	5.255	157.5E6	742.2E6	45.202m	46.761
10) B trans-Chl...	5.955	5.134	163.0E6	829.2E6	44.248	46.123
11) B cis-Chlor...	6.035	5.198	167.5E6	811.7E6	45.059m	46.896
12) B 4,4'-DDE	6.204	5.384	318.5E6	1514.1E6	90.426m	92.440
13) MA Dieldrin	6.355	5.521	353.7E6	1559.8E6	92.785m	93.455
14) MA Endrin	6.585	5.798	291.6E6	1412.4E6	89.851	94.525
15) B Endosulfa...	6.796	6.090	282.1E6	1329.5E6	87.636	89.743
16) A 4,4'-DDD	6.715	5.939	250.8E6	1271.6E6	91.234	95.111
17) MA 4,4'-DDT	7.032	6.194	253.6E6	1195.7E6	87.492	86.766
18) B Endrin al...	6.925	6.268	205.0E6	986.4E6	81.366	85.559
19) B Endosulfa...	7.159	6.492	267.0E6	1302.0E6	86.494	89.562
20) A Methoxychlor	7.504	6.766	639.1E6	2599.8E6	403.406	422.085
21) B Endrin ke...	7.641	7.002	289.7E6	1380.6E6	84.147	86.932

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012925\
Data File : PD087603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 16:51
Operator : AR\AJ
Sample : Q1174-15MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 07:42:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

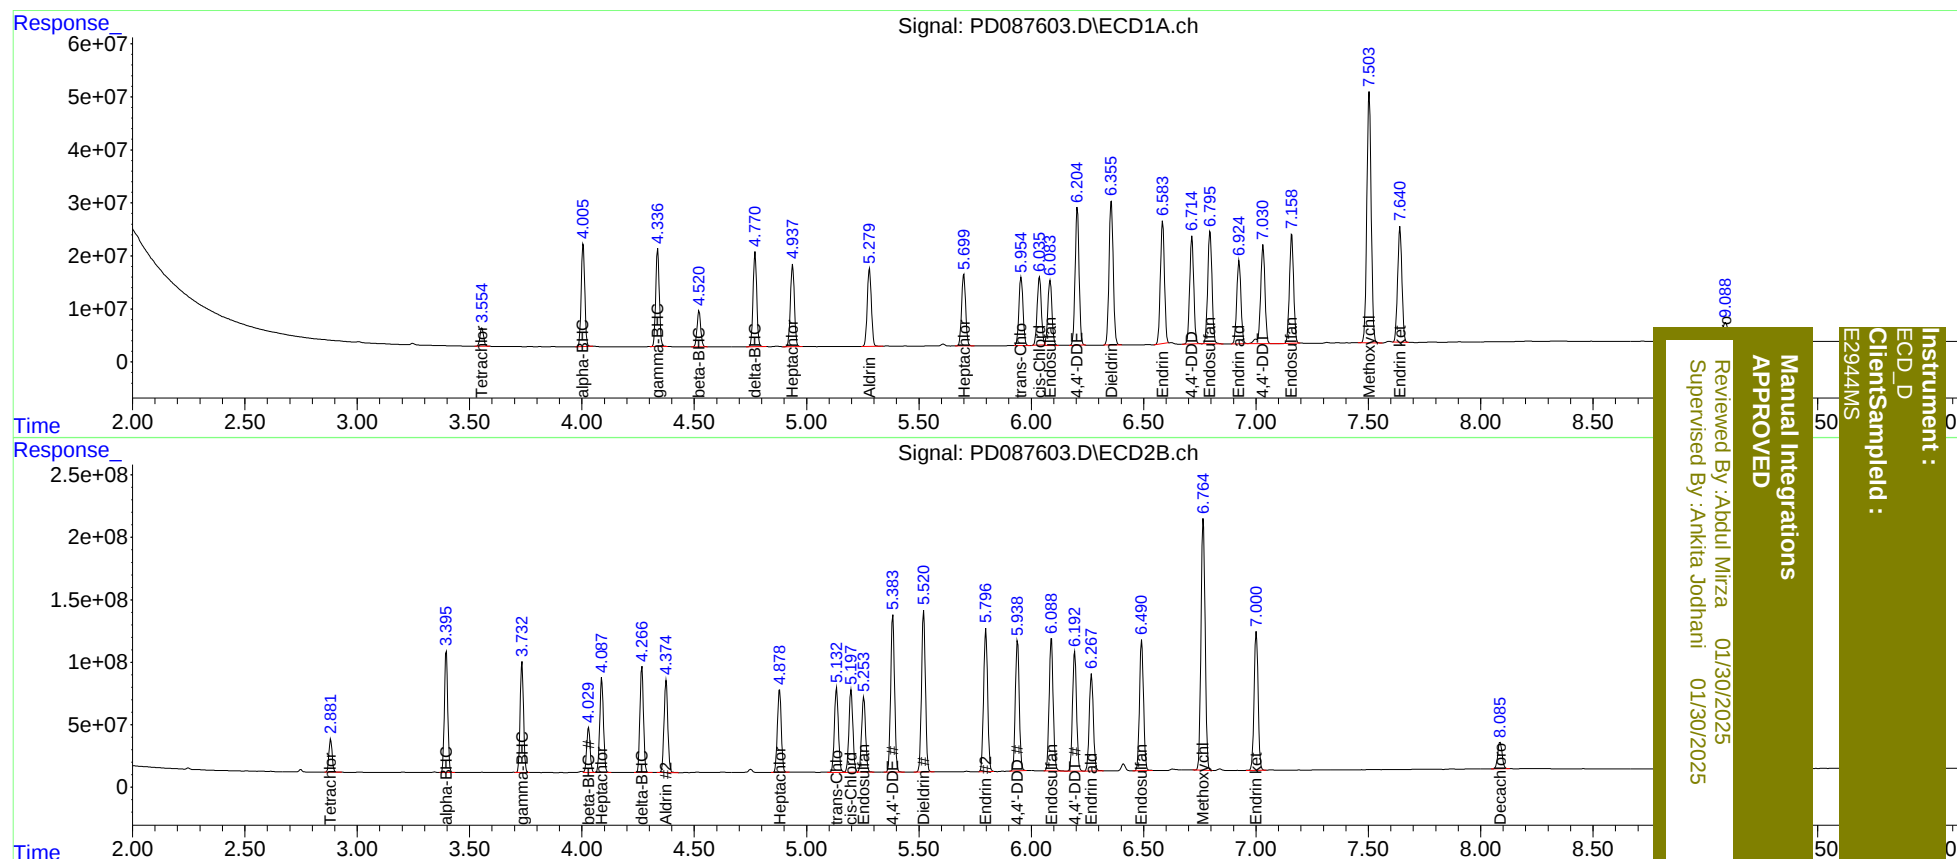

880.60
Reviewed By: Abdul Miza 01/30/2025
Supervised By: Ankita Jodhani 01/30/2025

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EZ944MS